


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP120619\
 Data File : BP001226.D
 Acq On : 06 Dec 2019 12:41
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 05 12:34:47 2019

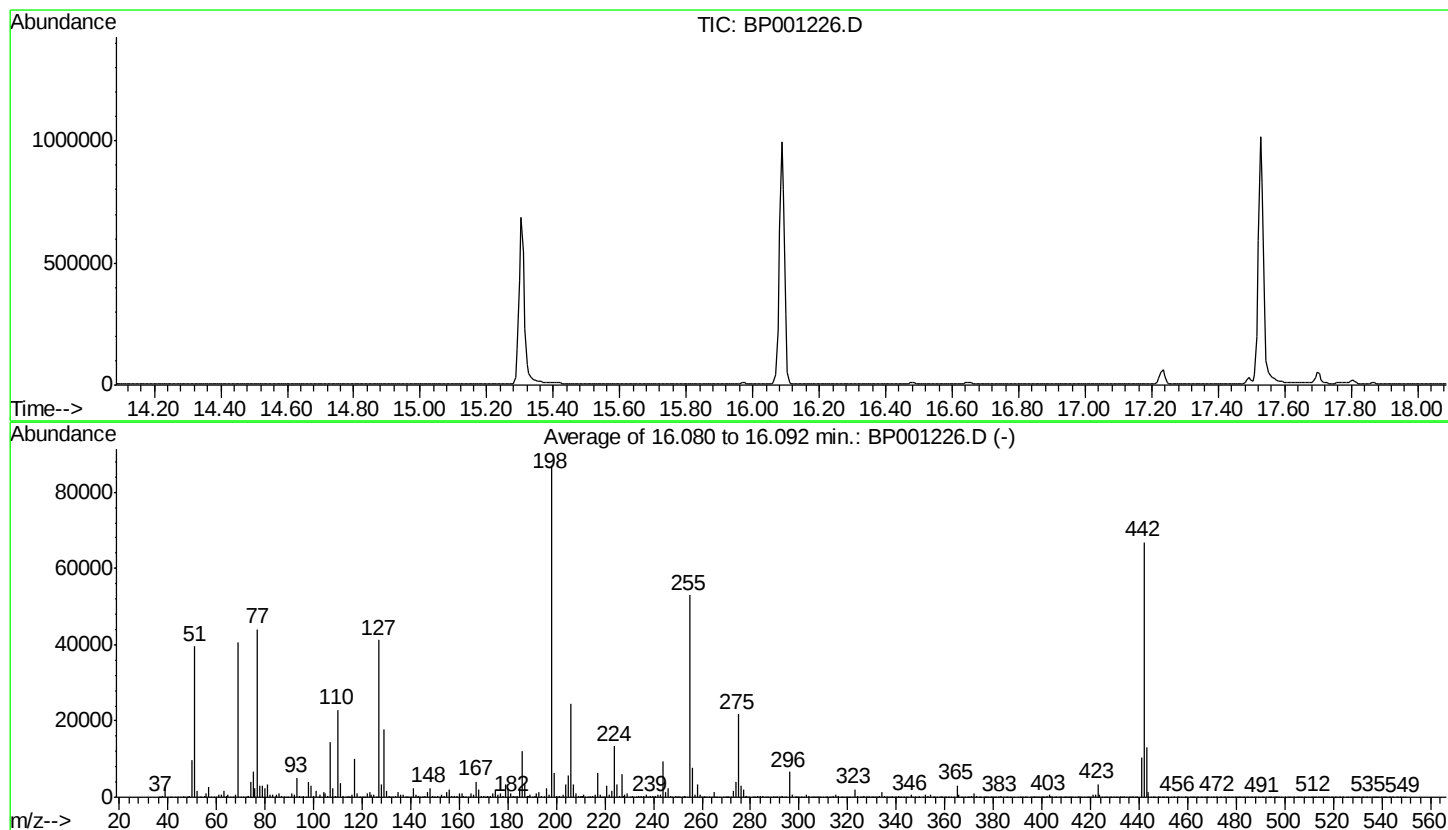

AutoFind: Scans 2379, 2380, 2381; Background Corrected with Scan 2368

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	39524	PASS
68	69	0.00	2	1.6	633	PASS
69	198	0.00	100	46.8	40693	PASS
70	69	0.00	2	0.4	161	PASS
127	198	10	80	47.4	41189	PASS
197	198	0.00	2	0.8	724	PASS
198	198	100	100	100.0	86960	PASS
199	198	5	9	7.2	6286	PASS
275	198	10	60	25.1	21805	PASS
365	198	1	100	3.5	3055	PASS
441	198	0.01	100	12.1	10482	PASS
442	198	50	100	76.9	66906	PASS
443	442	15	24	19.7	13196	PASS