

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
 Data File : BP008240.D
 Acq On : 06 Dec 2021 21:34
 Operator : CG/JU
 Sample : M4915-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B-4-7

Quant Time: Dec 07 05:12:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 03 14:39:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	72239	20.000	ng	-0.01
21) Naphthalene-d8	10.587	136	270331	20.000	ng	-0.01
39) Acenaphthene-d10	14.434	164	181041	20.000	ng	-0.01
64) Phenanthrene-d10	17.198	188	374291	20.000	ng	-0.01
76) Chrysene-d12	21.310	240	408193	20.000	ng	0.00
86) Perylene-d12	23.721	264	445058	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.381	112	291793	65.036	ng	0.00
7) Phenol-d6	6.975	99	375997	62.080	ng	-0.01
23) Nitrobenzene-d5	8.946	82	241550	40.632	ng	-0.02
42) 2,4,6-Tribromophenol	15.940	330	151319	65.393	ng	-0.01
45) 2-Fluorobiphenyl	13.057	172	530137	42.534	ng	-0.01
79) Terphenyl-d14	19.775	244	881444	45.129	ng	0.00
Target Compounds						
					Qvalue	
9) Benzaldehyde	6.940	77	373	Below Cal	#	47
71) Phenanthrene	17.239	178	70822	3.584 ng	#	90
78) Pyrene	19.575	202	55806	Below Cal	#	69
83) Chrysene	21.351	228	80313	3.120 ng	#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
Data File : BP008240.D
Acq On : 06 Dec 2021 21:34
Operator : CG/JU
Sample : M4915-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-4-7

Quant Time: Dec 07 05:12:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 03 14:39:24 2021
Response via : Initial Calibration




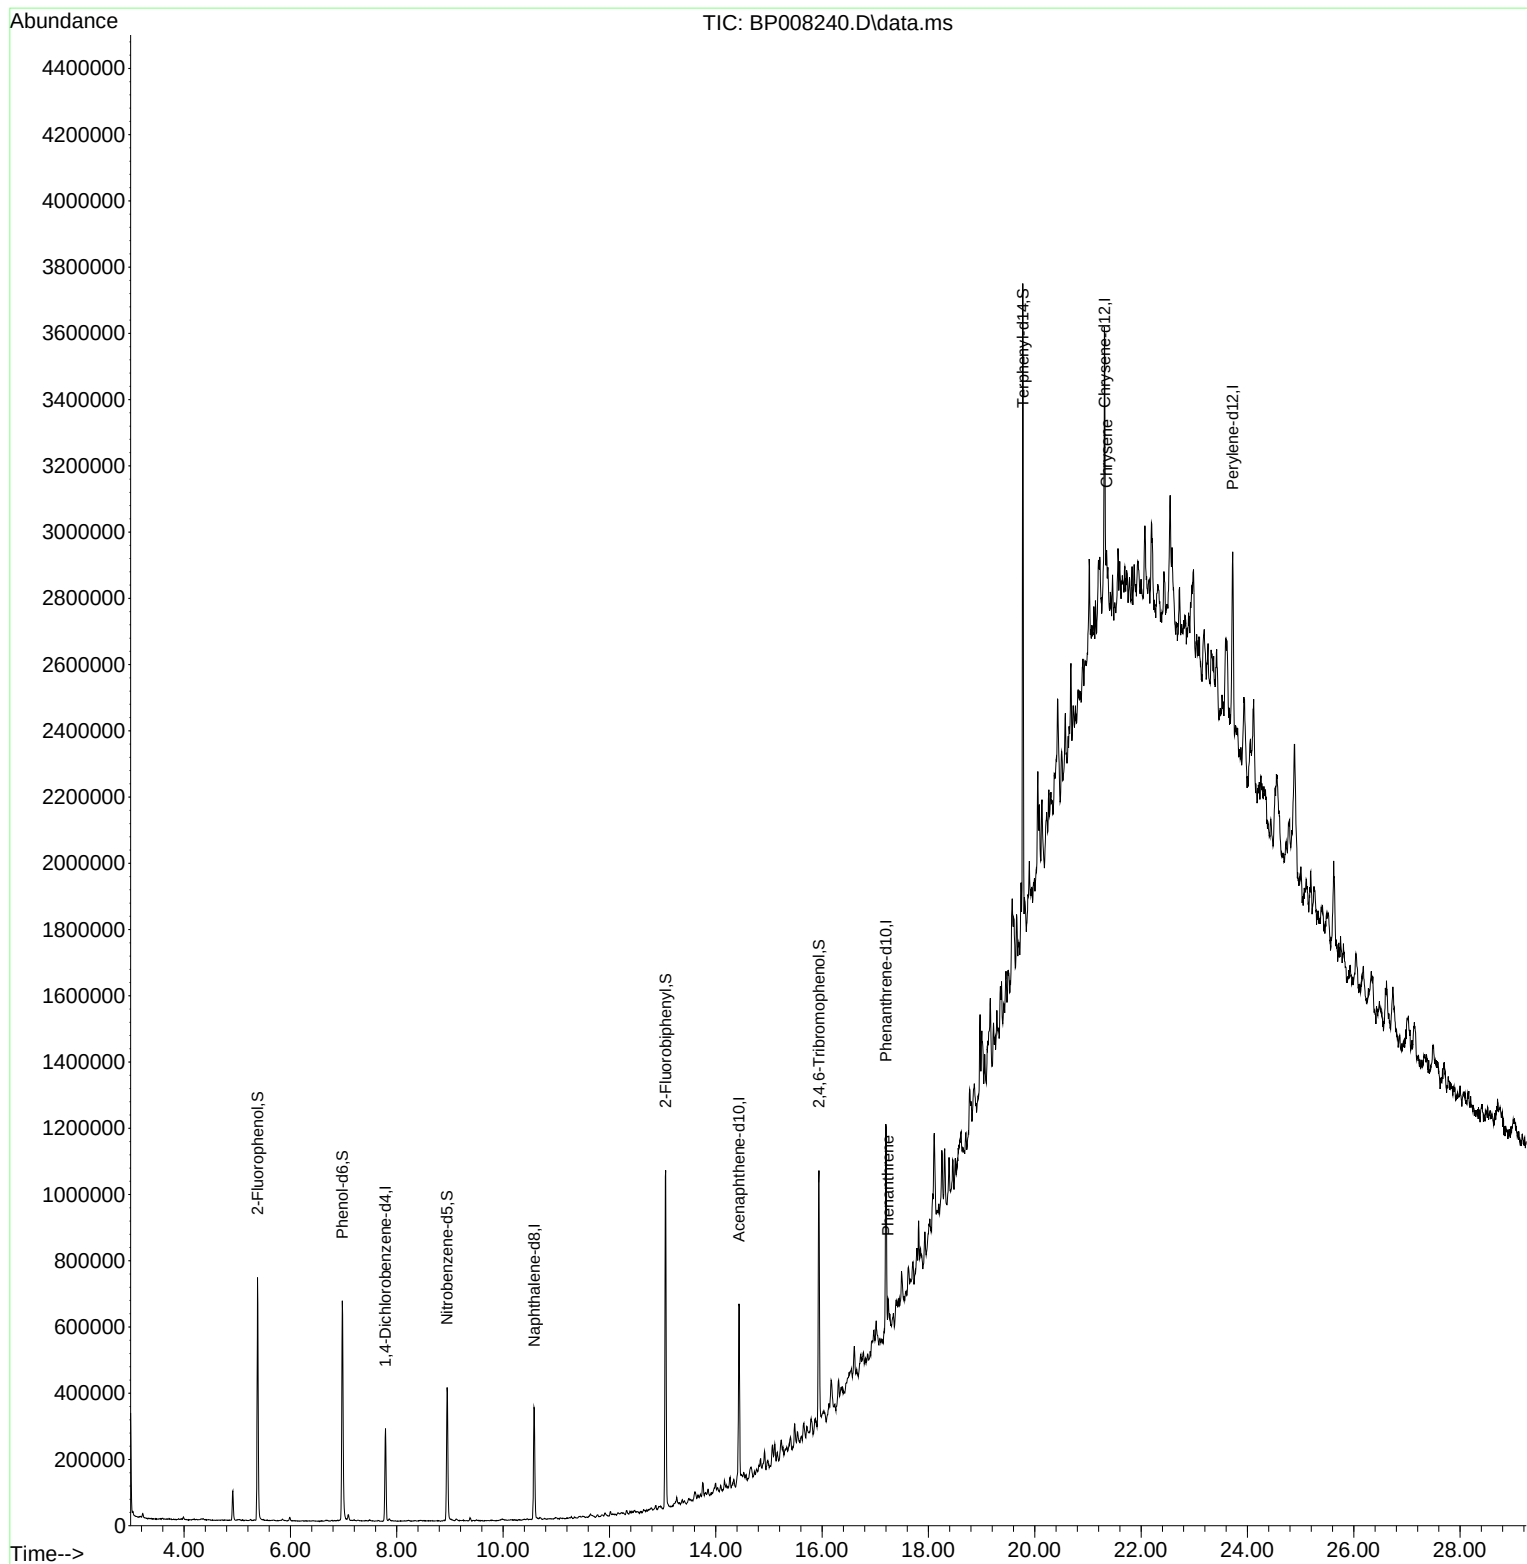


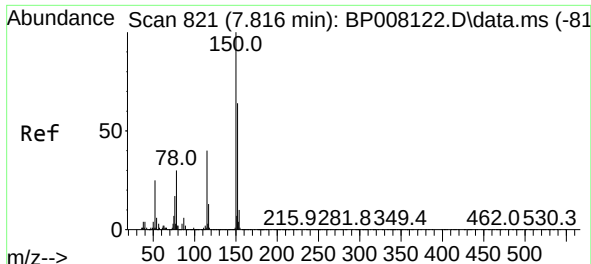

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.787 min Scan# 81
Delta R.T. -0.012 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34




Instrument :
BNA_P
ClientSampleId :
B-4-7


Tgt Ion:152 Resp: 72239
Ion Ratio Lower Upper
152 100
150 148.6 125.7 188.5
115 60.2 50.7 76.1

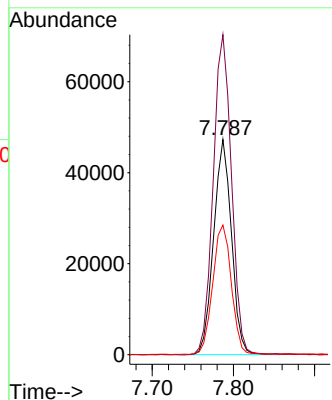

#5
2-Fluorophenol
Concen: 65.036 ng
RT: 5.381 min Scan# 407
Delta R.T. -0.006 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34

Tgt Ion:112 Resp: 291793
Ion Ratio Lower Upper
112 100
64 67.8 53.4 80.2
63 36.1 27.8 41.8


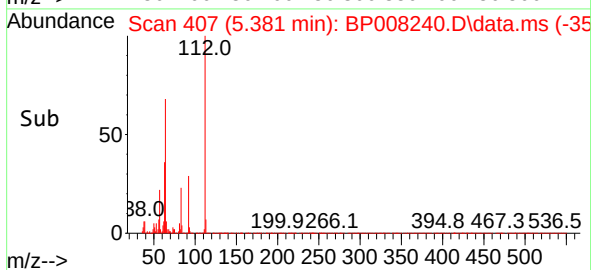
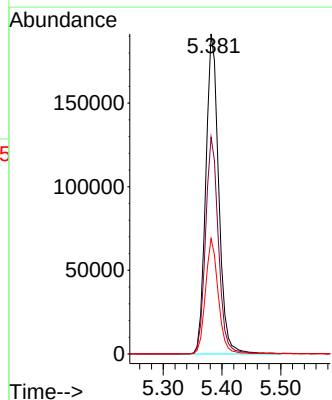
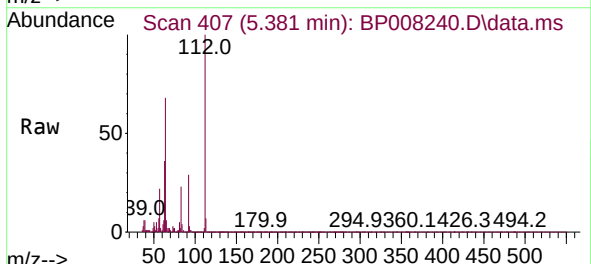




#7
Phenol-d6
Concen: 62.080 ng
RT: 6.975 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34




Instrument :
BNA_P
ClientSampleId :
B-4-7


Tgt Ion: 99 Resp: 375997
Ion Ratio Lower Upper
99 100
42 18.9 14.6 22.0
71 41.2 31.1 46.7

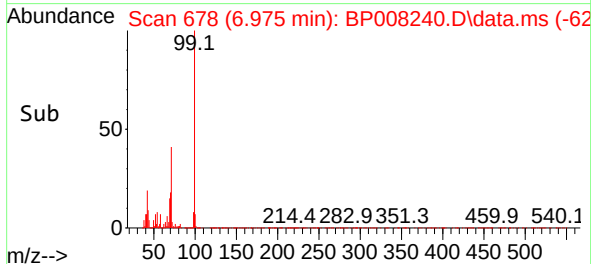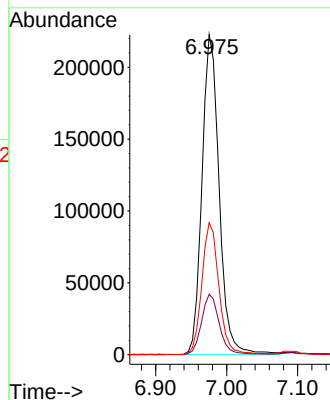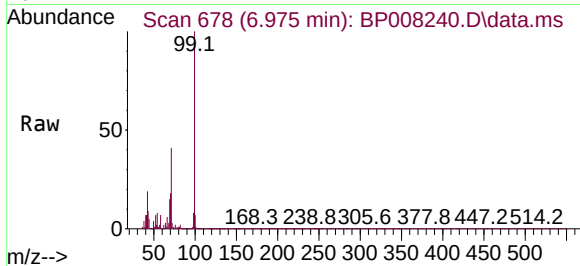

#9
Benzaldehyde
Concen: Below Cal
RT: 6.940 min Scan# 672
Delta R.T. 0.000 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34

Tgt Ion: 77 Resp: 373
Ion Ratio Lower Upper
77 100
105 49.0 71.8 111.8#
106 31.2 67.3 107.3#


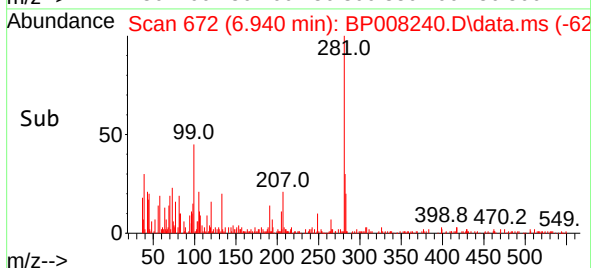
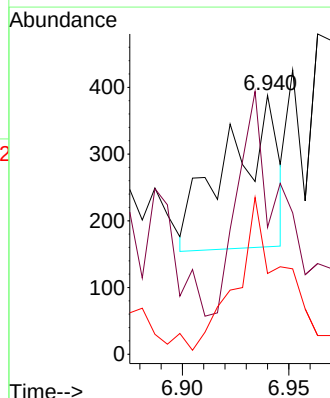
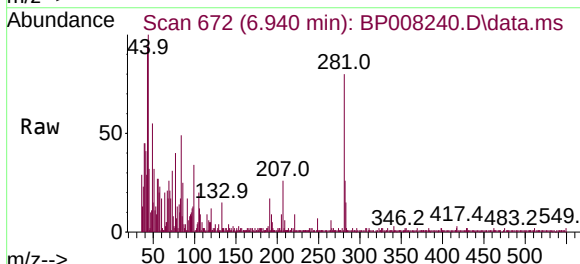




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.587 min Scan# 1013
Delta R.T. -0.012 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34




Instrument :
BNA_P
ClientSampleId :
B-4-7


Tgt Ion:	136	Resp:	270331
Ion Ratio	Lower	Upper	
136	100		
137	10.4	9.0	13.6
54	10.0	8.2	12.4
68	6.4	5.8	8.8

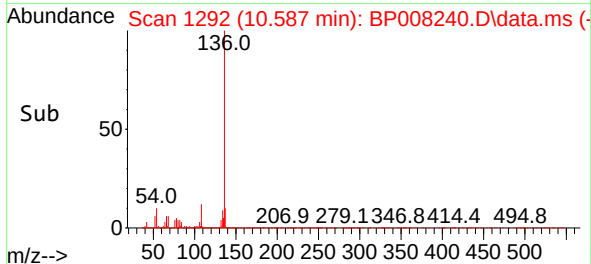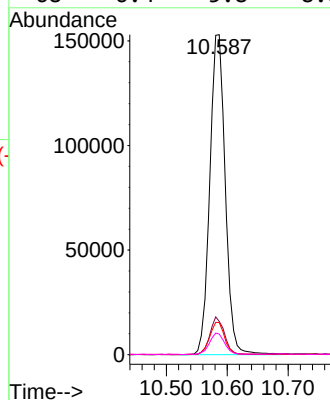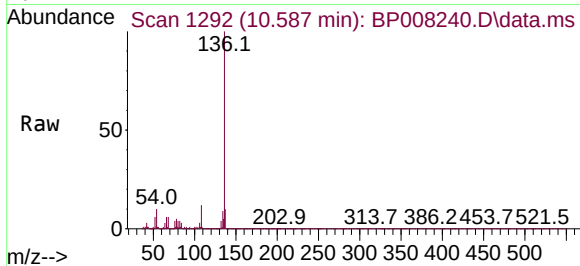

#23
Nitrobenzene-d5
Concen: 40.632 ng
RT: 8.946 min Scan# 1013
Delta R.T. -0.018 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34

Tgt Ion:	82	Resp:	241550
Ion Ratio	Lower	Upper	
82	100		
128	37.9	29.6	44.4
54	53.1	42.7	64.1


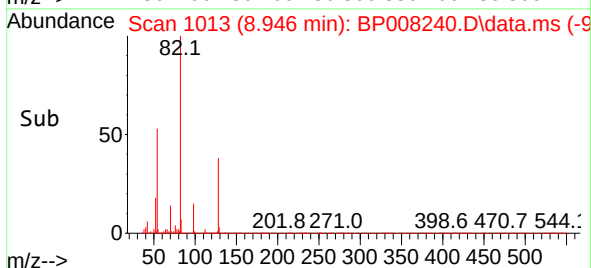
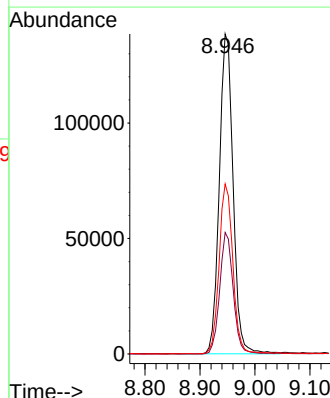
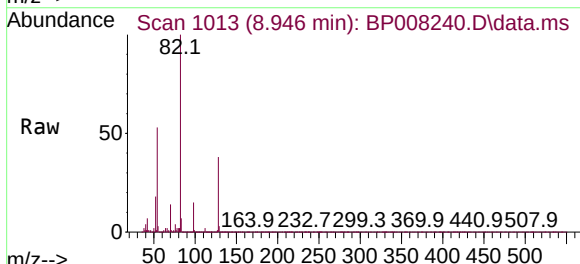




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.434 min Scan# 1946
Delta R.T. -0.012 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34




Instrument :
BNA_P
ClientSampleId :
B-4-7


Tgt Ion:	164	Resp:	181041
Ion Ratio	Lower	Upper	
164	100		
162	99.0	81.9	122.9
160	45.0	35.4	53.0

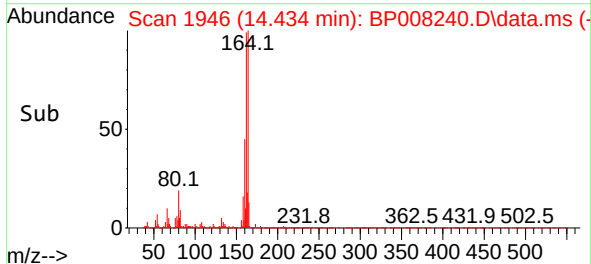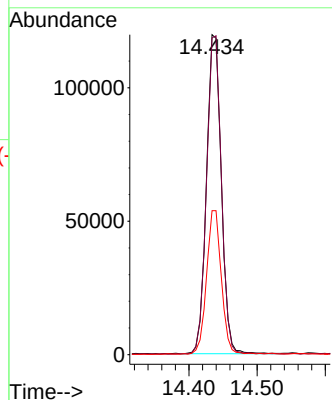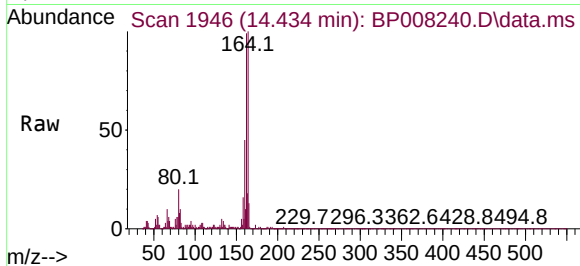

#42
2,4,6-Tribromophenol
Concen: 65.393 ng
RT: 15.940 min Scan# 2202
Delta R.T. -0.012 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34

Tgt Ion:	330	Resp:	151319
Ion Ratio	Lower	Upper	
330	100		
332	97.2	77.0	115.4
141	32.4	28.4	42.6


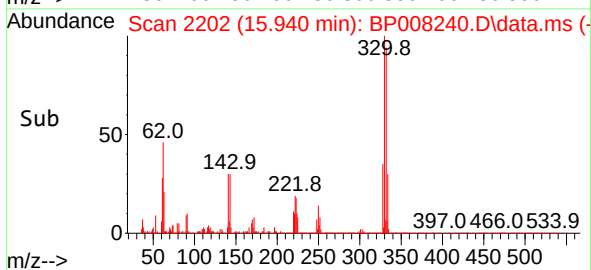
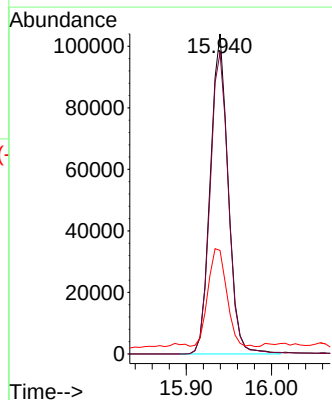
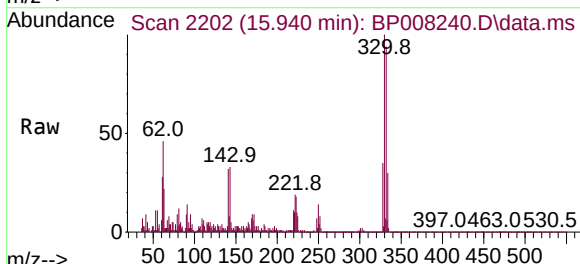


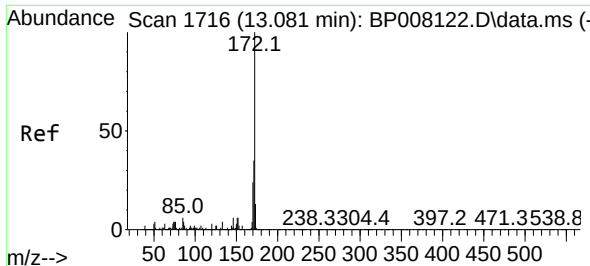

#45
2-Fluorobiphenyl
Concen: 42.534 ng
RT: 13.057 min Scan# 1
Delta R.T. -0.012 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34




Instrument :
BNA_P
ClientSampleId :
B-4-7


Tgt Ion:172	Resp: 530137
Ion Ratio	Lower Upper
172 100	
171 36.4	28.0 42.0
170 23.8	18.9 28.3

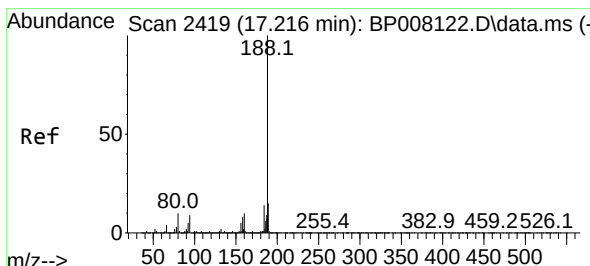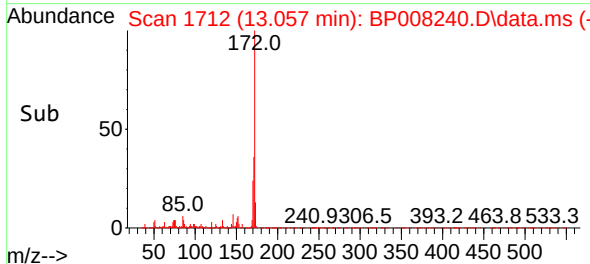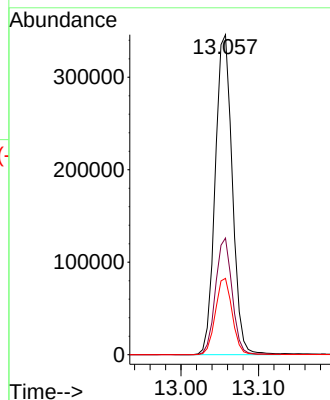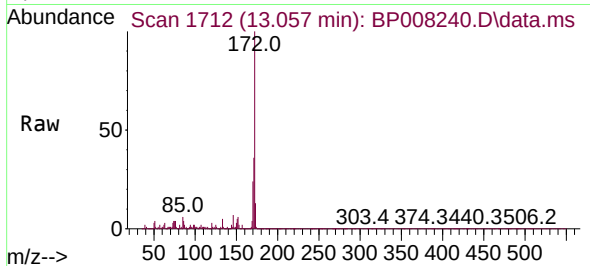

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.198 min Scan# 2416
Delta R.T. -0.012 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34

Tgt	Ion:188	Resp:	374291
Ion	Ratio	Lower	Upper
188	100		
94	9.4	7.2	10.8
80	10.5	8.2	12.4


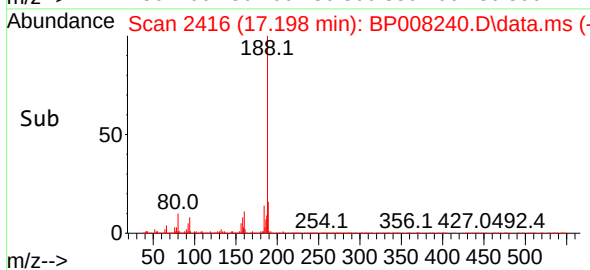
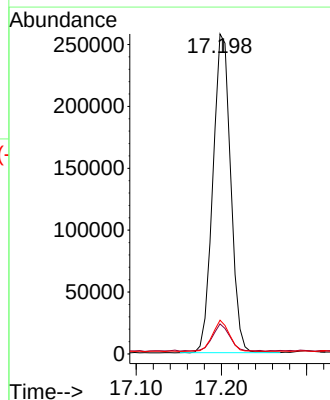
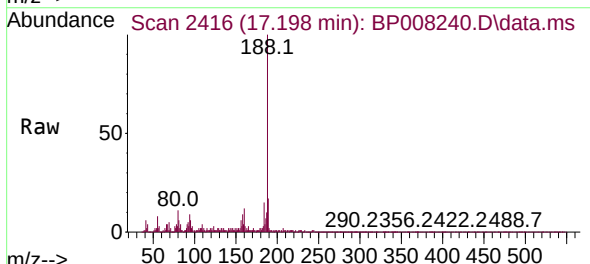


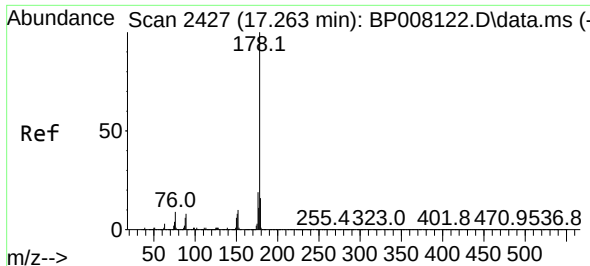

#71
Phenanthrene
Concen: 3.584 ng
RT: 17.239 min Scan# 2423
Delta R.T. -0.012 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34




Instrument :
BNA_P
ClientSampleId :
B-4-7


Tgt Ion:178 Resp: 70822
Ion Ratio Lower Upper
178 100
176 21.0 15.3 22.9
179 22.9 12.5 18.7#

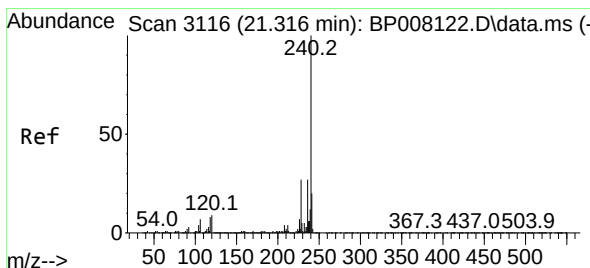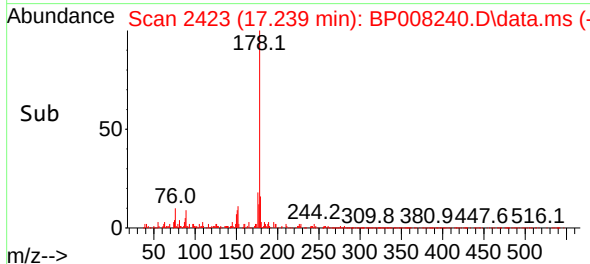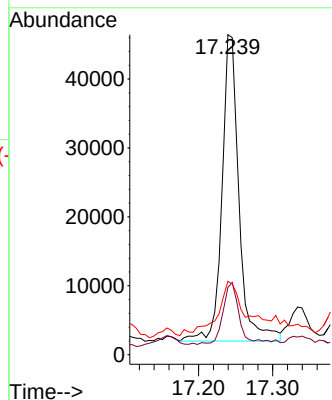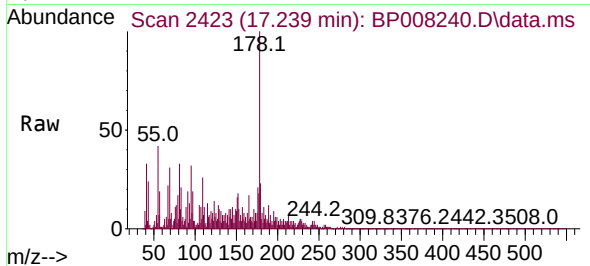

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.310 min Scan# 3115
Delta R.T. -0.006 min
Lab File: BP008240.D
Acq: 06 Dec 2021 21:34

Tgt Ion:240 Resp: 408193
Ion Ratio Lower Upper
240 100
120 9.7 7.3 10.9
236 28.8 21.4 32.2


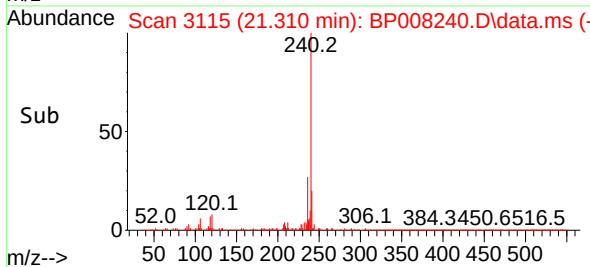
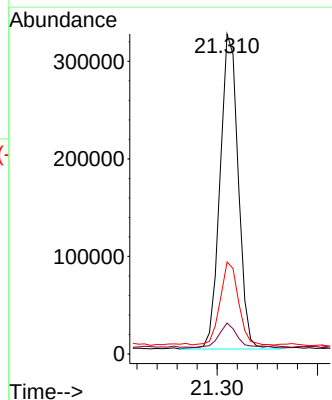
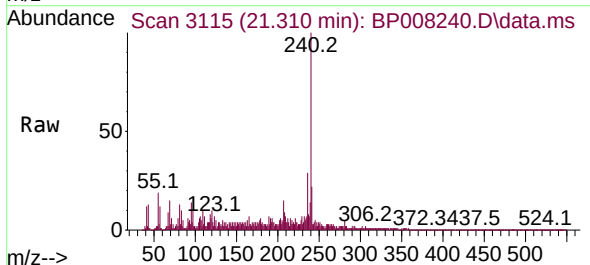




#79
 Terphenyl-d14
 Concen: 45.129 ng
 RT: 19.775 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP008240.D
 Acq: 06 Dec 2021 21:34




Instrument :
 BNA_P
 ClientSampleId :
 B-4-7


Tgt Ion:244	Resp: 881444
Ion Ratio	Lower Upper
244 100	
212 8.2	6.0 9.0
122 8.4	6.6 9.8

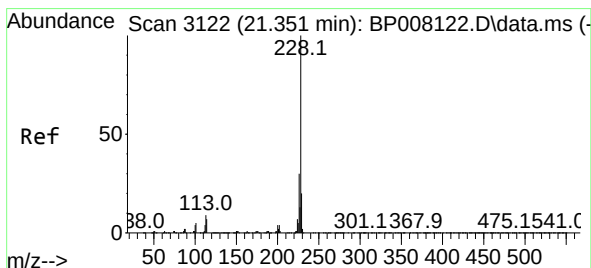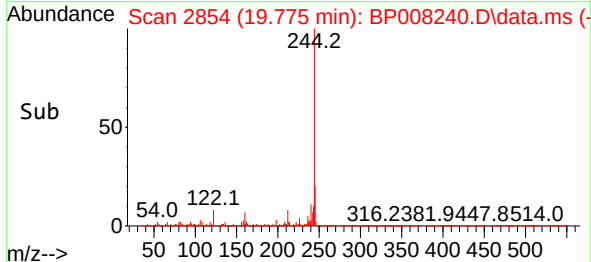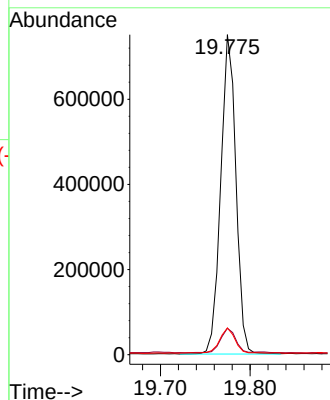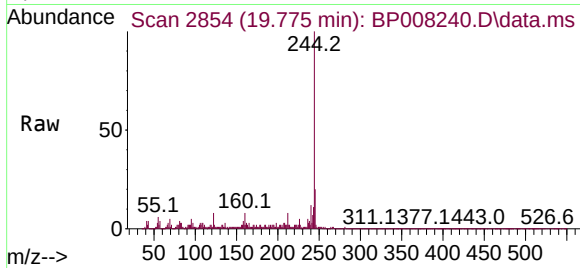

#83
 Chrysene
 Concen: 3.120 ng
 RT: 21.351 min Scan# 3122
 Delta R.T. 0.000 min
 Lab File: BP008240.D
 Acq: 06 Dec 2021 21:34

Tgt	Ion:228	Resp:	80313
Ion	Ratio	Lower	Upper
228	100		
226	44.7	24.0	36.0#
229	64.9	15.8	23.8#

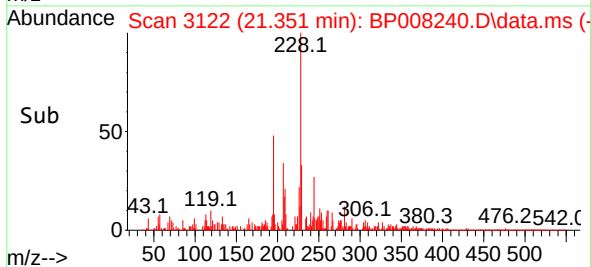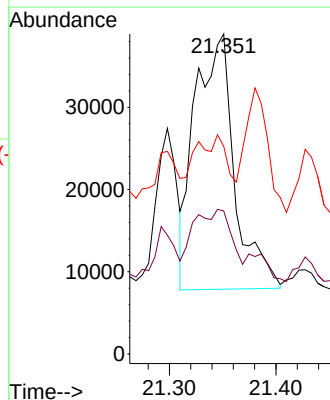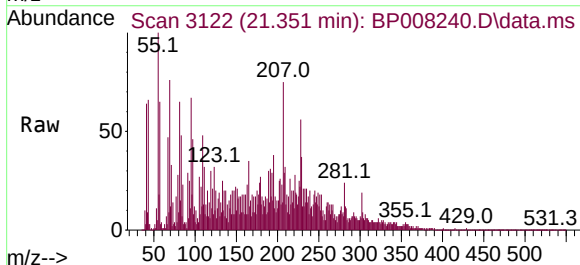

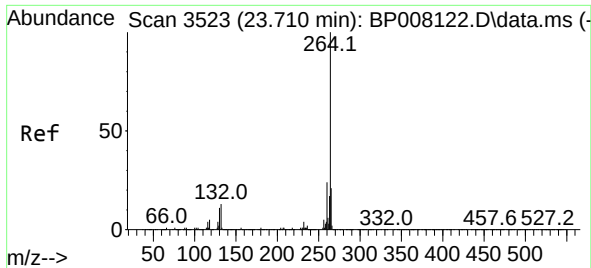

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.721 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BP008240.D
 Acq: 06 Dec 2021 21:34

Instrument :
 BNA_P
 ClientSampleId :
 B-4-7

Tgt Ion:264 Resp: 445058
 Ion Ratio Lower Upper
 264 100
 260 26.0 19.4 29.2
 265 25.3 17.6 26.4

