
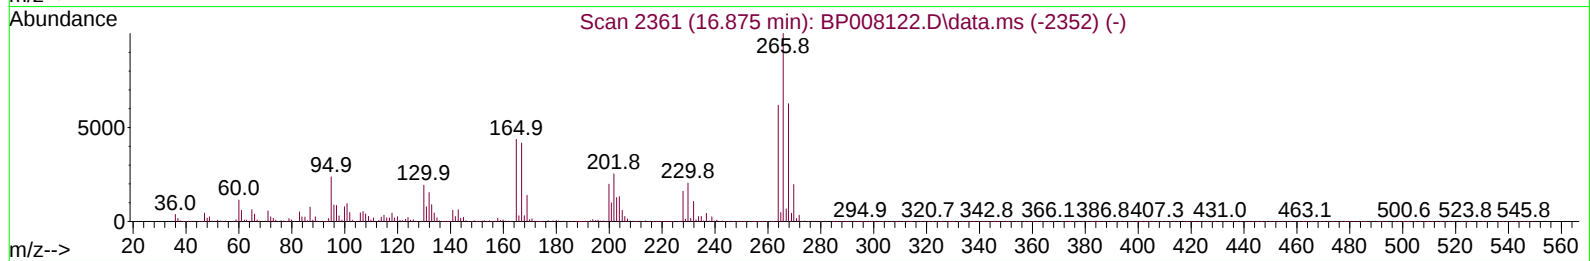
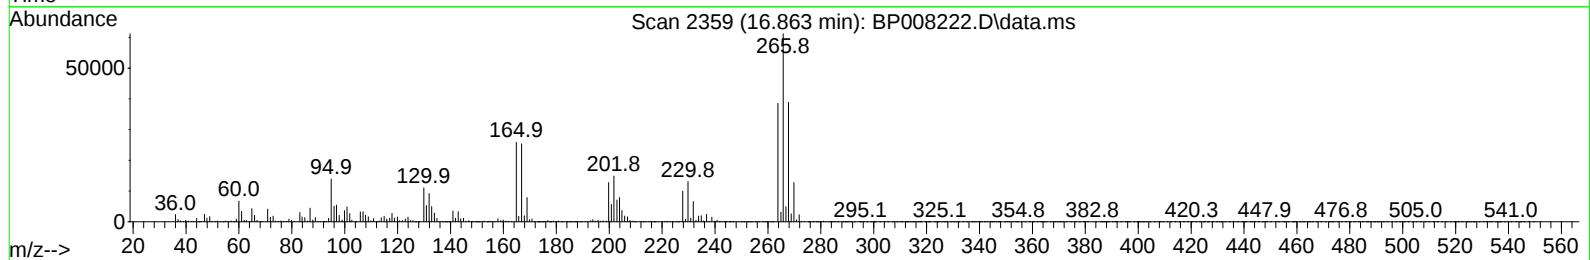


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
Data File : BP008222.D
Acq On : 06 Dec 2021 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 12:54:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 03 14:39:24 2021
Response via : Initial Calibration

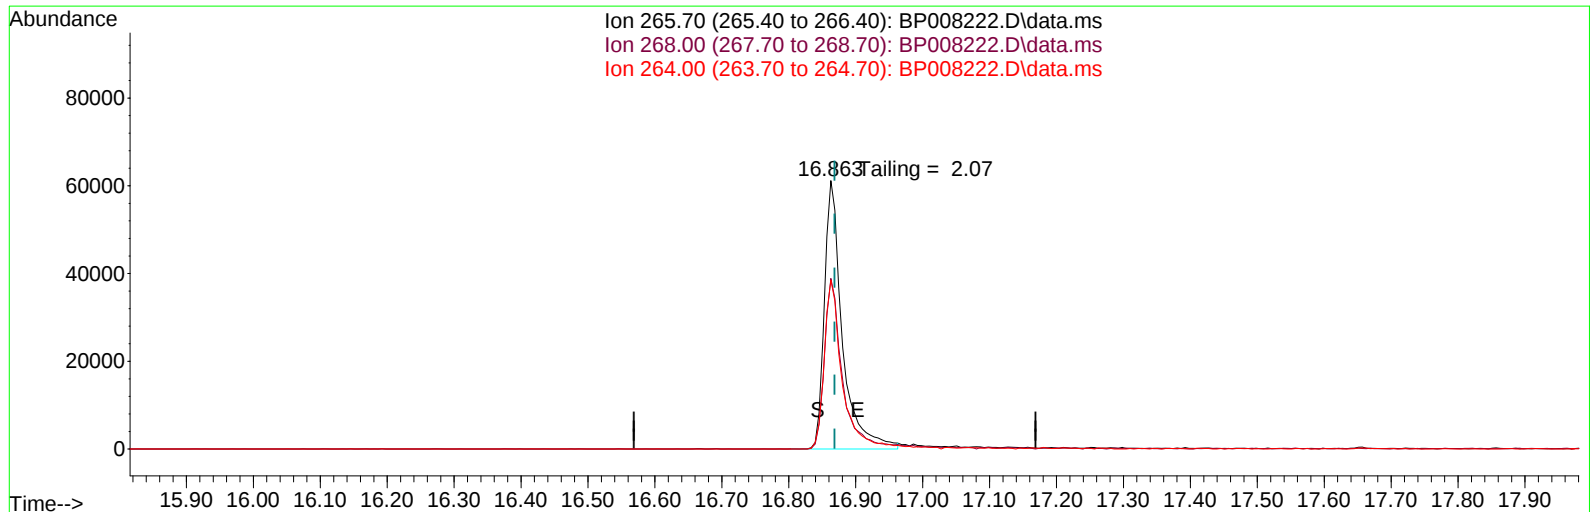

TIC: BP008222.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.006) 509562.62 ng

response 115252

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.54
264.00	61.90	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
 Data File : BP008222.D
 Acq On : 06 Dec 2021 10:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 12:54:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 03 14:39:24 2021
 Response via : Initial Calibration

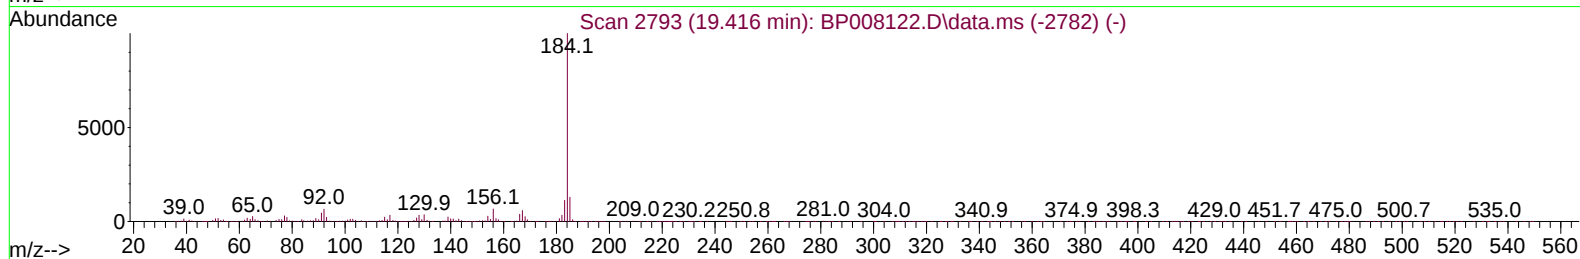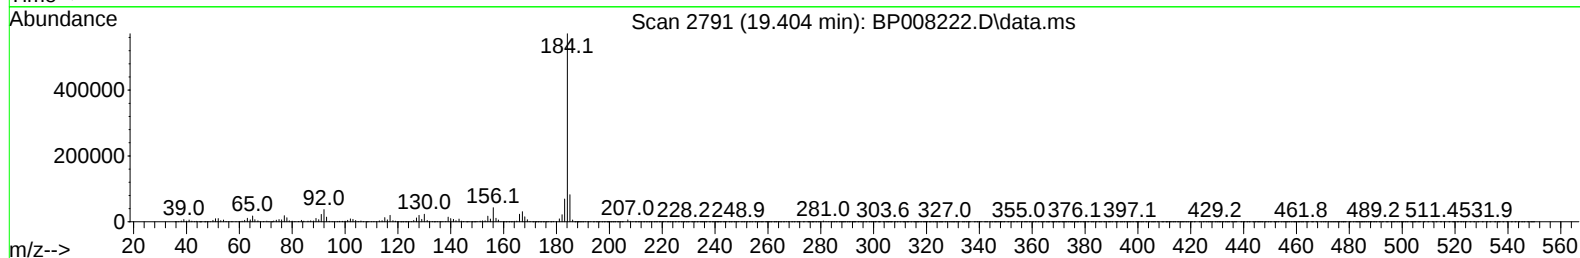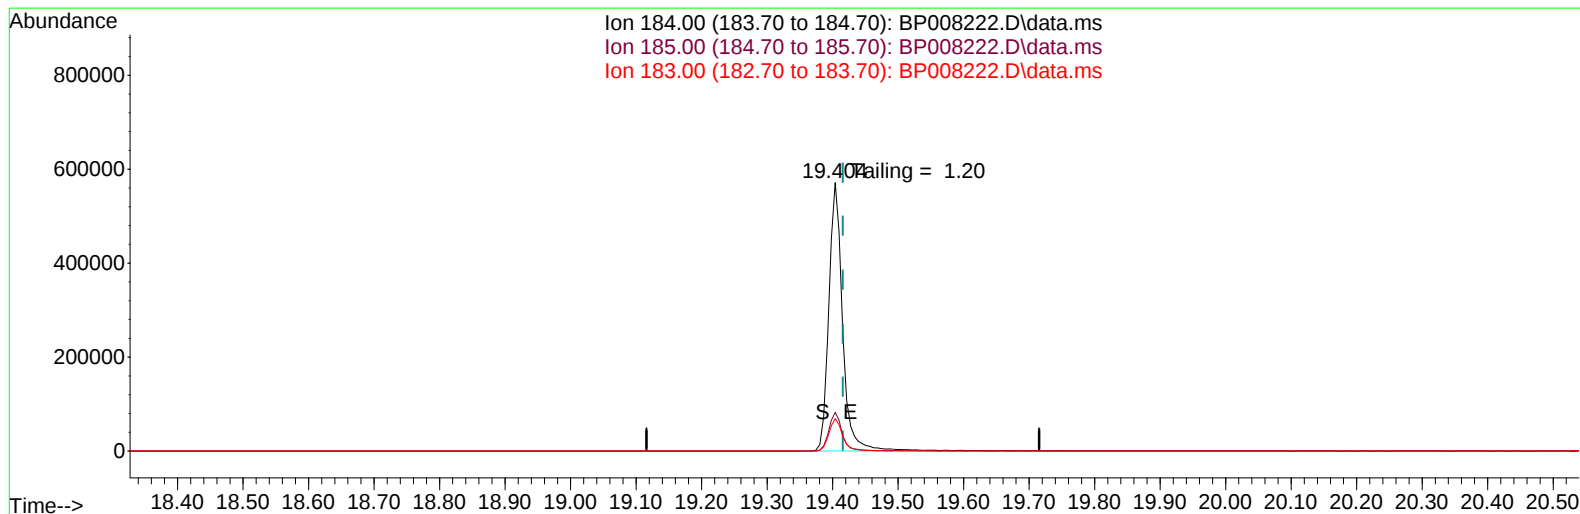

TIC: BP008222.D\data.ms

(77) Benzidine**19.404min (-0.012) 56498.33 ng****response 833900**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.39
183.00	11.40	12.05
0.00	0.00	0.00