

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
 Data File : BP008241.D
 Acq On : 06 Dec 2021 22:08
 Operator : CG/JU
 Sample : M4939-01 2X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OR-03-120321

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.928	325	330	336	rVB3	8775	19192	1.27%	0.162%
2	5.387	401	408	424	rVB	494308	789932	52.37%	6.674%
3	5.811	472	480	485	rVB3	19726	31113	2.06%	0.263%
4	6.981	667	679	693	rBV	454595	804464	53.33%	6.797%
5	7.087	693	697	707	rVB	20764	38708	2.57%	0.327%
6	7.787	809	816	825	rBV	307079	483397	32.05%	4.084%
7	8.952	1007	1014	1022	rBV	268539	461739	30.61%	3.901%
8	10.587	1282	1292	1299	rBV	373988	648371	42.99%	5.478%
9	11.781	1490	1495	1502	rBV6	10353	19895	1.32%	0.168%
10	12.252	1570	1575	1582	rVB3	19520	33951	2.25%	0.287%
11	12.469	1607	1612	1616	rBV	21769	39596	2.63%	0.335%
12	12.510	1616	1619	1624	rVB4	13603	20097	1.33%	0.170%
13	12.981	1695	1699	1704	rVB4	16656	24718	1.64%	0.209%
14	13.057	1705	1712	1732	rVV	734546	1110185	73.60%	9.380%
15	13.269	1744	1748	1756	rVB3	26746	41615	2.76%	0.352%
16	13.381	1761	1767	1770	rBV3	10801	20385	1.35%	0.172%
17	13.599	1799	1804	1806	rBV4	20677	33544	2.22%	0.283%
18	13.763	1826	1832	1836	rBV	32247	59224	3.93%	0.500%
19	13.810	1836	1840	1846	rVB3	22884	39522	2.62%	0.334%
20	13.928	1857	1860	1863	rVB2	20873	23250	1.54%	0.196%
21	14.098	1884	1889	1893	rBV8	11953	22442	1.49%	0.190%
22	14.163	1896	1900	1907	rVB	30389	48792	3.23%	0.412%
23	14.346	1927	1931	1935	rVB	37436	52097	3.45%	0.440%
24	14.440	1939	1947	1954	rBV	574281	850863	56.41%	7.189%
25	14.657	1978	1984	1992	rVB4	16815	44039	2.92%	0.372%
26	14.846	2013	2016	2020	rVB2	29778	41321	2.74%	0.349%
27	14.922	2025	2029	2033	rVB	22062	31430	2.08%	0.266%
28	14.969	2033	2037	2042	rBV6	17148	25821	1.71%	0.218%
29	15.304	2090	2094	2101	rVB2	38463	53141	3.52%	0.449%
30	15.493	2121	2126	2130	rBV3	31056	48821	3.24%	0.412%
31	15.616	2144	2147	2151	rVB5	14448	20147	1.34%	0.170%
32	15.710	2159	2163	2168	rVB2	37963	53946	3.58%	0.456%
33	15.940	2195	2202	2210	rBV	553673	839997	55.69%	7.097%
34	16.169	2237	2241	2243	rBV3	63333	87840	5.82%	0.742%
35	16.551	2304	2306	2312	rBV3	14789	20709	1.37%	0.175%
36	16.969	2374	2377	2382	rVV	42147	49286	3.27%	0.416%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
Data File : BP008241.D
Acq On : 06 Dec 2021 22:08
Operator : CG/JU
Sample : M4939-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-03-120321

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.022	2382	2386	2393	rVB	57558	94615	6.27%	0.799%
38	17.204	2411	2417	2421	rBV	677684	973933	64.57%	8.228%
39	17.245	2421	2424	2429	rVB	151095	203060	13.46%	1.716%
40	17.334	2437	2439	2445	rVB	54783	70235	4.66%	0.593%
41	17.710	2500	2503	2510	rBV2	43951	53649	3.56%	0.453%
42	18.075	2563	2565	2567	rBV	40444	35616	2.36%	0.301%
43	18.263	2594	2597	2601	rVB3	56301	80608	5.34%	0.681%
44	18.386	2615	2618	2622	rBV	48596	67871	4.50%	0.573%
45	19.222	2756	2760	2767	rBV	273628	409679	27.16%	3.461%
46	19.575	2816	2820	2827	rVB	243828	375080	24.87%	3.169%
47	19.775	2849	2854	2858	rVB	1296962	1508360	100.00%	12.744%
48	21.310	3111	3115	3119	rVB	762861	929808	61.64%	7.856%




Sum of corrected areas: 11836104

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
Data File : BP008241.D
Acq On : 06 Dec 2021 22:08
Operator : CG/JU
Sample : M4939-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-03-120321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

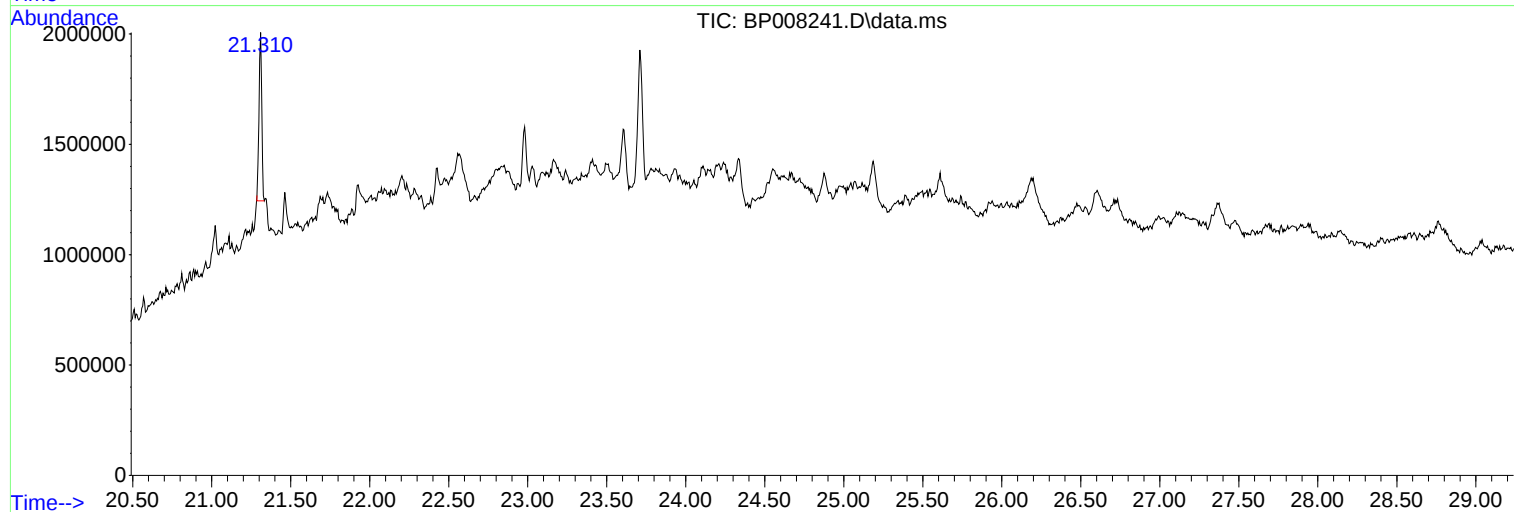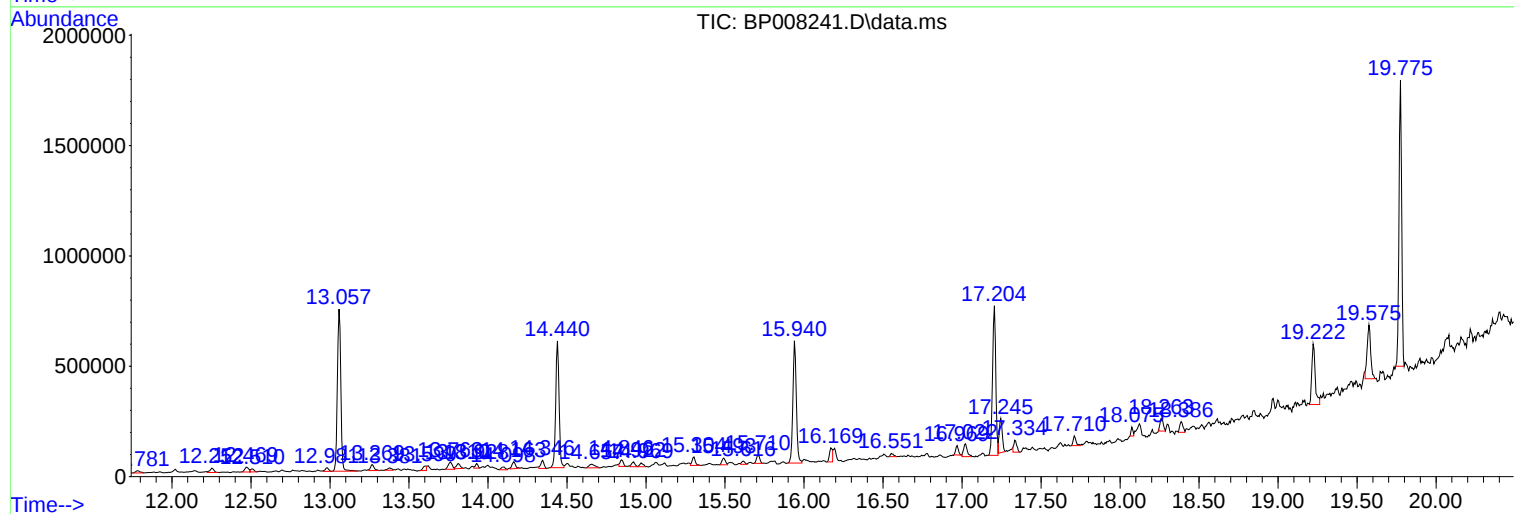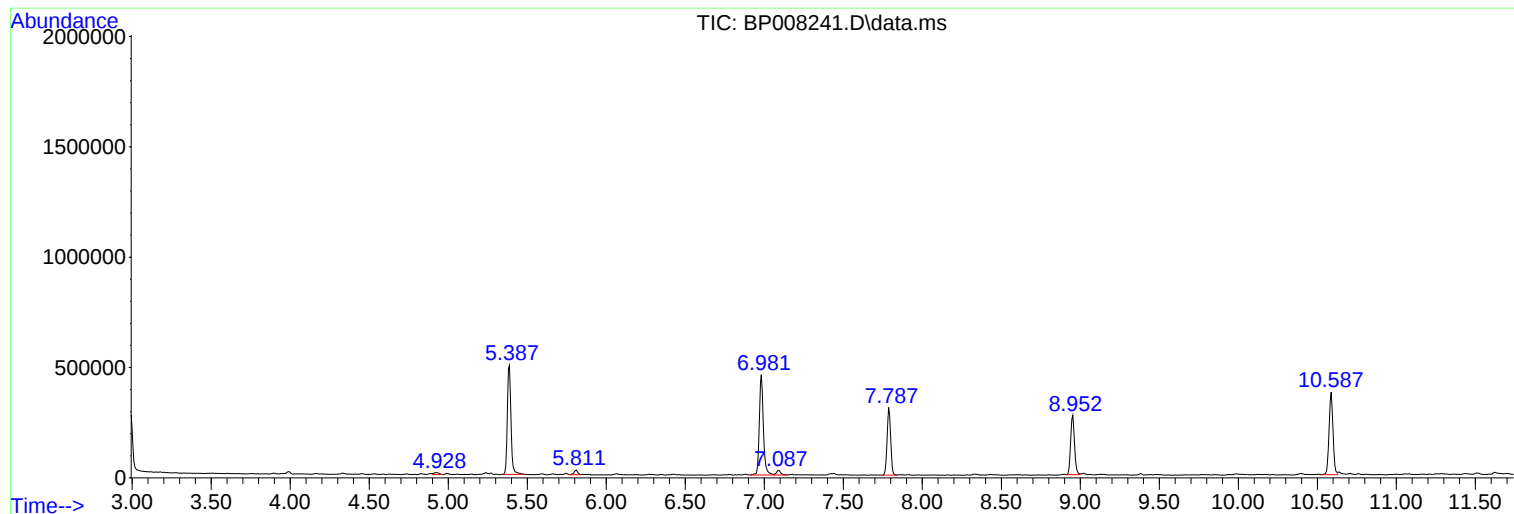

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
Data File : BP008241.D
Acq On : 06 Dec 2021 22:08
Operator : CG/JU
Sample : M4939-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-03-120321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
Data File : BP008241.D
Acq On : 06 Dec 2021 22:08
Operator : CG/JU
Sample : M4939-01 2X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OR-03-120321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------