
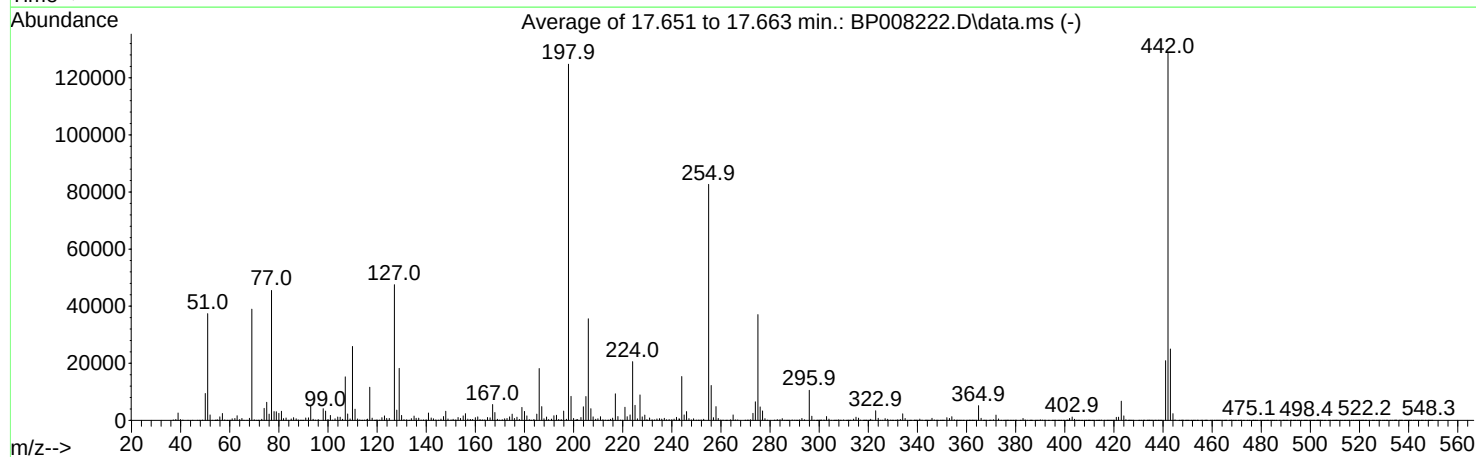


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
 Data File : BP008222.D
 Acq On : 06 Dec 2021 10:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 03 14:39:24 2021

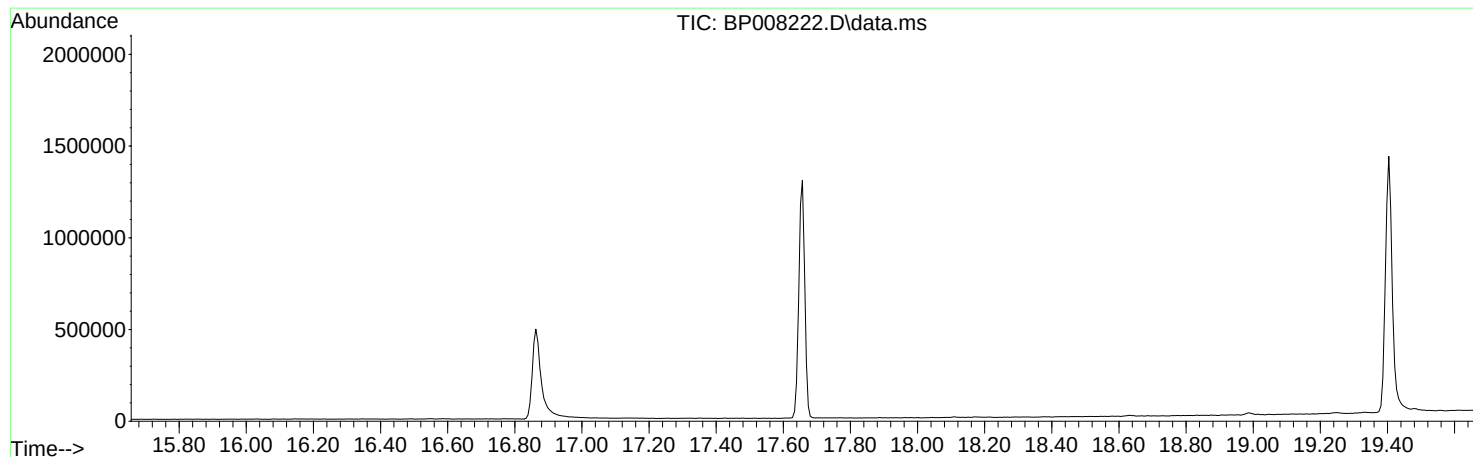




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	37411	PASS
68	69	0.00	2	1.8	706	PASS
69	198	0.00	100	31.2	38966	PASS
70	69	0.00	2	0.6	252	PASS
127	198	10	80	38.1	47533	PASS
197	198	0.00	2	0.3	390	PASS
198	198	100	100	100.0	124773	PASS
199	198	5	9	6.8	8436	PASS
275	198	10	60	29.7	37043	PASS
365	198	1	100	4.1	5140	PASS
441	198	0.01	100	16.8	20928	PASS
442	442	100	100	100.0	128875	PASS
443	442	15	24	19.4	24981	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
Data File : BP008222.D
Acq On : 06 Dec 2021 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 06 12:54:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 03 14:39:24 2021
Response via : Initial Calibration

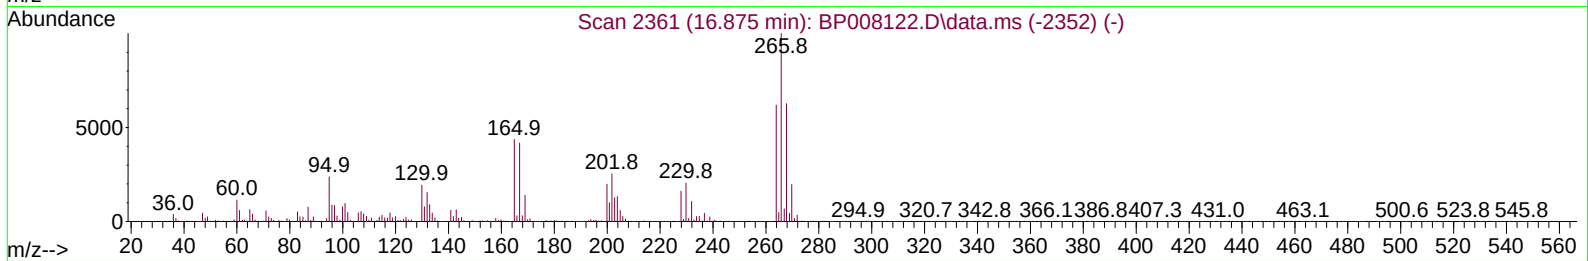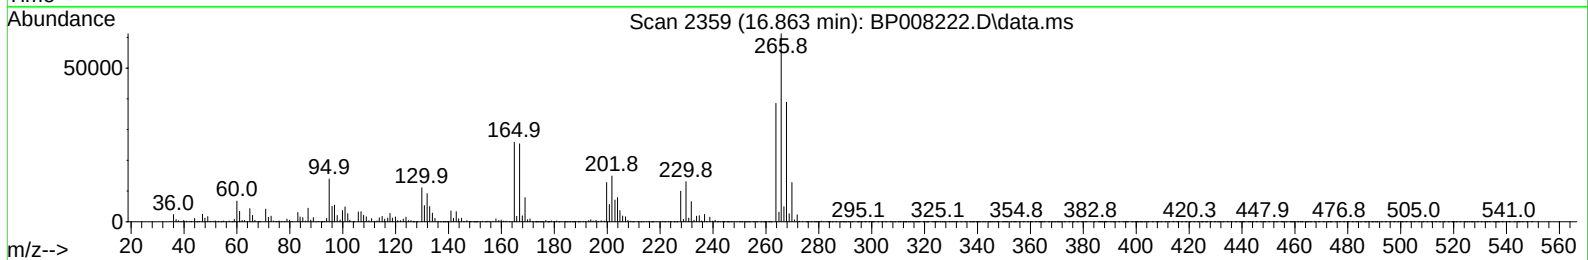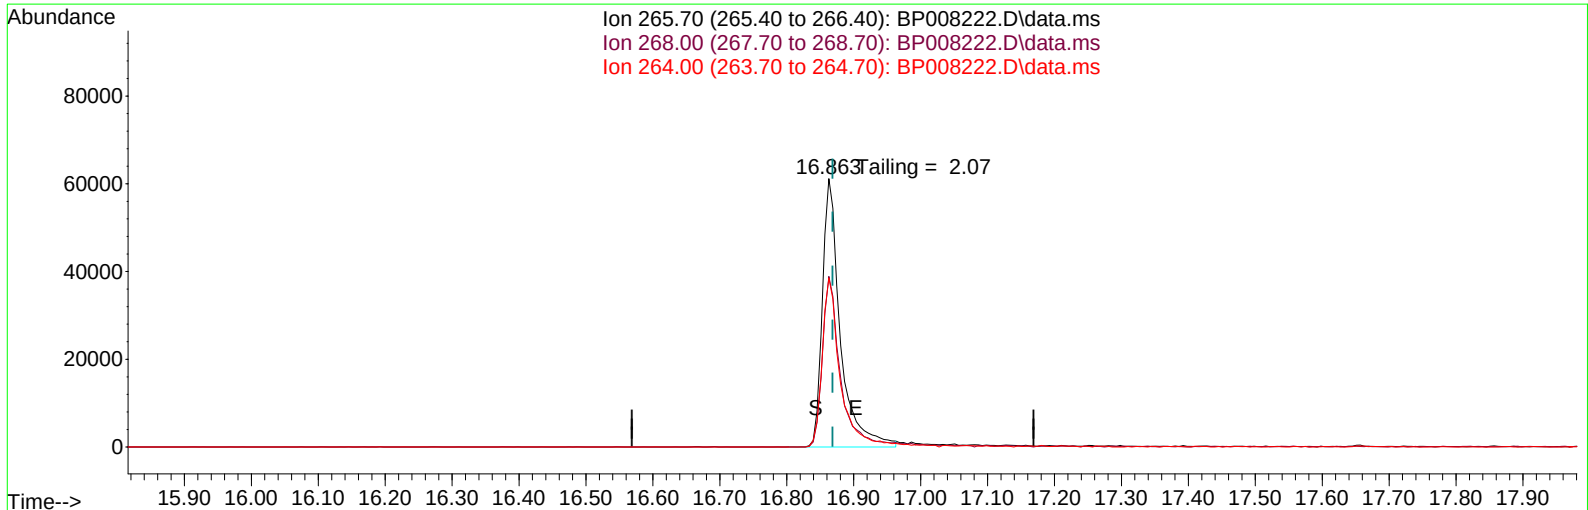

TIC: BP008222.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.006) 509562.62 ng




response 115252

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.54
264.00	61.90	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120621\
Data File : BP008222.D
Acq On : 06 Dec 2021 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 06 12:54:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 03 14:39:24 2021
Response via : Initial Calibration

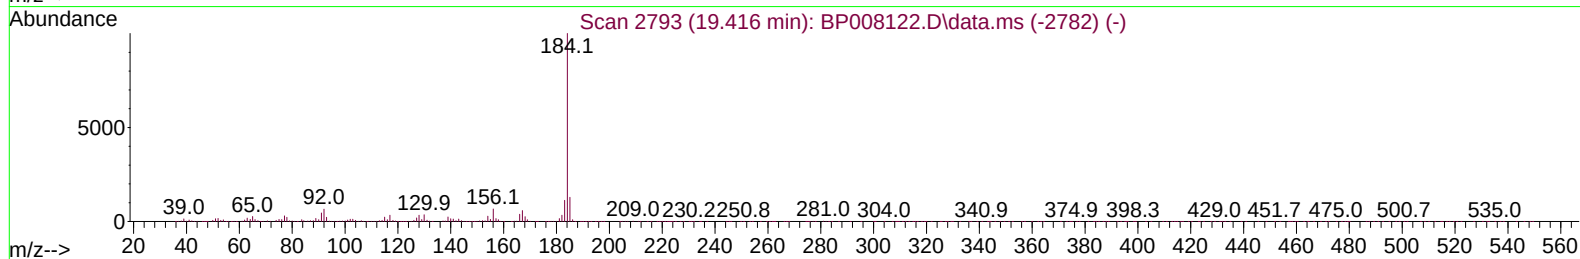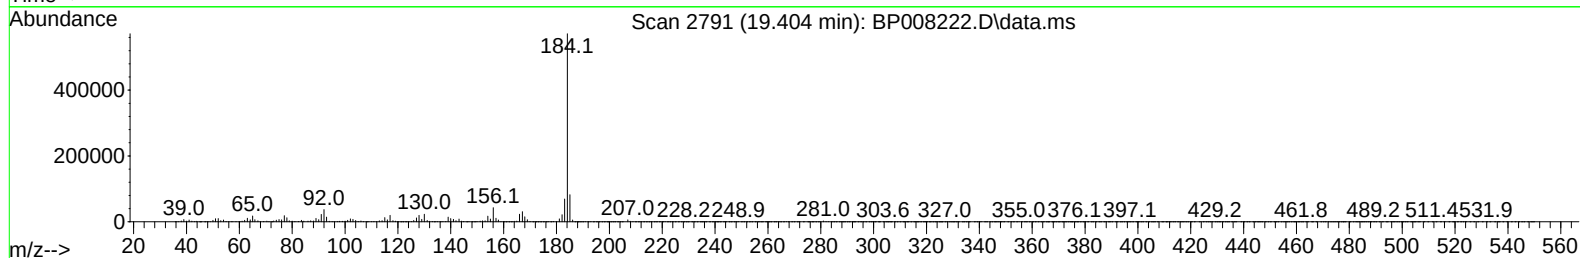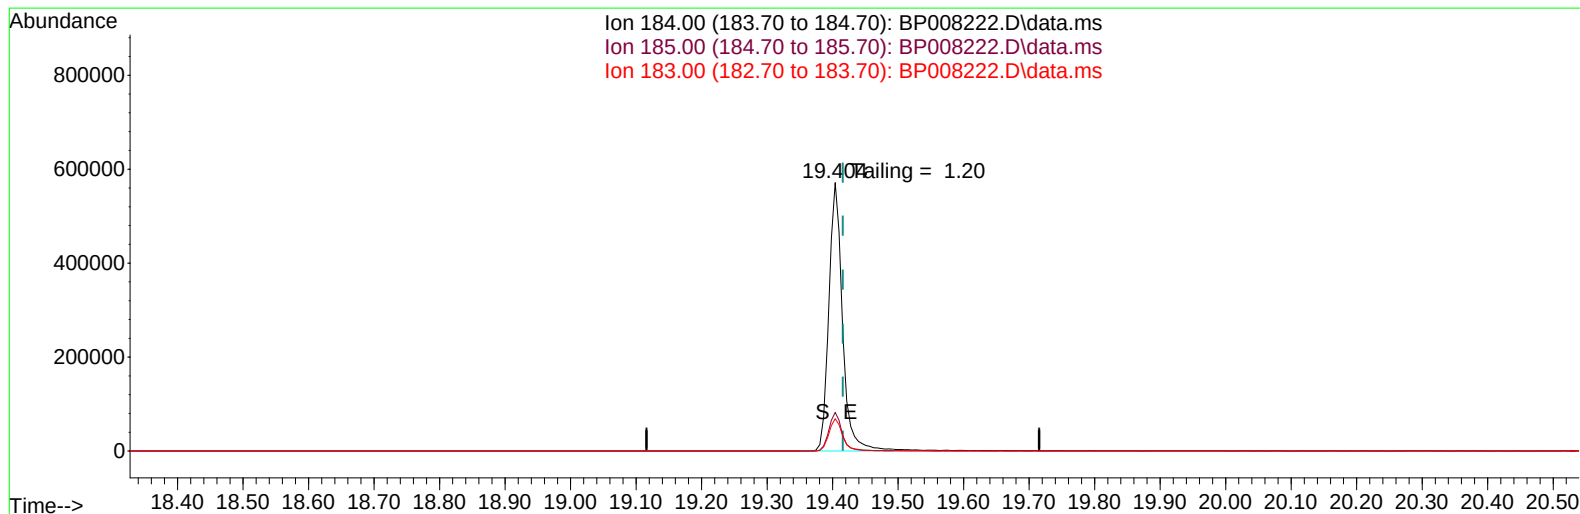

TIC: BP008222.D\data.ms

(77) Benzidine**19.404min (-0.012) 56498.33 ng****response 833900**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.39
183.00	11.40	12.05
0.00	0.00	0.00

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2021	BNA_P	<u>BP008222.D</u>
Compound Name	Response	Retention Time
DDT	459542	20.61
DDD	3841	20.18
DDE	1015	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4856	464398	1.05