
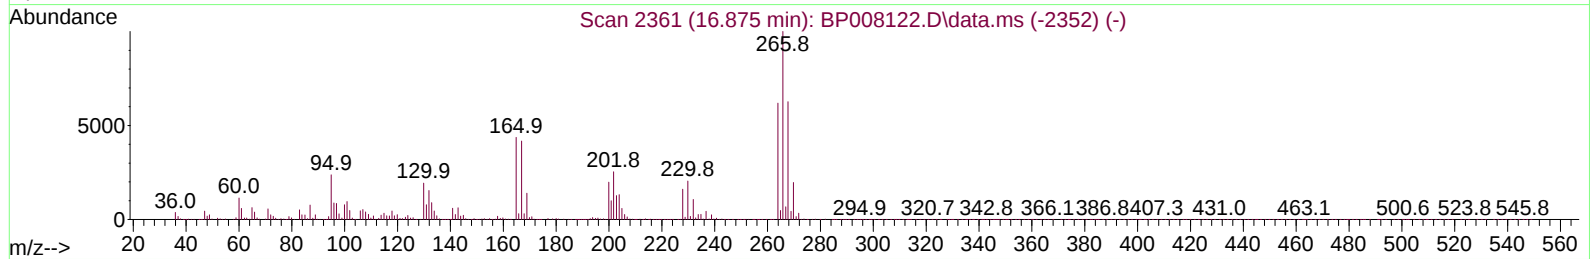
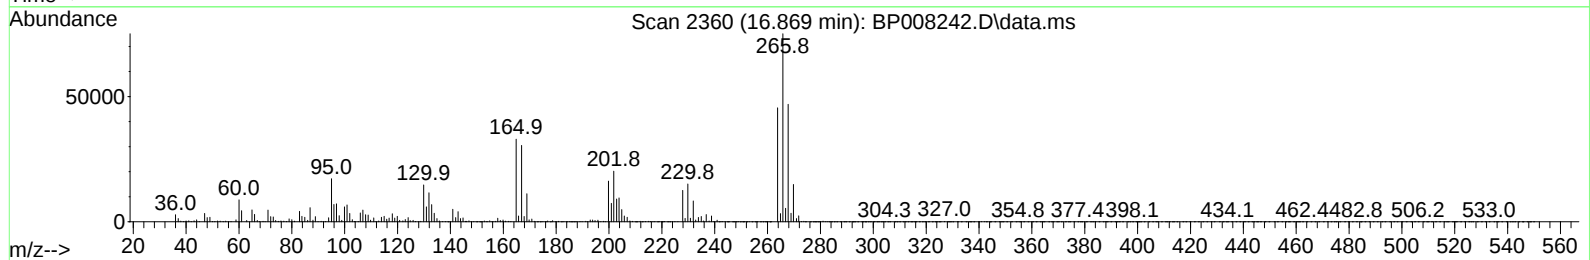


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP120721\  
 Data File : BP008242.D  
 Acq On : 07 Dec 2021 09:28  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 09:13:26 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP112521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 03 14:39:24 2021  
 Response via : Initial Calibration

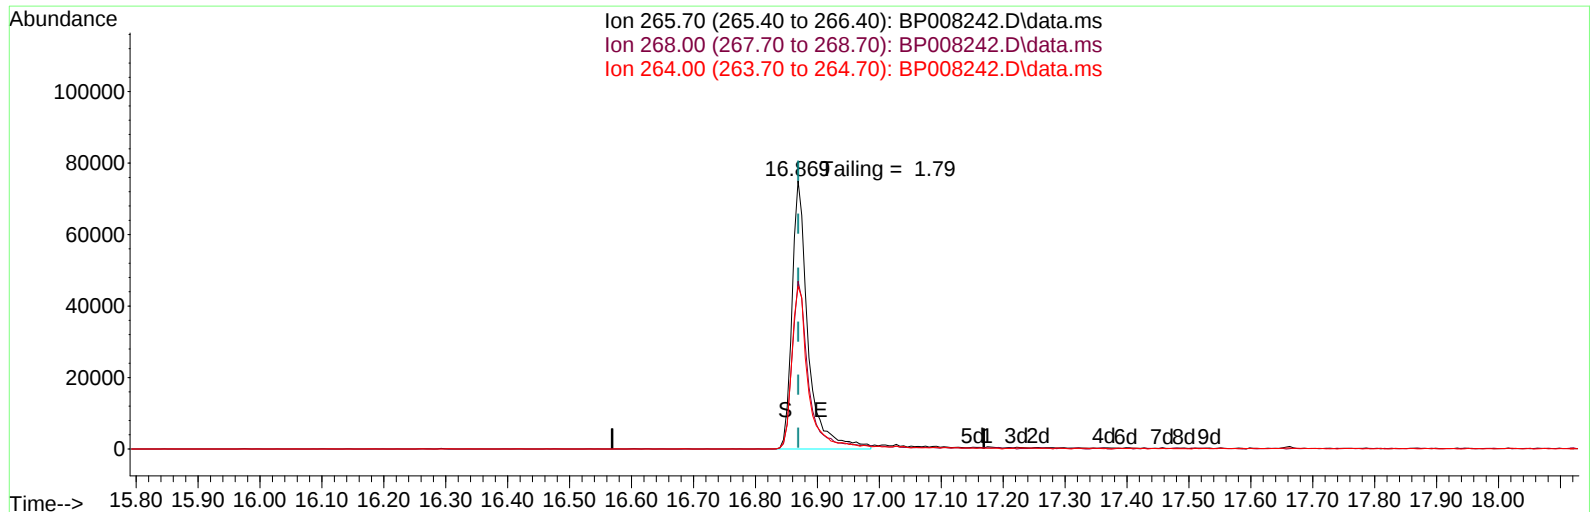

TIC: BP008242.D\data.ms

**(70) Pentachlorophenol (C)**




16.869min (-0.000) 347341.49 ng m

response 142392

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.60  | 62.51  |
| 264.00 | 61.90  | 60.57  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP120721\  
 Data File : BP008242.D  
 Acq On : 07 Dec 2021 09:28  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 09:13:26 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP112521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Dec 03 14:39:24 2021  
 Response via : Initial Calibration

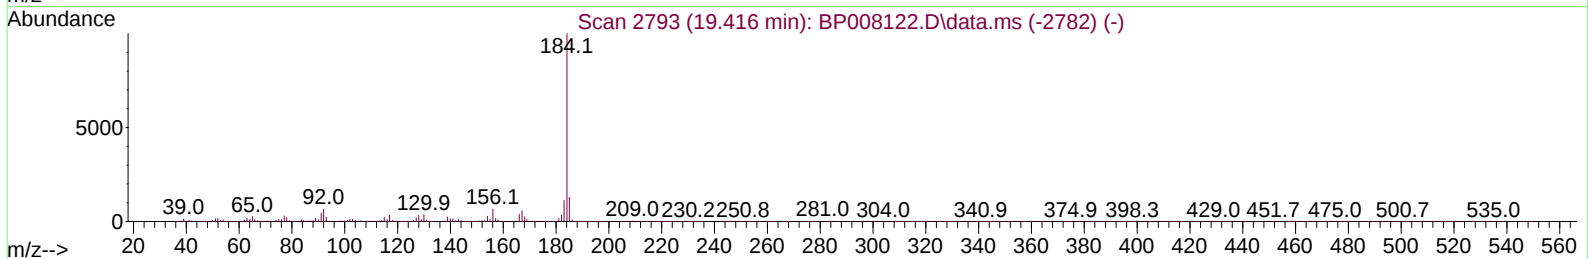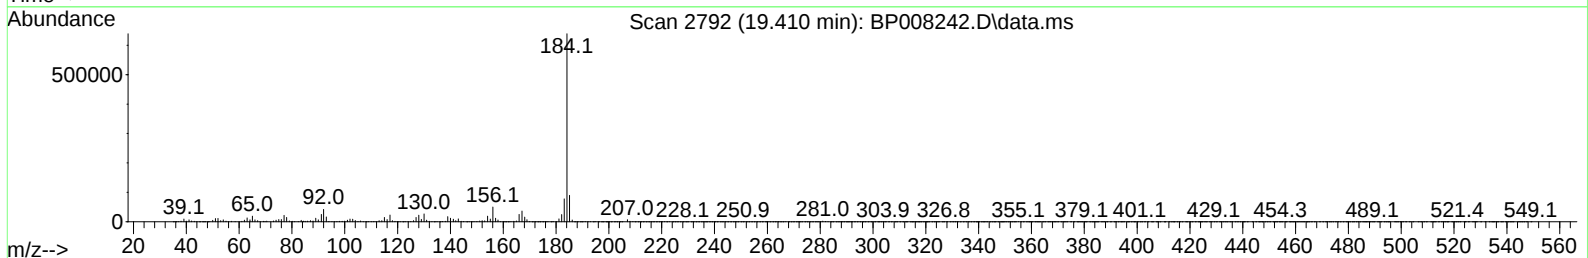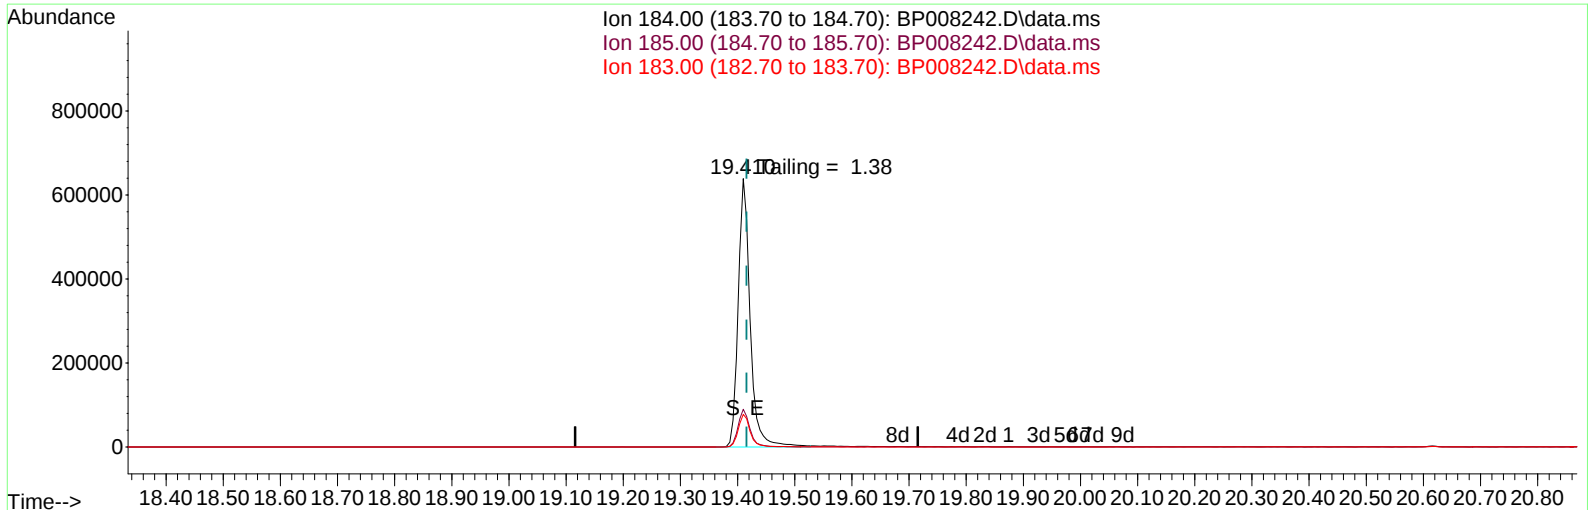

TIC: BP008242.D\data.ms

**(77) Benzidine**

19.410min (-0.006) 487039.19 ng m

response 948677

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 12.90  | 14.06  |
| 183.00 | 11.40  | 12.18  |
| 0.00   | 0.00   | 0.00   |