
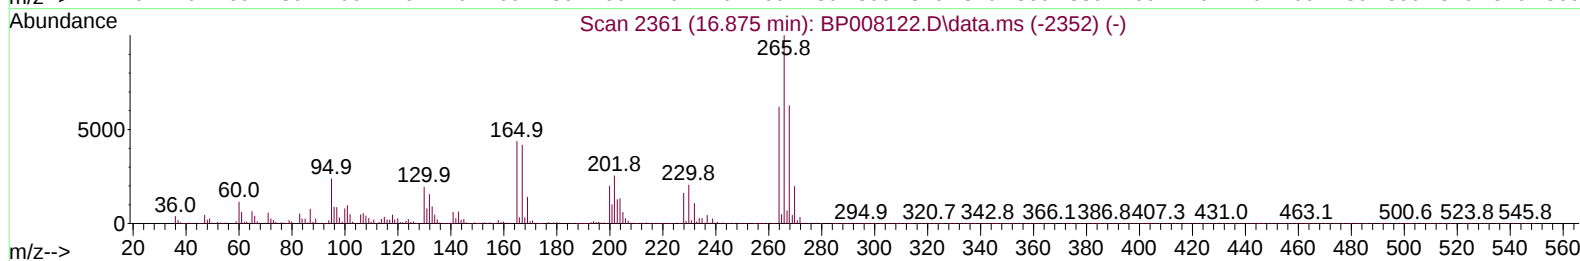
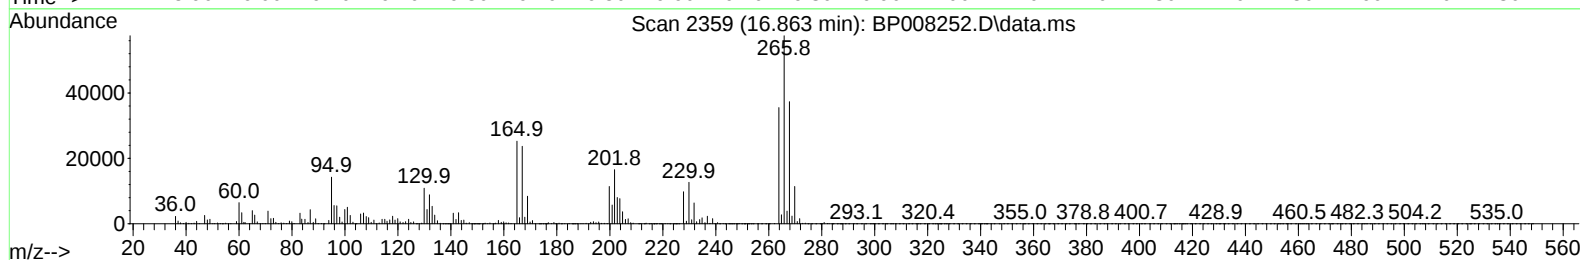


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120721\
Data File : BP008252.D
Acq On : 07 Dec 2021 16:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 09:13:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 03 14:39:24 2021
Response via : Initial Calibration

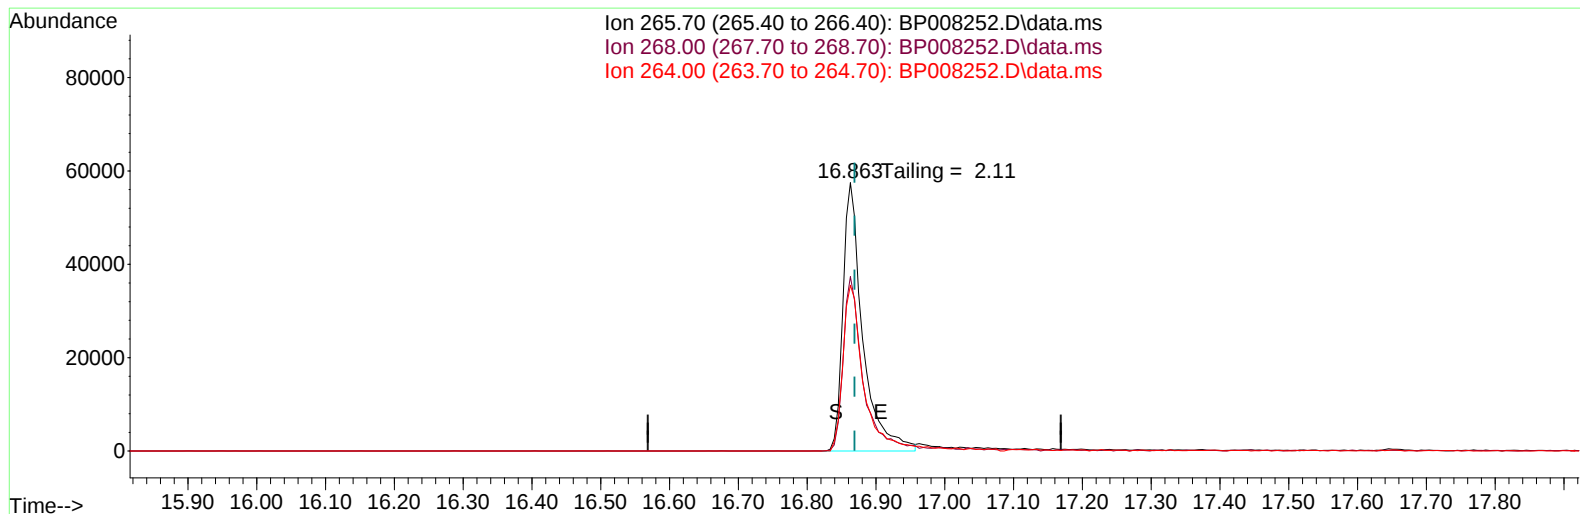

TIC: BP008252.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.006) 354506.68 ng

response 70159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.96
264.00	61.90	61.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120721\
Data File : BP008252.D
Acq On : 07 Dec 2021 16:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 09:13:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 03 14:39:24 2021
Response via : Initial Calibration

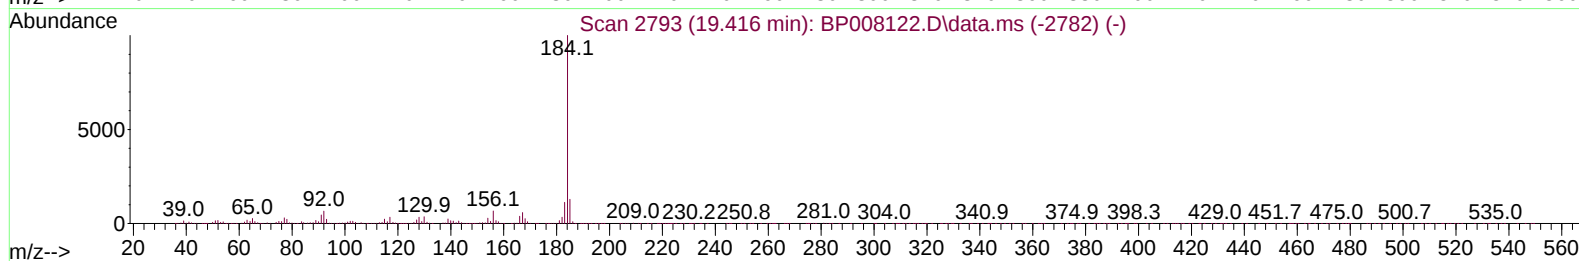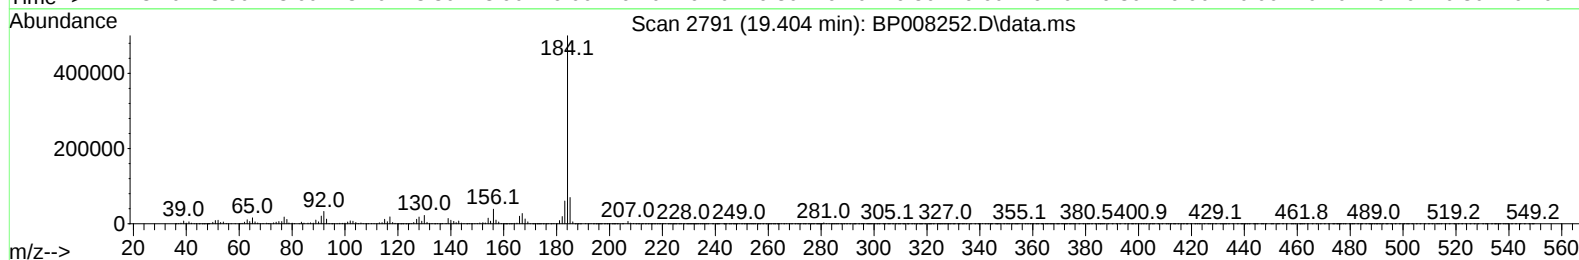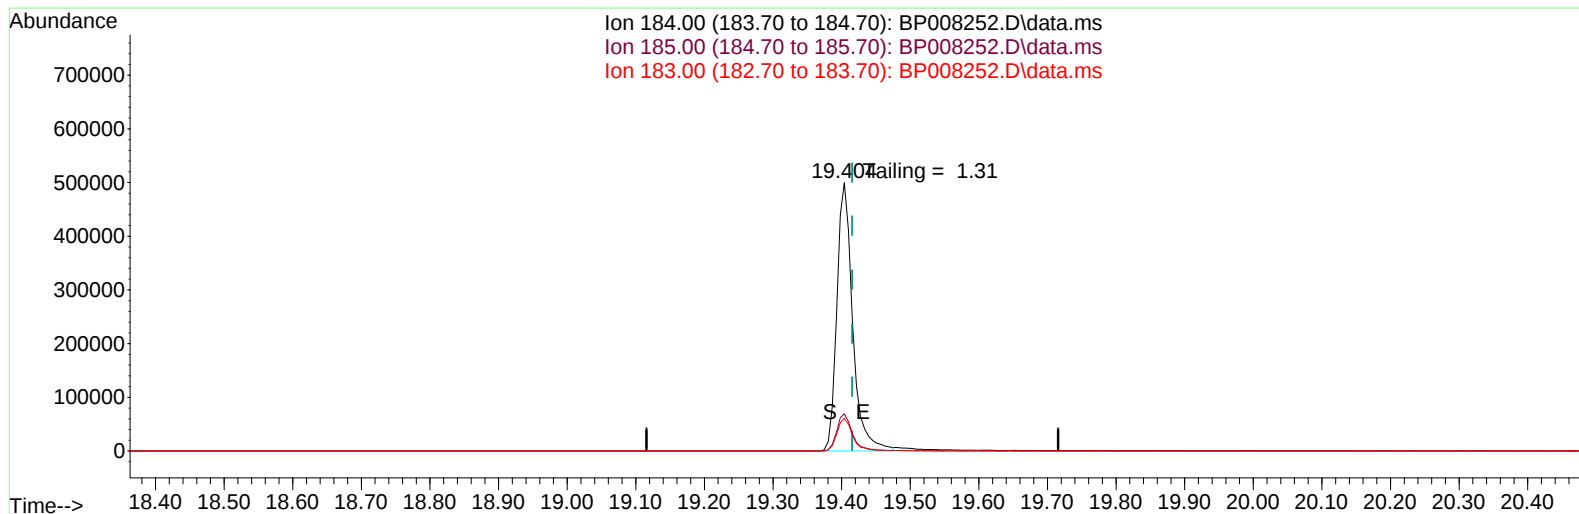

TIC: BP008252.D\data.ms

(77) Benzidine

19.404min (-0.012) 653778.40 ng m

response 798154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.93
183.00	11.40	12.12
0.00	0.00	0.00