
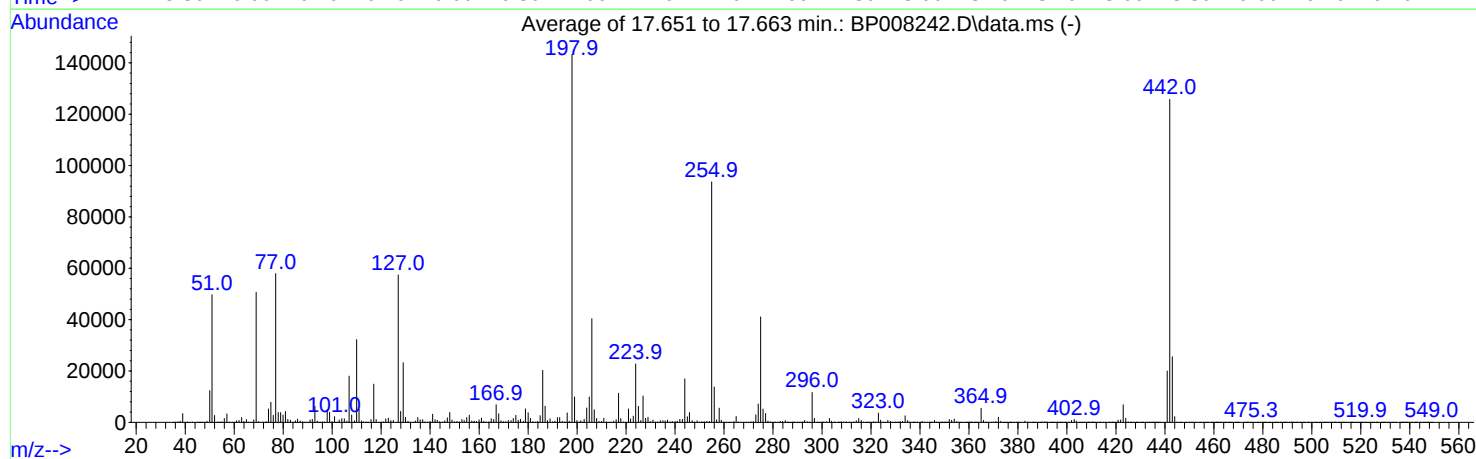


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120721\
 Data File : BP008242.D
 Acq On : 07 Dec 2021 09:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 03 14:39:24 2021

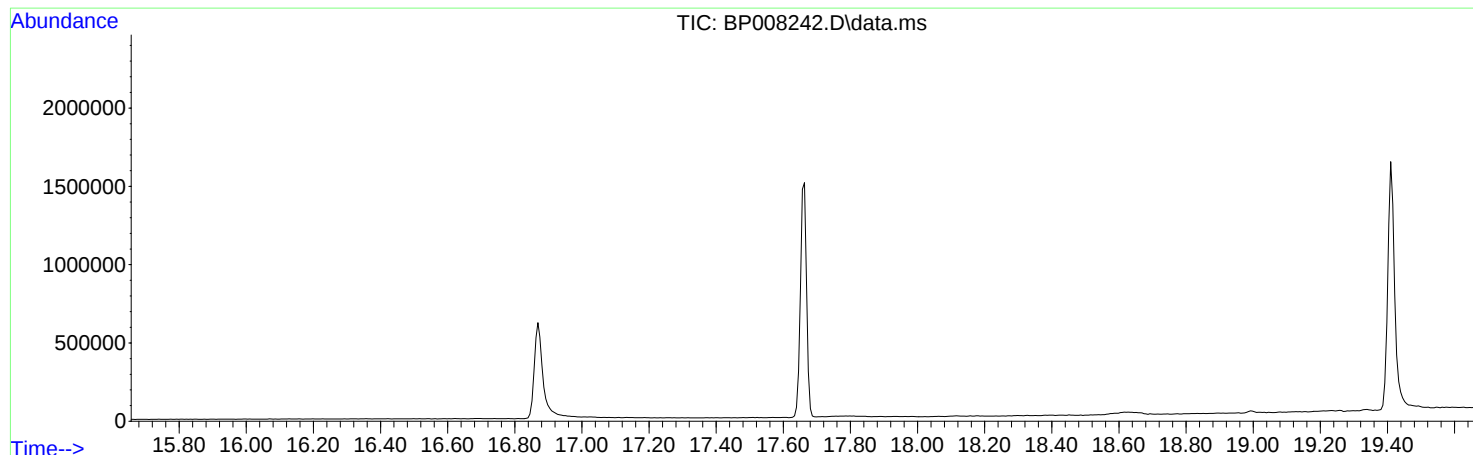




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	49743	PASS
68	69	0.00	2	2.0	990	PASS
69	198	0.00	100	35.3	50632	PASS
70	69	0.00	2	0.6	310	PASS
127	198	10	80	40.1	57420	PASS
197	198	0.00	2	0.3	409	PASS
198	198	100	100	100.0	143259	PASS
199	198	5	9	6.9	9888	PASS
275	198	10	60	28.7	41092	PASS
365	198	1	100	3.8	5483	PASS
441	198	0.01	100	13.9	19984	PASS
442	442	100	100	100.0	125832	PASS
443	442	15	24	20.3	25558	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120721\
 Data File : BP008242.D
 Acq On : 07 Dec 2021 09:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 08 09:13:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 03 14:39:24 2021
 Response via : Initial Calibration

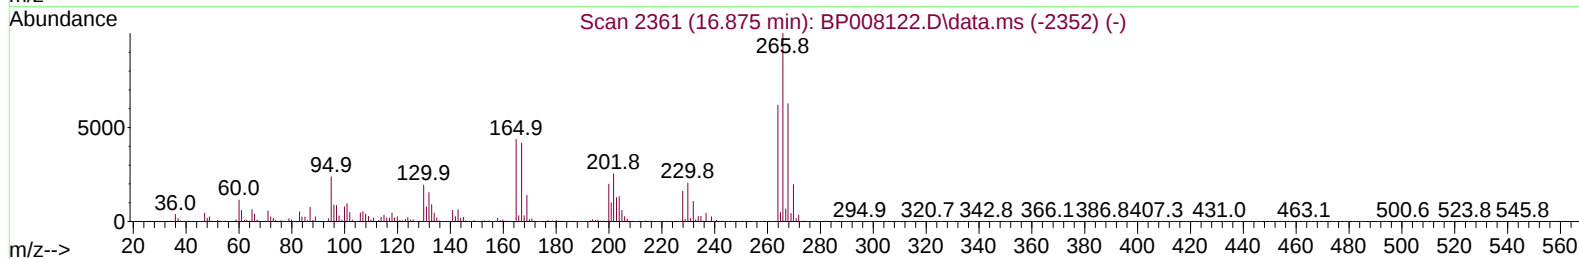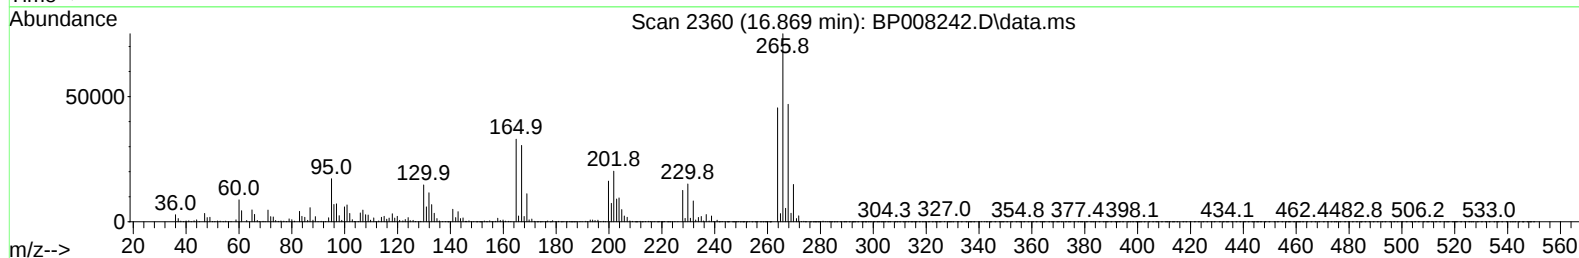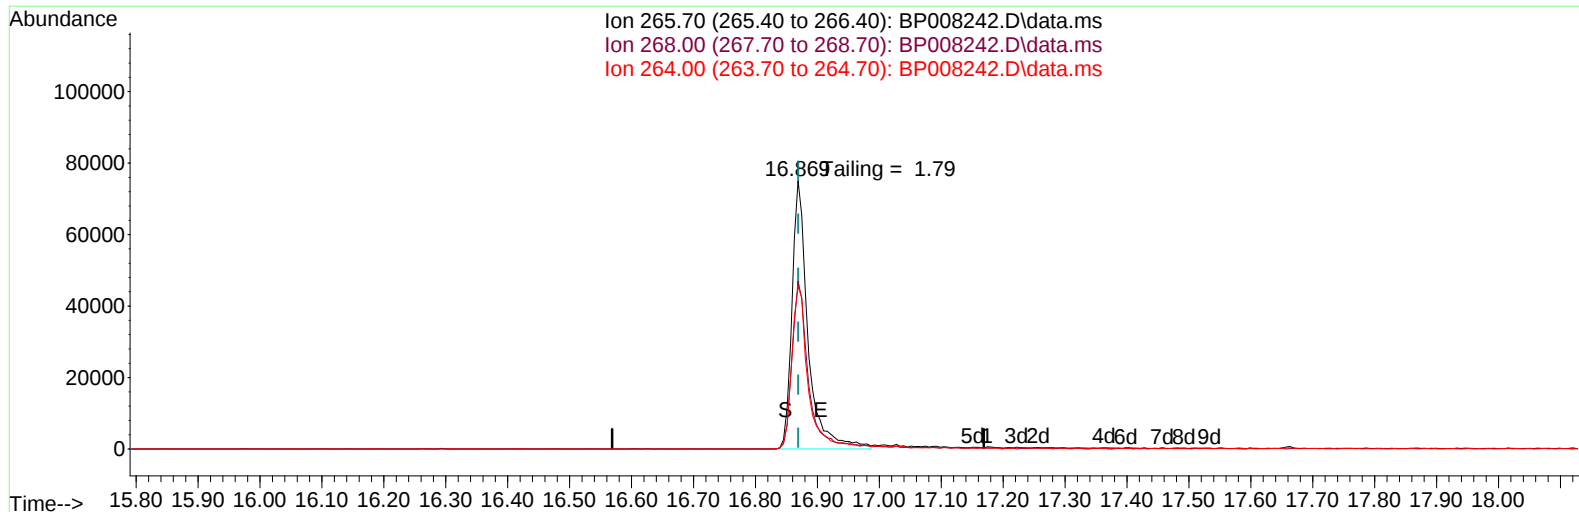

TIC: BP008242.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.000) 347341.49 ng m




response 142392

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.51
264.00	61.90	60.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120721\
 Data File : BP008242.D
 Acq On : 07 Dec 2021 09:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 08 09:13:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 03 14:39:24 2021
 Response via : Initial Calibration

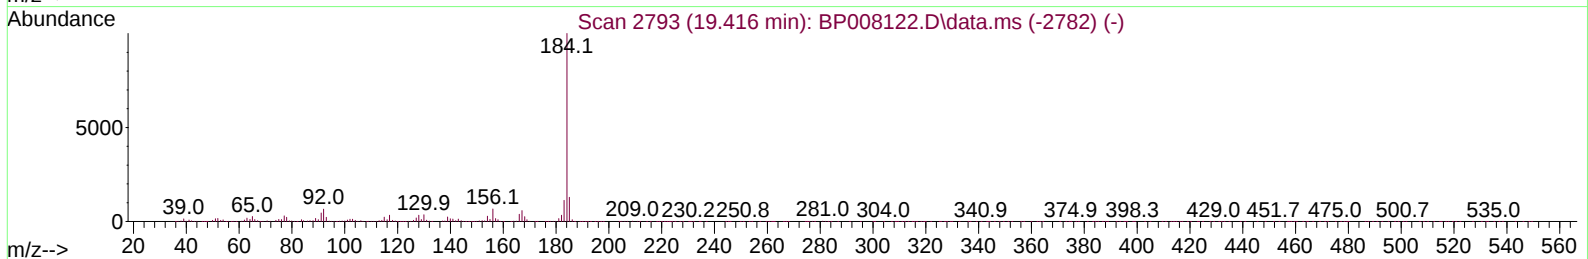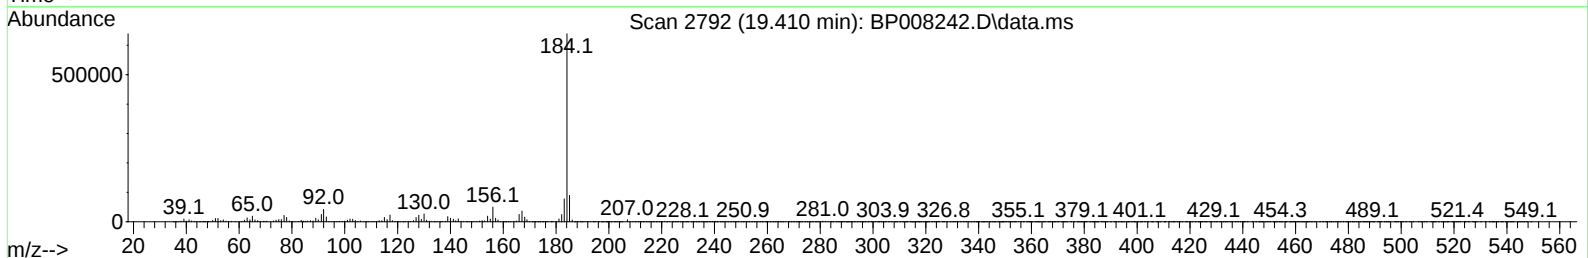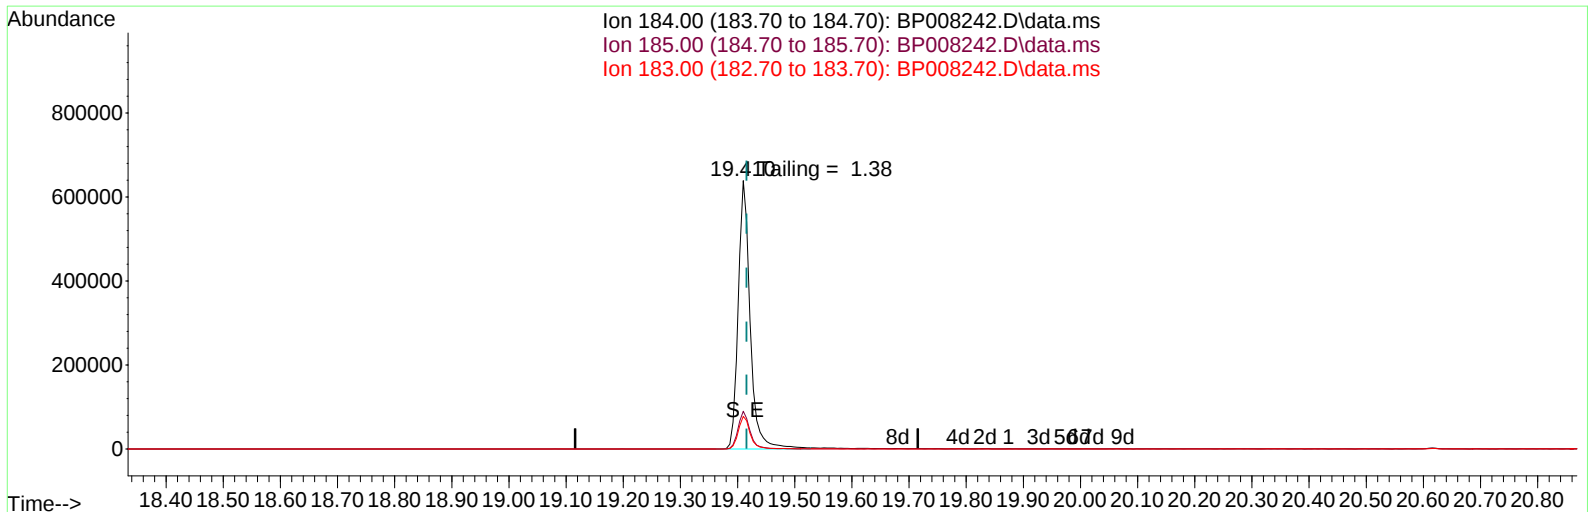

TIC: BP008242.D\data.ms

(77) Benzidine

19.410min (-0.006) 487039.19 ng m

response 948677

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.06
183.00	11.40	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2021	BNA_P	BP008242.D
Compound Name	Response	Retention Time
DDT	516929	20.616
DDD	16861	20.186
DDE	1955	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18816	535745	3.51

Instrument :
BNA_P
ClientSampleId :
DFTPP