
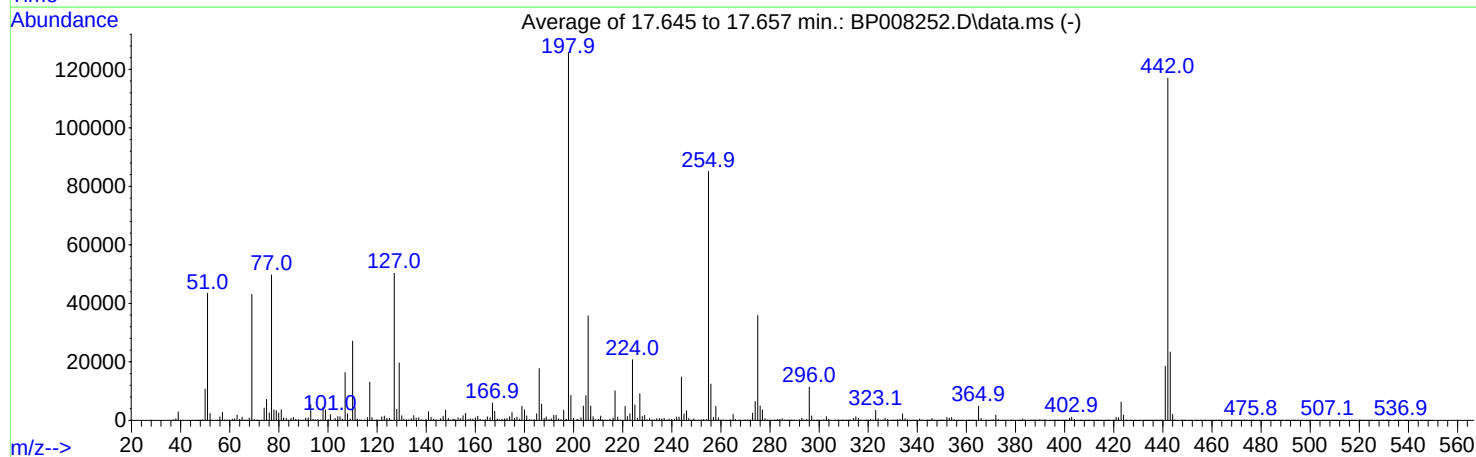


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120721\
 Data File : BP008252.D
 Acq On : 07 Dec 2021 16:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 03 14:39:24 2021

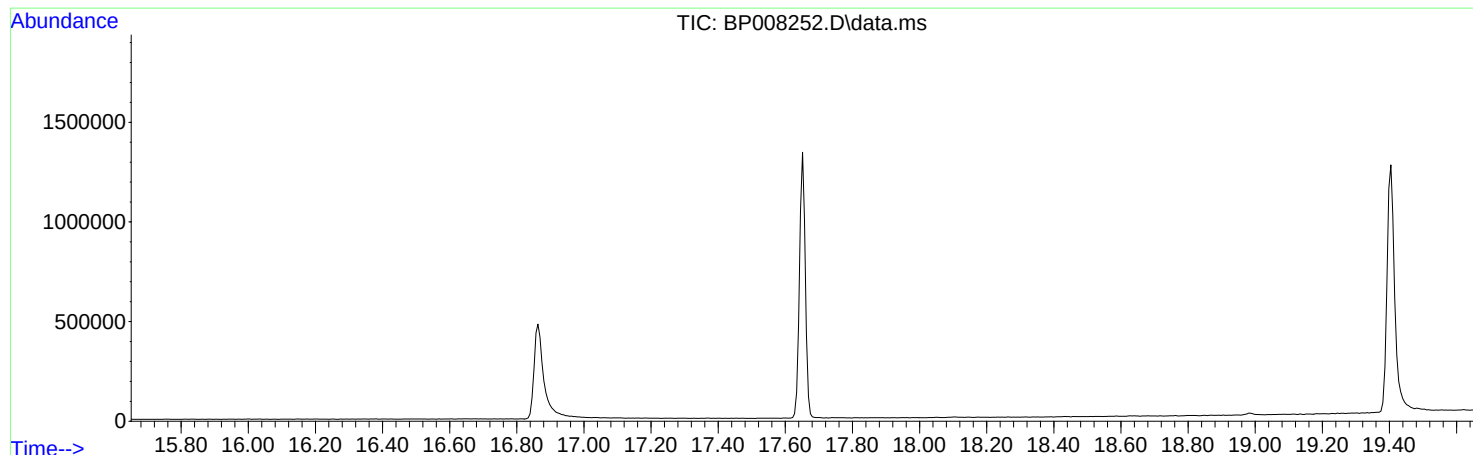




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	43434	PASS
68	69	0.00	2	1.9	837	PASS
69	198	0.00	100	34.3	43109	PASS
70	69	0.00	2	0.6	248	PASS
127	198	10	80	40.0	50318	PASS
197	198	0.00	2	0.2	304	PASS
198	198	100	100	100.0	125765	PASS
199	198	5	9	6.8	8514	PASS
275	198	10	60	28.5	35830	PASS
365	198	1	100	3.9	4890	PASS
441	198	0.01	100	14.7	18485	PASS
442	442	100	100	100.0	117008	PASS
443	442	15	24	20.0	23384	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120721\
Data File : BP008252.D
Acq On : 07 Dec 2021 16:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 08 09:13:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 03 14:39:24 2021
Response via : Initial Calibration

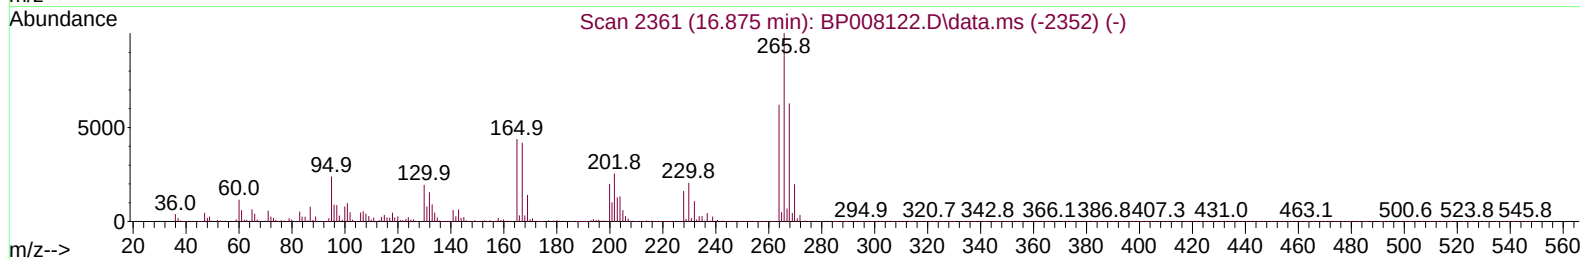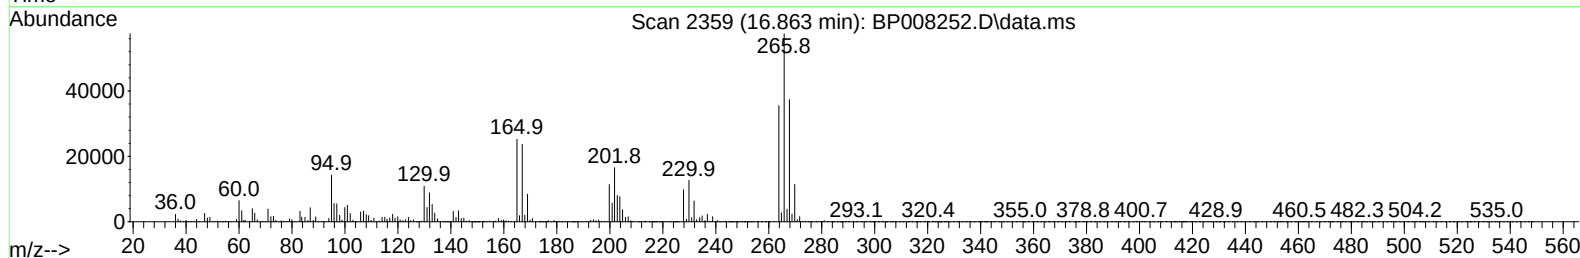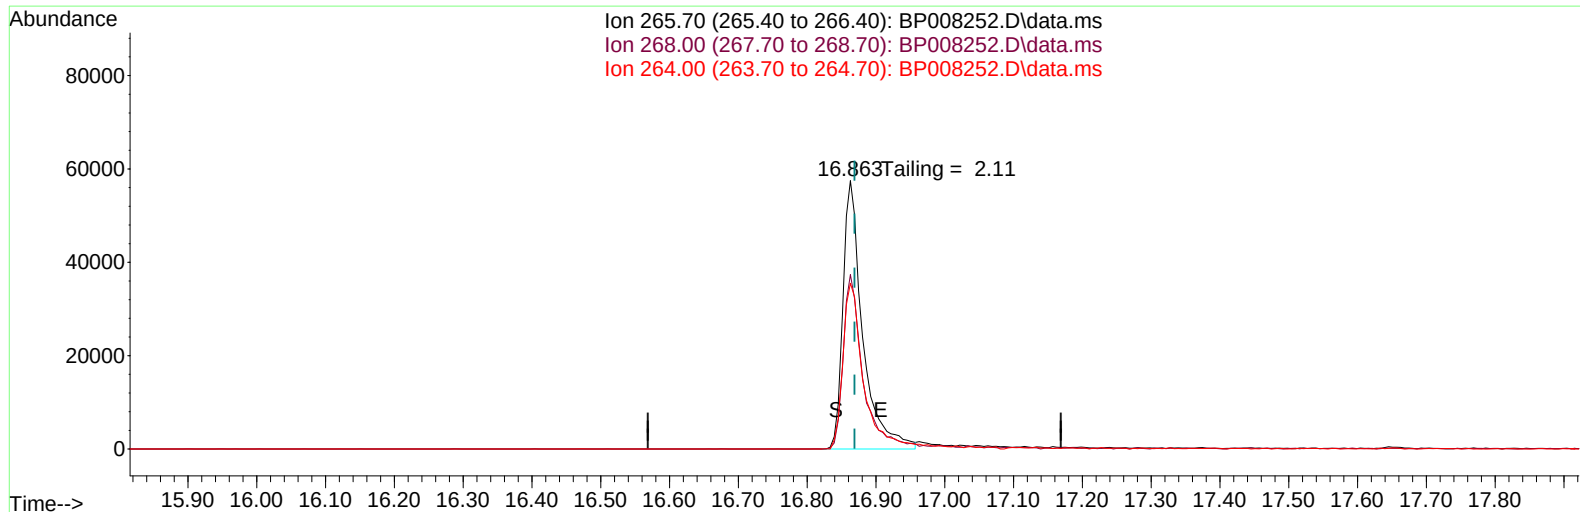

TIC: BP008252.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.006) 354506.68 ng




response 70159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.96
264.00	61.90	61.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120721\
 Data File : BP008252.D
 Acq On : 07 Dec 2021 16:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 08 09:13:08 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 03 14:39:24 2021
 Response via : Initial Calibration

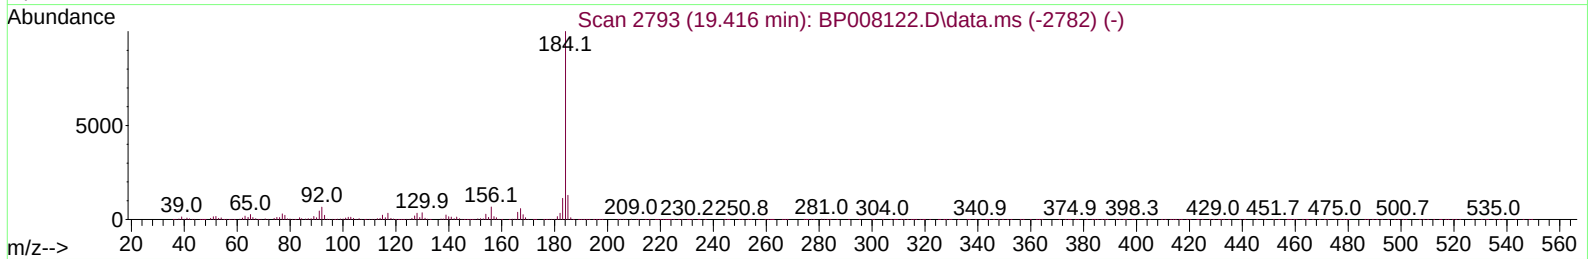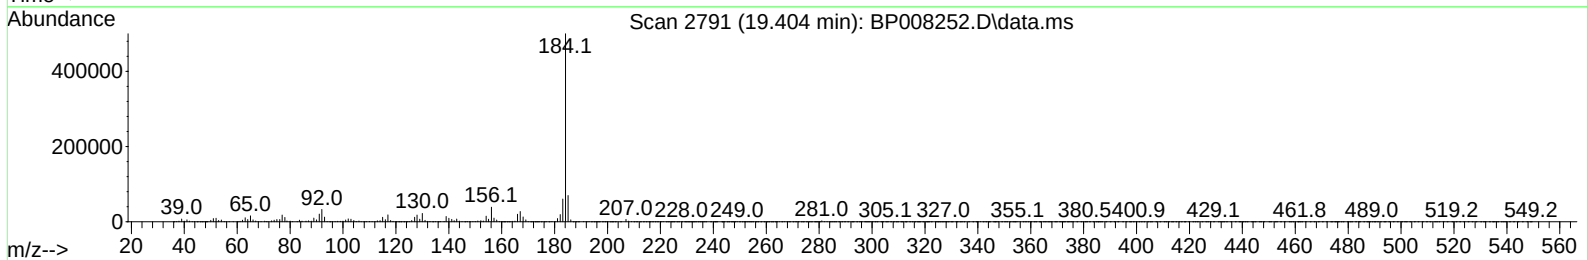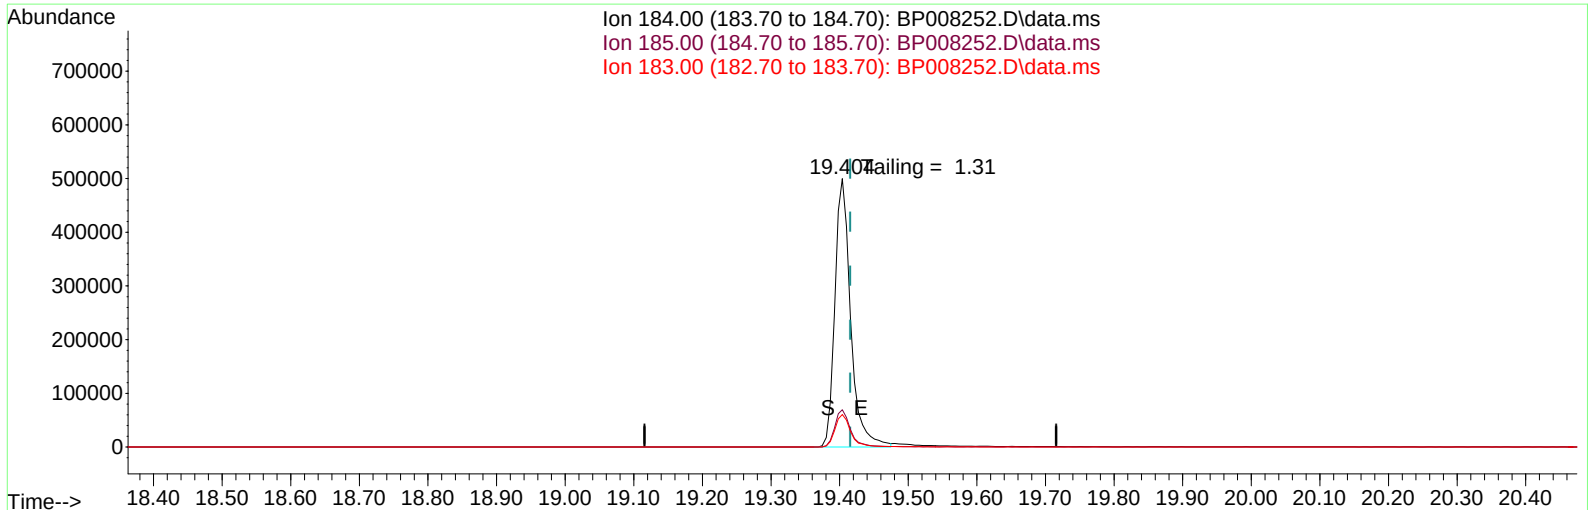

TIC: BP008252.D\data.ms

(77) Benzidine

19.404min (-0.012) 653778.40 ng m

response 798154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.93
183.00	11.40	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/7/2021	BNA_P	BP008252.D
Compound Name	Response	Retention Time
DDT	436875	20.61
DDD	12972	20.18
DDE	1392	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14364	451239	3.18

Instrument :
BNA_P
ClientSampleId :
DFTPP