

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018678.D
 Acq On : 07 Dec 2023 18:01
 Operator : MA/JU
 Sample : 05459-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Quant Time: Dec 07 21:39:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	215700	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.640	136	806479	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.475	164	524757	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.222	188	1288940	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	1466660	20.000	ng/ul	0.00
88) Perylene-d12	23.680	264	1755055	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	4573	0.722	ng/uL	0.00
4) Pyridine-d5	3.693	84	16914	0.998	ng/ul	0.00
7) Phenol-d5	7.010	99	72887	3.367	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.181	67	50477	3.934	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.375	132	60290	3.569	ng/ul	-0.01
15) 4-Methylphenol-d8	8.557	113	32111	1.833	ng/ul	-0.01
21) Nitrobenzene-d5	9.004	128	28607	3.985	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.728	143	28261	3.798	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.263	165	52679	3.462	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.781	131	46700	2.348	ng/ul	-0.01
46) Dimethylphthalate-d6	13.887	166	203717	4.350	ng/ul	-0.02
49) Acenaphthylene-d8	14.169	160	206488	4.004	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.681	143	15512	2.018	ng/ul	0.00
60) Fluorene-d10	15.469	176	182589	4.644	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	12400	1.604	ng/ul	-0.01
73) Anthracene-d10	17.322	188	281948	4.161	ng/ul	0.00
81) Pyrene-d10	19.557	212	417245	3.655	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.521	264	426331	4.166	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.669	105	98304	3.765	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018678.D
Acq On : 07 Dec 2023 18:01
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Time: Dec 07 21:39:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

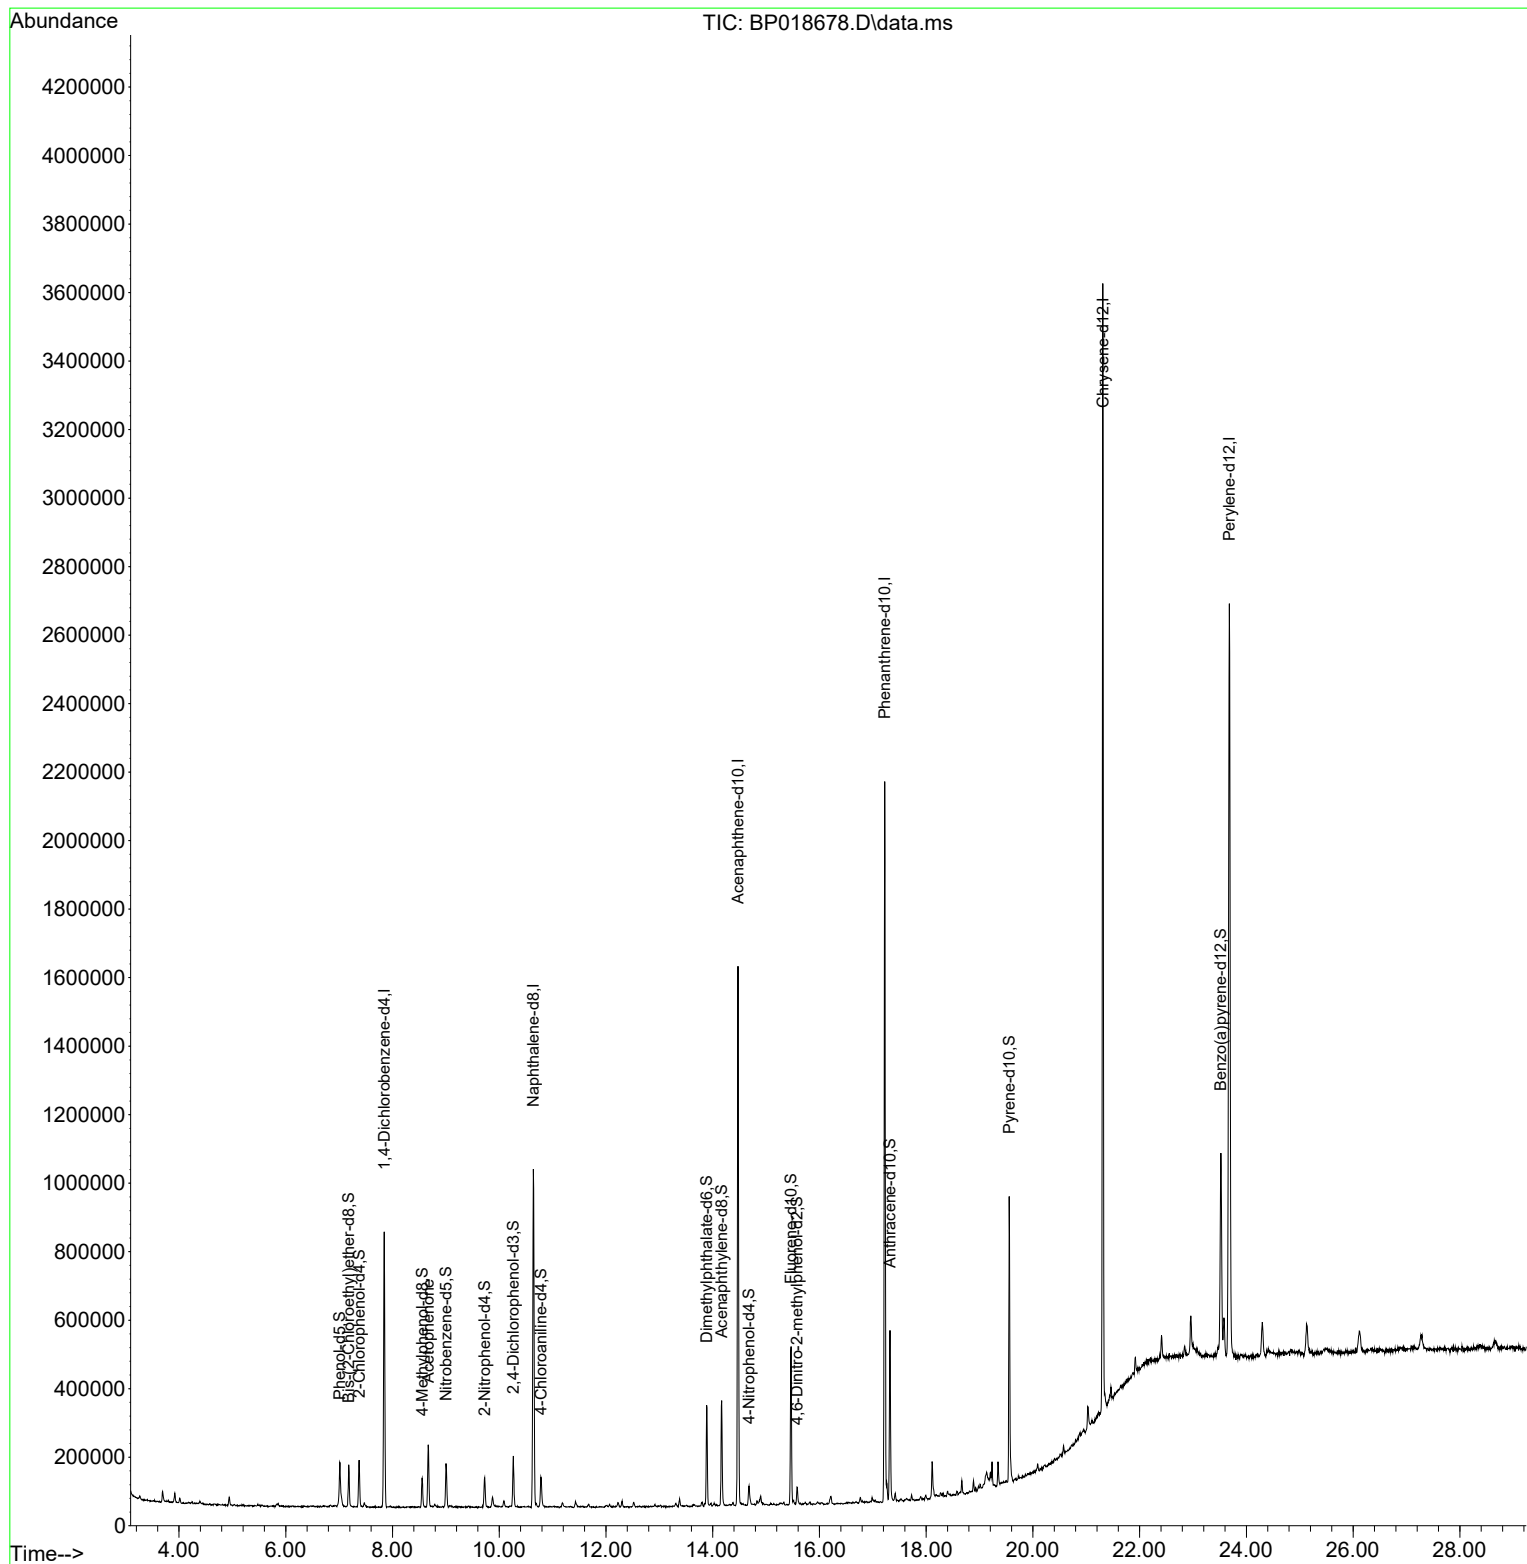

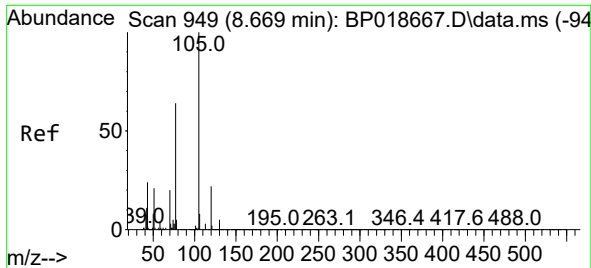

#16
Acetophenone
Concen: 3.765 ng/ul
RT: 8.669 min Scan# 94
Delta R.T. -0.012 min
Lab File: BP018678.D
Acq: 07 Dec 2023 18:01

Instrument :
BNA_P
ClientSampleId :
C0AA3

Tgt Ion:	105	Resp:	98304
Ion Ratio	Lower	Upper	
105	100		
77	74.5	59.4	89.0
51	25.8	19.4	29.0

