

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018681.D
 Acq On : 07 Dec 2023 19:43
 Operator : MA/JU
 Sample : 05459-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ7

Quant Time: Dec 07 21:40:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	281102	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.640	136	1092579	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.475	164	692575	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.222	188	1653468	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	1791410	20.000	ng/ul	0.00
88) Perylene-d12	23.680	264	2079450	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	7474	0.906	ng/uL	0.00
4) Pyridine-d5	3.693	84	22557	1.021	ng/ul	0.00
7) Phenol-d5	7.010	99	84631	3.000	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.181	67	58289	3.486	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.375	132	72762	3.306	ng/ul	-0.01
15) 4-Methylphenol-d8	8.557	113	37956	1.663	ng/ul	-0.01
21) Nitrobenzene-d5	9.004	128	41156	4.232	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.722	143	40186	3.986	ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	10.263	165	79835	3.873	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.781	131	61879	2.297	ng/ul	-0.01
46) Dimethylphthalate-d6	13.892	166	304270	4.922	ng/ul	-0.01
49) Acenaphthylene-d8	14.169	160	315572	4.636	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.681	143	25460	2.509	ng/ul	0.00
60) Fluorene-d10	15.469	176	280245	5.401	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.586	200	18752	1.891	ng/ul	0.00
73) Anthracene-d10	17.322	188	438212	5.041	ng/ul	0.00
81) Pyrene-d10	19.557	212	654757	4.695	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.521	264	634361	5.232	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.669	105	139319	4.095	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018681.D
Acq On : 07 Dec 2023 19:43
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7


Quant Time: Dec 07 21:40:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

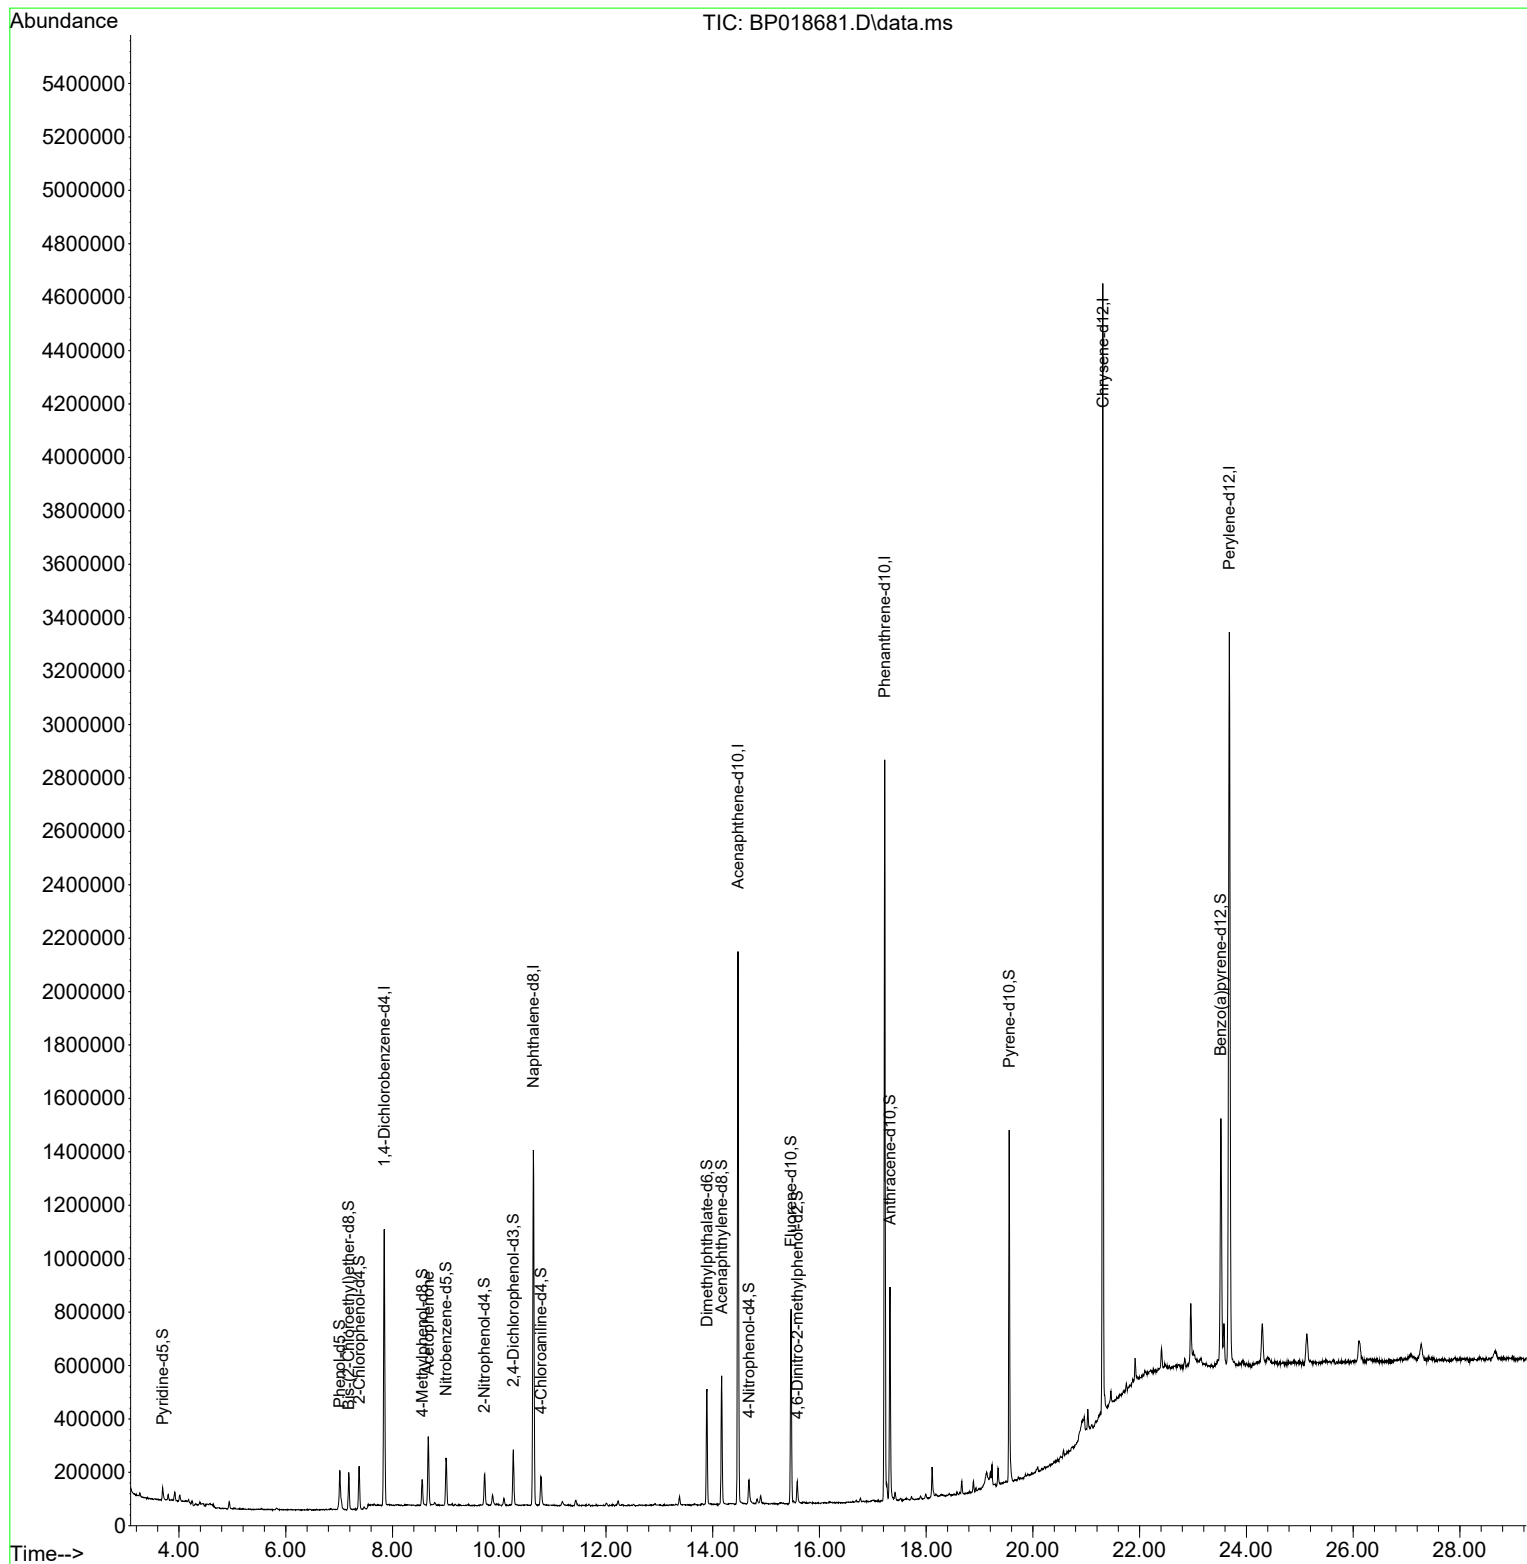

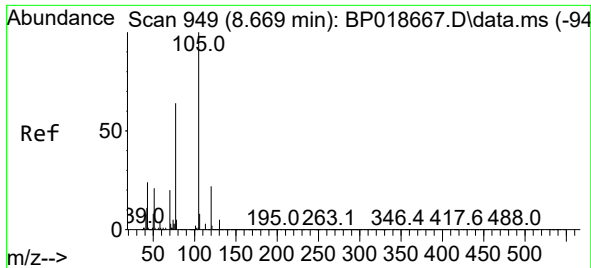

#16
 Acetophenone
 Concen: 4.095 ng/ul
 RT: 8.669 min Scan# 94
 Delta R.T. -0.012 min
 Lab File: BP018681.D
 Acq: 07 Dec 2023 19:43

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ7

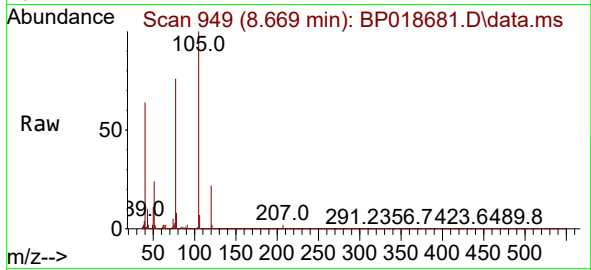

Tgt Ion:	105	Resp:	139319
Ion	Ratio	Lower	Upper
105	100		
77	75.9	59.4	89.0
51	24.2	19.4	29.0

