

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018689.D
 Acq On : 08 Dec 2023 00:15
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Quant Time: Dec 08 00:58:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	601001	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.640	136	2266538	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.475	164	1404361	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.222	188	3307742	20.000	ng/u1	0.00
79) Chrysene-d12	21.310	240	3755773	20.000	ng/u1	0.00
88) Perylene-d12	23.686	264	4503186	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	10755	0.610	ng/uL	0.00
4) Pyridine-d5	3.687	84	41807	0.885	ng/u1	0.00
7) Phenol-d5	7.011	99	130314	2.161	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.181	67	102435	2.866	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.375	132	116765	2.481	ng/u1	-0.01
15) 4-Methylphenol-d8	8.558	113	55102	1.129	ng/u1	-0.01
21) Nitrobenzene-d5	9.005	128	57717	2.861	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.728	143	56173	2.686	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.263	165	109098	2.551	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.781	131	118379	2.118	ng/u1	-0.01
46) Dimethylphthalate-d6	13.893	166	372132	2.969	ng/u1	-0.01
49) Acenaphthylene-d8	14.169	160	412642	2.990	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.681	143	25593	1.244	ng/u1	0.00
60) Fluorene-d10	15.463	176	344742	3.277	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.581	200	19055	0.961	ng/u1	-0.01
73) Anthracene-d10	17.322	188	536217	3.084	ng/u1	0.00
81) Pyrene-d10	19.557	212	789458	2.700	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.522	264	821908	3.130	ng/u1	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.669	105	119439	1.642	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018689.D
Acq On : 08 Dec 2023 00:15
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6


Quant Time: Dec 08 00:58:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

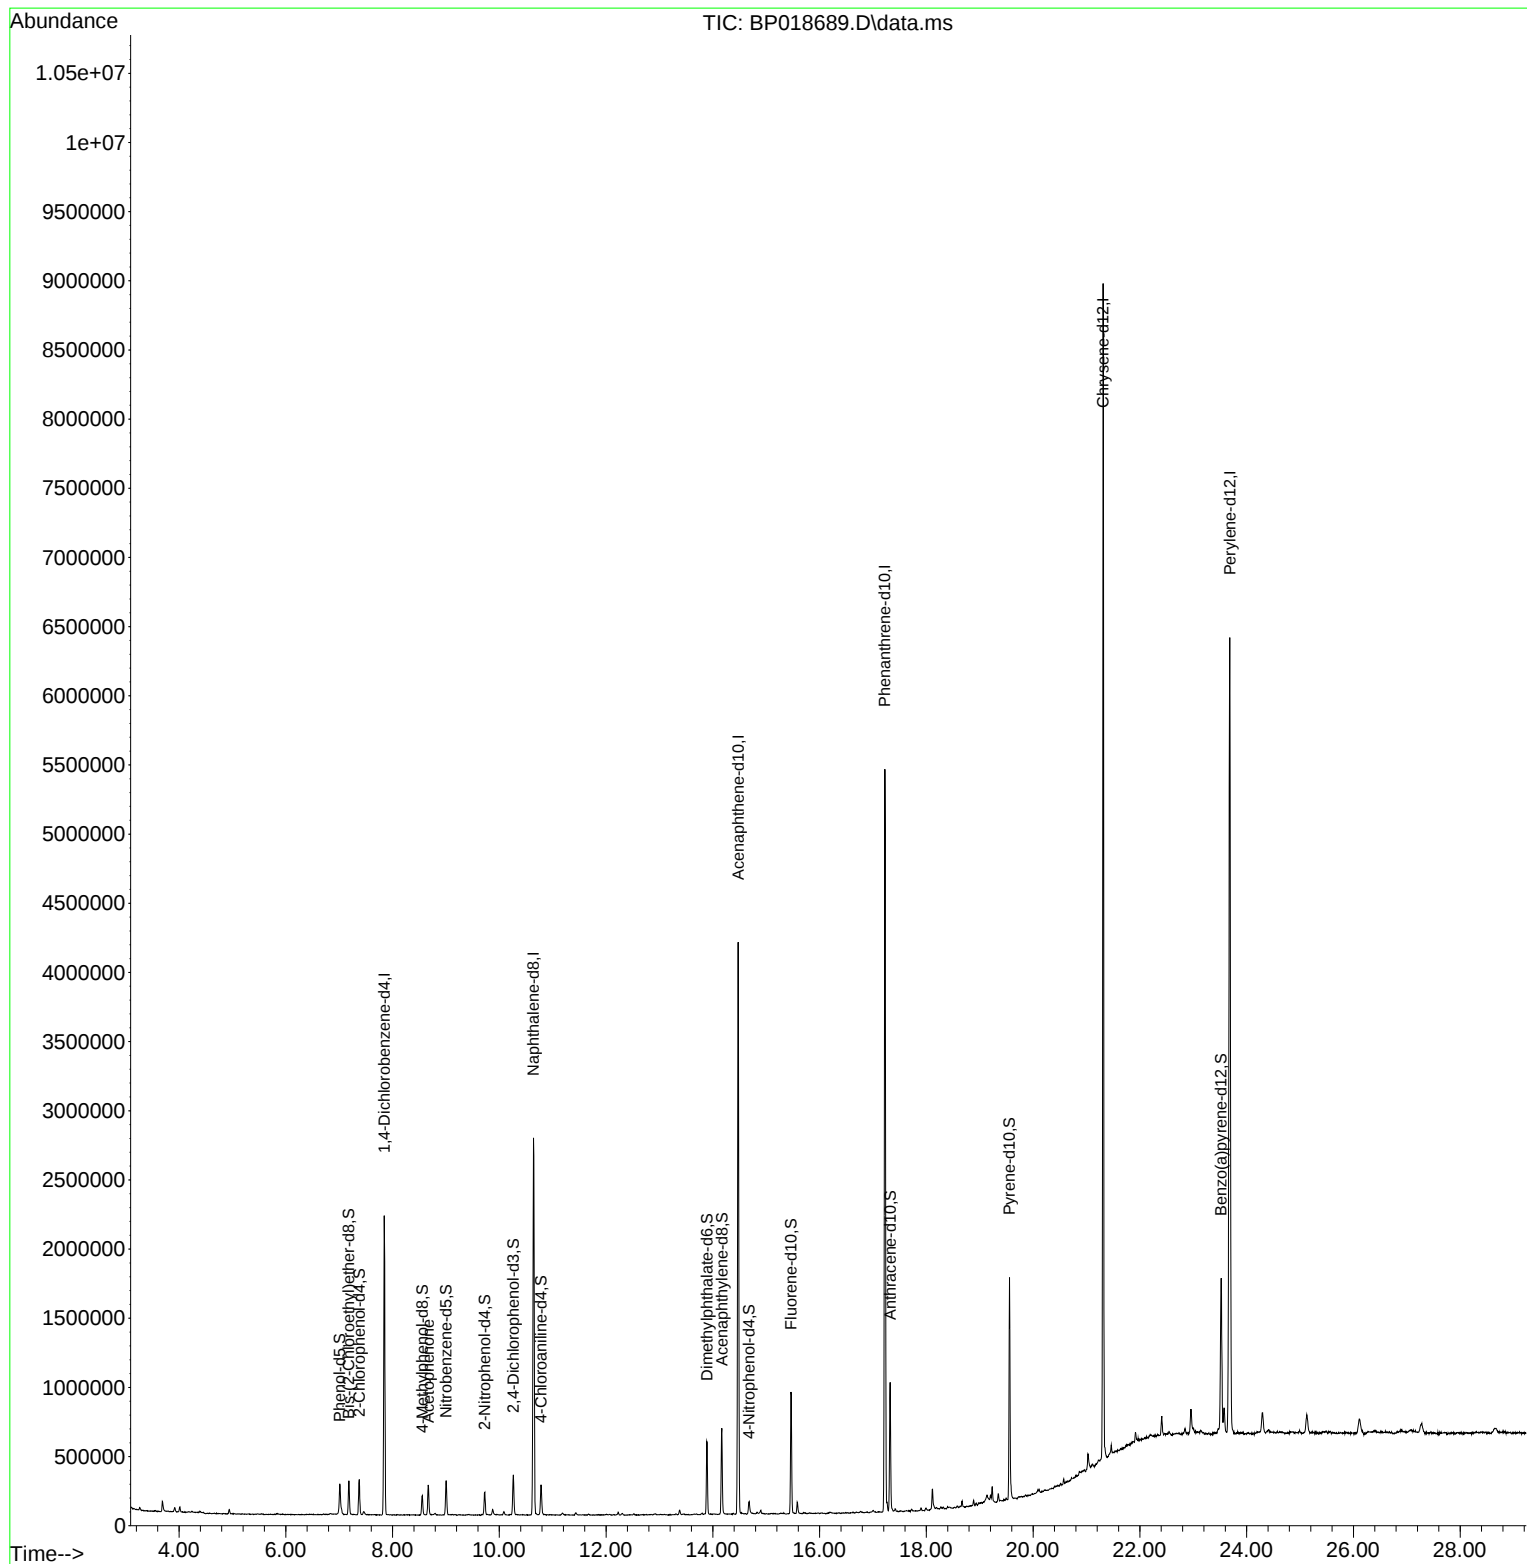

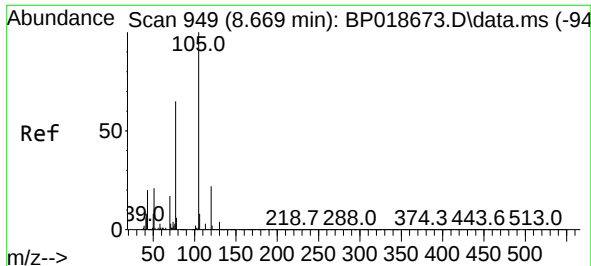

#16
Acetophenone
Concen: 1.642 ng/ul
RT: 8.669 min Scan# 94
Delta R.T. -0.012 min
Lab File: BP018689.D
Acq: 08 Dec 2023 00:15

Instrument :
BNA_P
ClientSampleId :
C0AA6

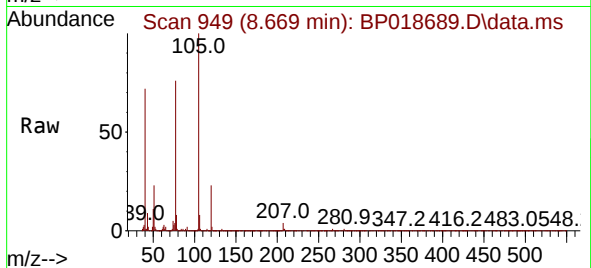

Tgt Ion:105 Resp: 119439
Ion Ratio Lower Upper
105 100
77 76.4 59.4 89.0
51 23.3 19.4 29.0

