

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018697.D
 Acq On : 08 Dec 2023 05:19
 Operator : MA/JU
 Sample : 05459-13
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ8

Quant Time: Dec 08 05:51:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	183861	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.640	136	700500	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.475	164	556745	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.222	188	1352631	20.000	ng/u1	0.00
79) Chrysene-d12	21.310	240	1497352	20.000	ng/u1	0.00
88) Perylene-d12	23.680	264	1711597	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	17195	3.187	ng/uL	0.00
4) Pyridine-d5	3.687	84	175147	12.119	ng/u1	0.00
7) Phenol-d5	7.011	99	200552	10.869	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.181	67	124612	11.395	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.375	132	164406	11.419	ng/u1	-0.01
15) 4-Methylphenol-d8	8.558	113	85684	5.738	ng/u1	-0.01
21) Nitrobenzene-d5	9.005	128	77732	12.468	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.728	143	79130	12.242	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.263	165	155620	11.774	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.781	131	126552	7.326	ng/u1	-0.01
46) Dimethylphthalate-d6	13.887	166	639947	12.879	ng/u1	-0.02
49) Acenaphthylene-d8	14.169	160	711268	12.999	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.675	143	84095	10.310	ng/u1	-0.01
60) Fluorene-d10	15.463	176	594296	14.248	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.587	200	42368	5.224	ng/u1	0.00
73) Anthracene-d10	17.322	188	925098	13.009	ng/u1	0.00
81) Pyrene-d10	19.557	212	1384918	11.882	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.522	264	1376287	13.791	ng/u1	-0.01
Target Compounds						
					Qvalue	
8) Phenol	7.040	94	21548	1.191	ng/u1	92
16) Acetophenone	8.669	105	94412	4.243	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018697.D
Acq On : 08 Dec 2023 05:19
Operator : MA/JU
Sample : 05459-13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ8

Quant Time: Dec 08 05:51:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration




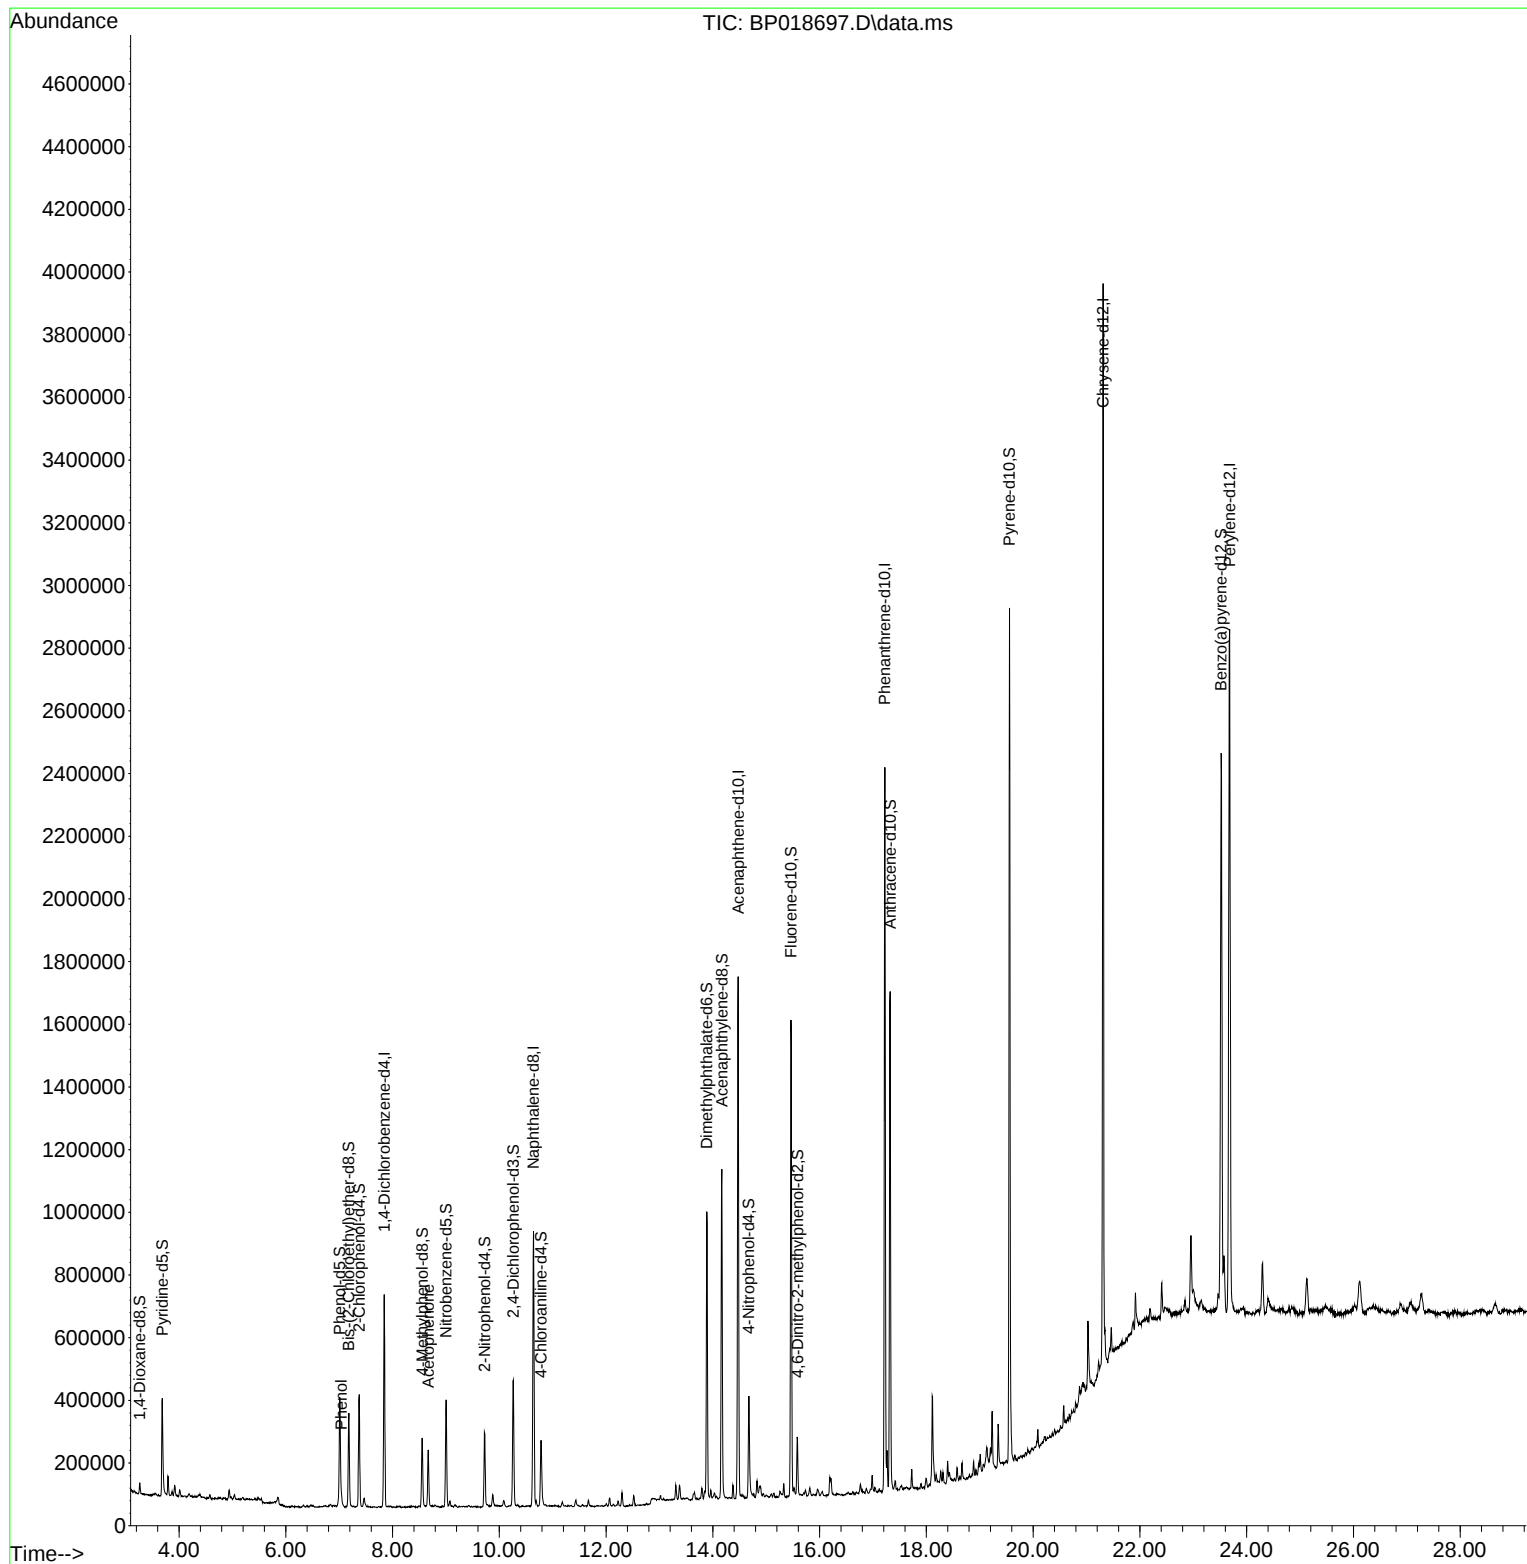


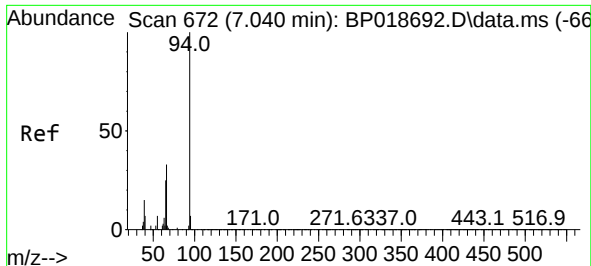

#8
Phenol
Concen: 1.191 ng/ul
RT: 7.040 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP018697.D
Acq: 08 Dec 2023 05:19

Instrument :
BNA_P
ClientSampleId :
C0AJ8

Tgt Ion: 94 Resp: 21548
Ion Ratio Lower Upper
94 100
65 30.5 21.0 31.6
66 40.0 28.6 43.0

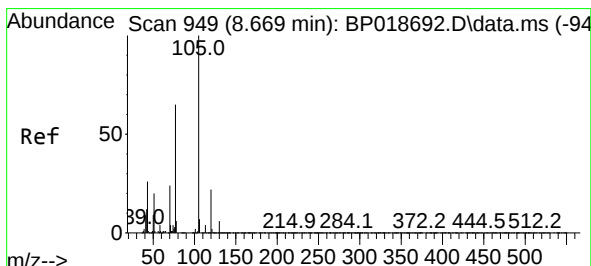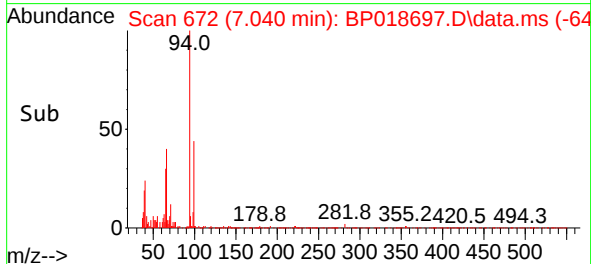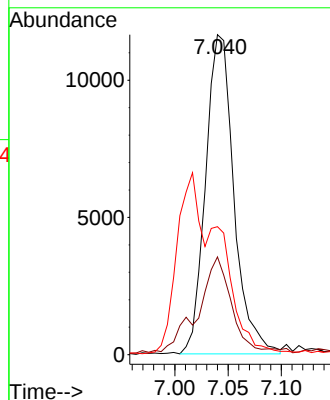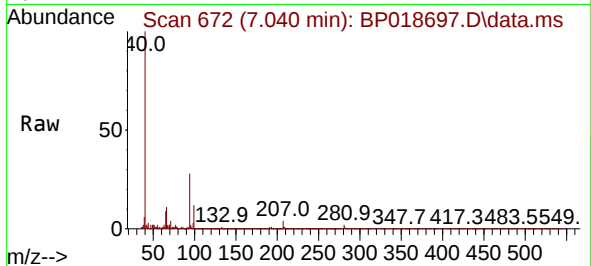

#16
Acetophenone
Concen: 4.243 ng/ul
RT: 8.669 min Scan# 949
Delta R.T. -0.012 min
Lab File: BP018697.D
Acq: 08 Dec 2023 05:19

Tgt Ion: 105 Resp: 94412
Ion Ratio Lower Upper
105 100
77 75.5 59.4 89.0
51 23.5 19.4 29.0

