

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018709.D
 Acq On : 08 Dec 2023 13:14
 Operator : MA/JU
 Sample : 05459-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Quant Time: Dec 08 14:39:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	188423	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.640	136	710078	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.475	164	434174	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.222	188	1066804	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	1173641	20.000	ng/ul	0.00
88) Perylene-d12	23.674	264	1351648	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	4603	0.832	ng/uL	0.00
4) Pyridine-d5	3.693	84	14376	0.971	ng/ul	0.00
7) Phenol-d5	7.010	99	166767	8.819	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.181	67	98637	8.801	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.375	132	123900	8.397	ng/ul	-0.01
15) 4-Methylphenol-d8	8.552	113	108260	7.075	ng/ul	-0.02
21) Nitrobenzene-d5	9.004	128	58391	9.239	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.722	143	57540	8.782	ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	10.263	165	117362	8.760	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.781	131	147473	8.422	ng/ul	-0.01
46) Dimethylphthalate-d6	13.887	166	370524	9.562	ng/ul	-0.02
49) Acenaphthylene-d8	14.169	160	427571	10.021	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.675	143	47580	7.480	ng/ul	-0.01
60) Fluorene-d10	15.463	176	354699	10.905	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.581	200	29322	4.584	ng/ul	-0.01
73) Anthracene-d10	17.322	188	588973	10.502	ng/ul	0.00
81) Pyrene-d10	19.557	212	804294	8.804	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.521	264	812990	10.316	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.669	105	78132	3.426	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018709.D
Acq On : 08 Dec 2023 13:14
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Time: Dec 08 14:39:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

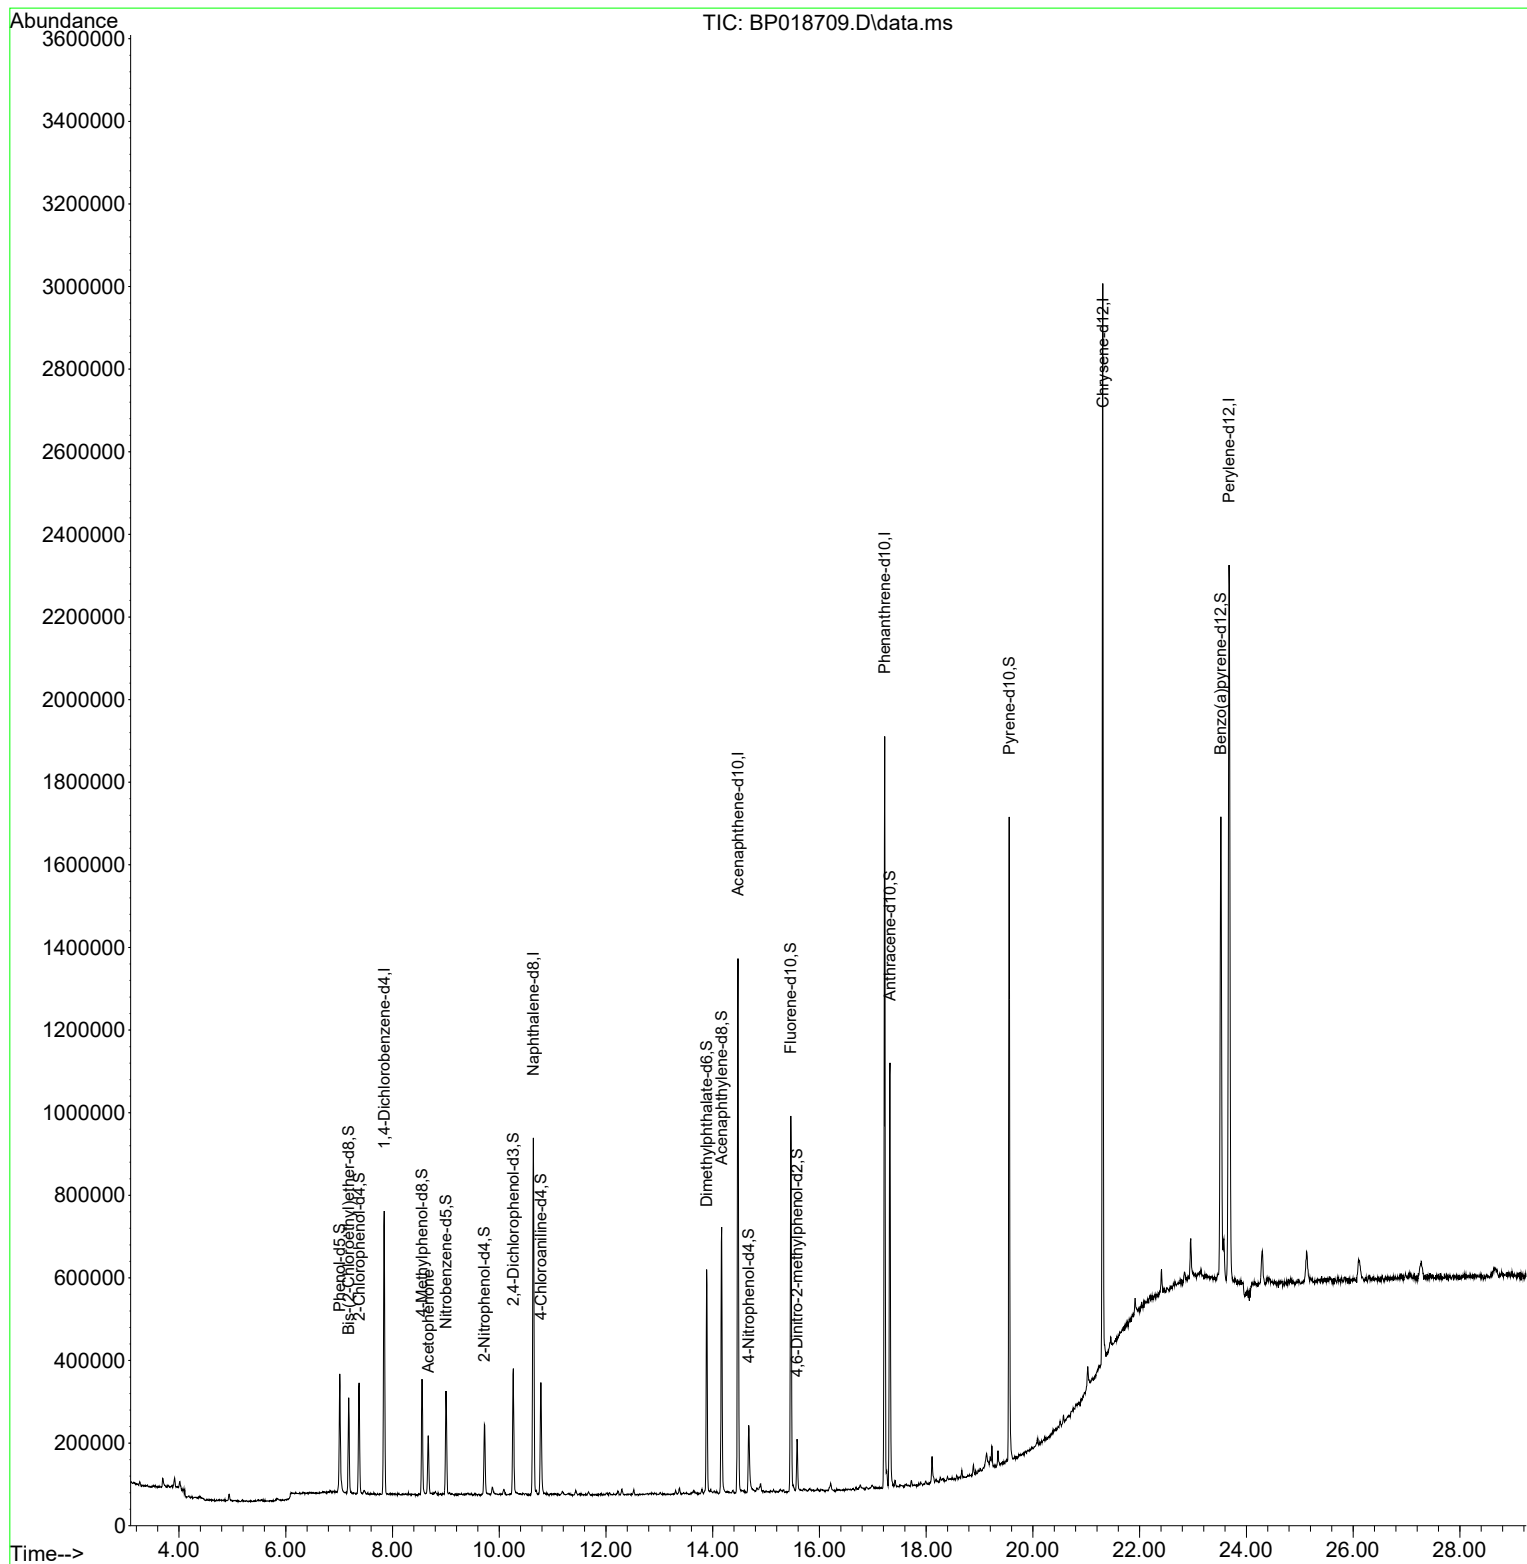

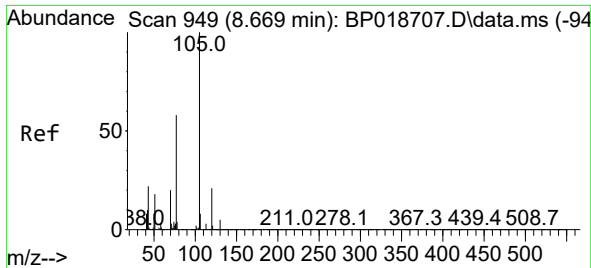

#16
 Acetophenone
 Concen: 3.426 ng/ul
 RT: 8.669 min Scan# 94
 Delta R.T. -0.012 min
 Lab File: BP018709.D
 Acq: 08 Dec 2023 13:14

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Tgt Ion:105 Resp: 78132
 Ion Ratio Lower Upper
 105 100
 77 74.1 59.4 89.0
 51 23.2 19.4 29.0

