

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018713.D
 Acq On : 08 Dec 2023 15:30
 Operator : MA/JU
 Sample : 05459-16
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Quant Time: Dec 08 16:44:51 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	120441	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.640	136	447383	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.475	164	280917	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.222	188	703107	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	830396	20.000	ng/ul	0.00
88) Perylene-d12	23.680	264	989491	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	4107	1.162	ng/uL	0.00
4) Pyridine-d5	3.693	84	18686	1.974	ng/ul	0.00
7) Phenol-d5	7.011	99	103612	8.572	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.181	67	73429	10.250	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.375	132	84754	8.987	ng/ul	-0.01
15) 4-Methylphenol-d8	8.552	113	56907	5.818	ng/ul	-0.02
21) Nitrobenzene-d5	9.005	128	43023	10.805	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.722	143	43097	10.440	ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	10.263	165	83222	9.859	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.781	131	95823	8.686	ng/ul	-0.01
46) Dimethylphthalate-d6	13.887	166	280914	11.204	ng/ul	-0.02
49) Acenaphthylene-d8	14.163	160	324103	11.740	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.681	143	26245	6.377	ng/ul	0.00
60) Fluorene-d10	15.463	176	270677	12.862	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.587	200	18866	4.475	ng/ul	0.00
73) Anthracene-d10	17.322	188	455756	12.330	ng/ul	0.00
81) Pyrene-d10	19.557	212	641013	9.917	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.521	264	691787	11.991	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.669	105	61354	4.209	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018713.D
Acq On : 08 Dec 2023 15:30
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Time: Dec 08 16:44:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

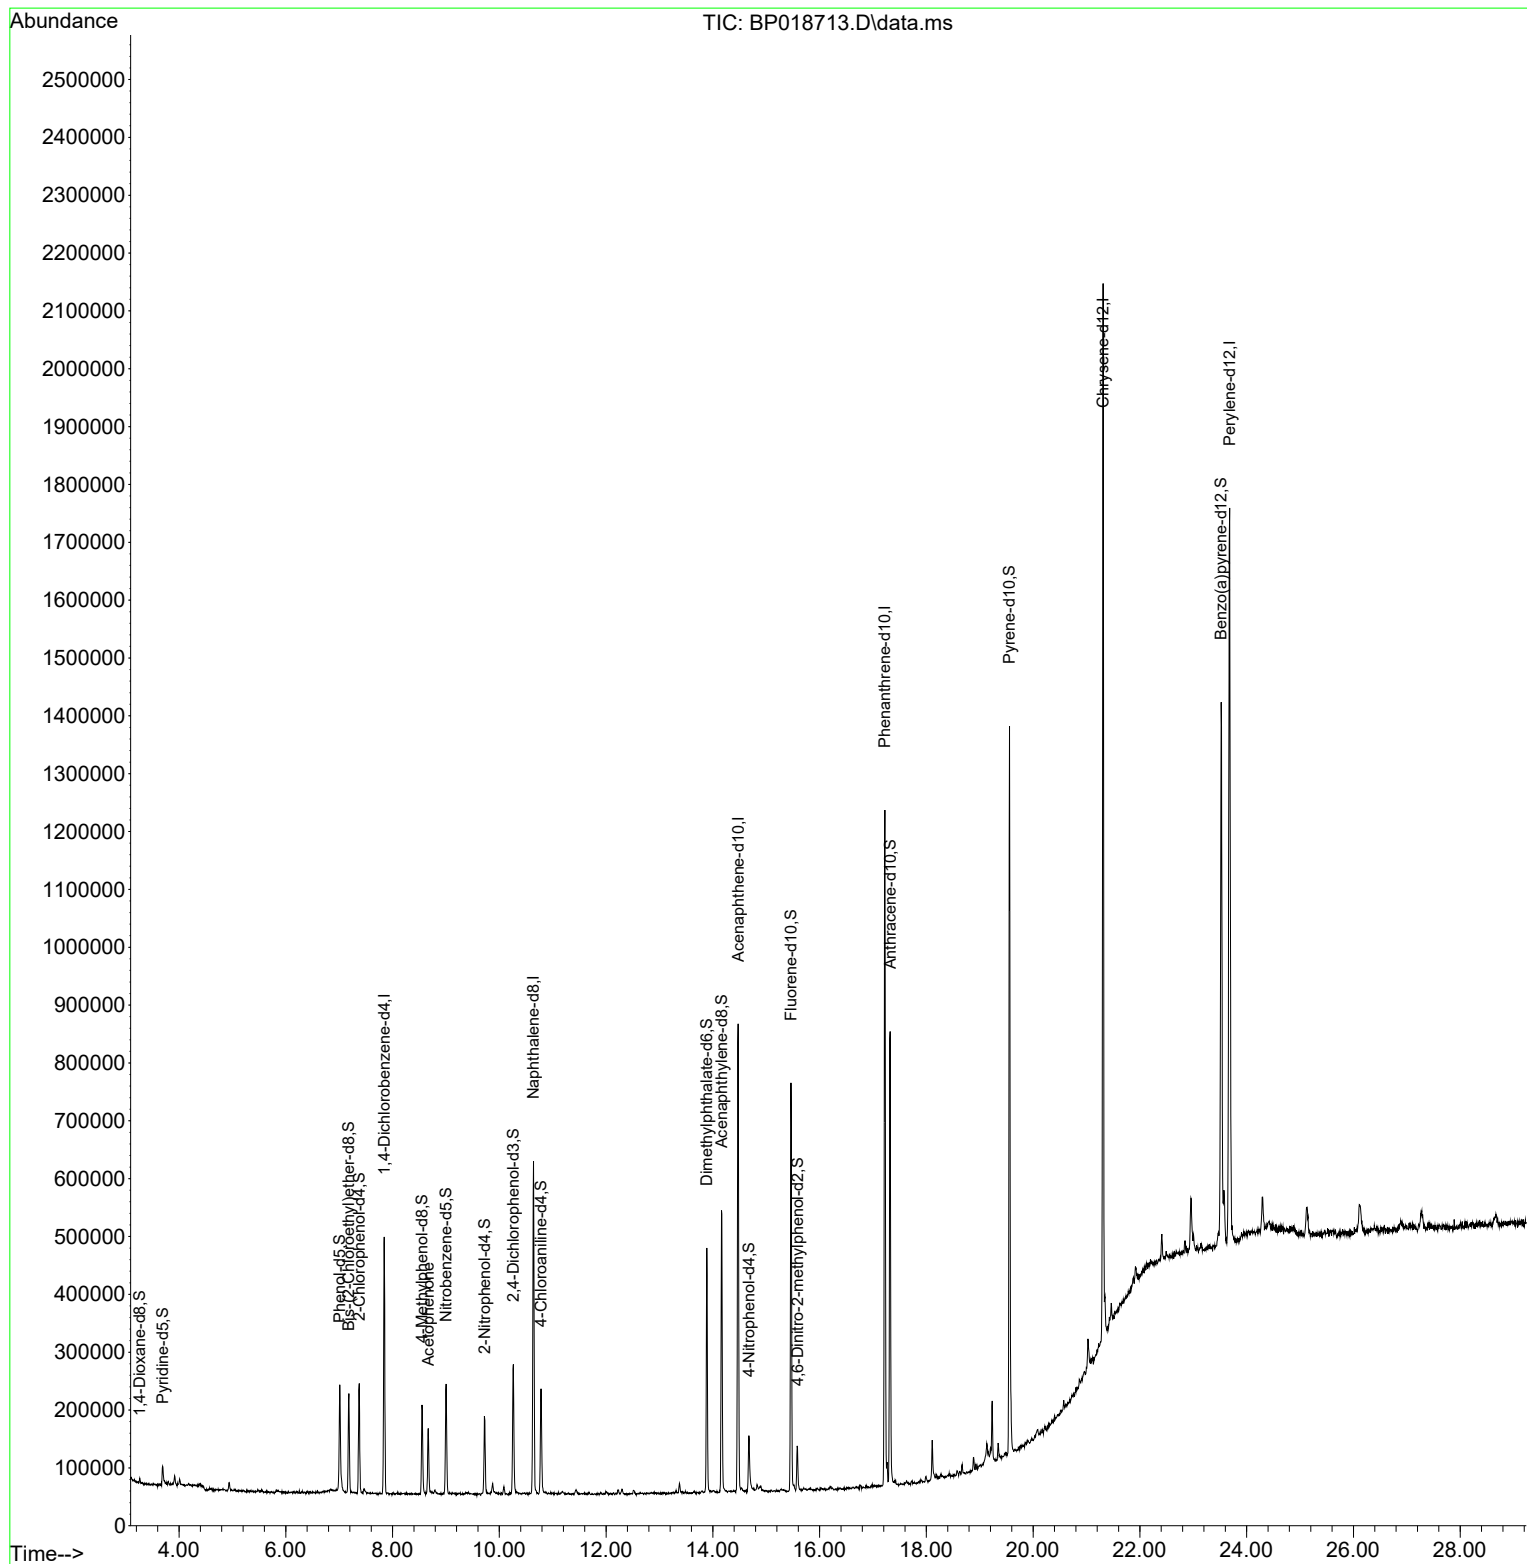

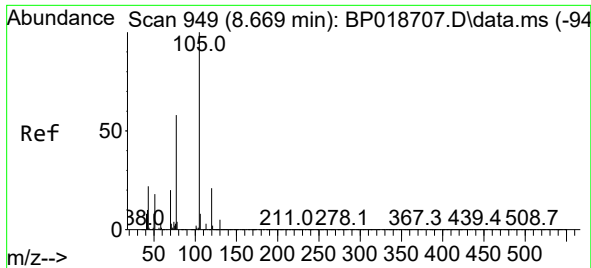

#16
Acetophenone
Concen: 4.209 ng/ul
RT: 8.669 min Scan# 94
Delta R.T. -0.012 min
Lab File: BP018713.D
Acq: 08 Dec 2023 15:30

Instrument :
BNA_P
ClientSampleId :
C0AA0

Tgt Ion:105 Resp: 61354
Ion Ratio Lower Upper
105 100
77 77.5 59.4 89.0
51 23.7 19.4 29.0

