

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018717.D
 Acq On : 08 Dec 2023 17:46
 Operator : MA/JU
 Sample : 05497-03
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Quant Time: Dec 09 02:15:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.846	152	324510	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.640	136	1199293	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.475	164	738238	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.222	188	1816109	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	2077920	20.000	ng/ul	0.00
88) Perylene-d12	23.680	264	2372832	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	8875	0.932	ng/uL	0.00
4) Pyridine-d5	3.693	84	27254	1.068	ng/ul	0.00
7) Phenol-d5	7.010	99	208884	6.414	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.181	67	141219	7.317	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.375	132	172282	6.780	ng/ul	-0.01
15) 4-Methylphenol-d8	8.557	113	79235	3.006	ng/ul	-0.01
21) Nitrobenzene-d5	9.004	128	63157	5.917	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.728	143	65618	5.929	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.263	165	157521	6.961	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.781	131	161996	5.478	ng/ul	-0.01
46) Dimethylphthalate-d6	13.887	166	503201	7.637	ng/ul	-0.02
49) Acenaphthylene-d8	14.169	160	567907	7.828	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.675	143	54379	5.028	ng/ul	-0.01
60) Fluorene-d10	15.463	176	476455	8.615	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.581	200	33366	3.064	ng/ul	-0.01
73) Anthracene-d10	17.322	188	773655	8.103	ng/ul	0.00
81) Pyrene-d10	19.557	212	1123090	6.943	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.527	264	1133280	8.191	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.040	94	33888	1.061	ng/ul	97
16) Acetophenone	8.669	105	133416	3.397	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018717.D
Acq On : 08 Dec 2023 17:46
Operator : MA/JU
Sample : 05497-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Time: Dec 09 02:15:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration




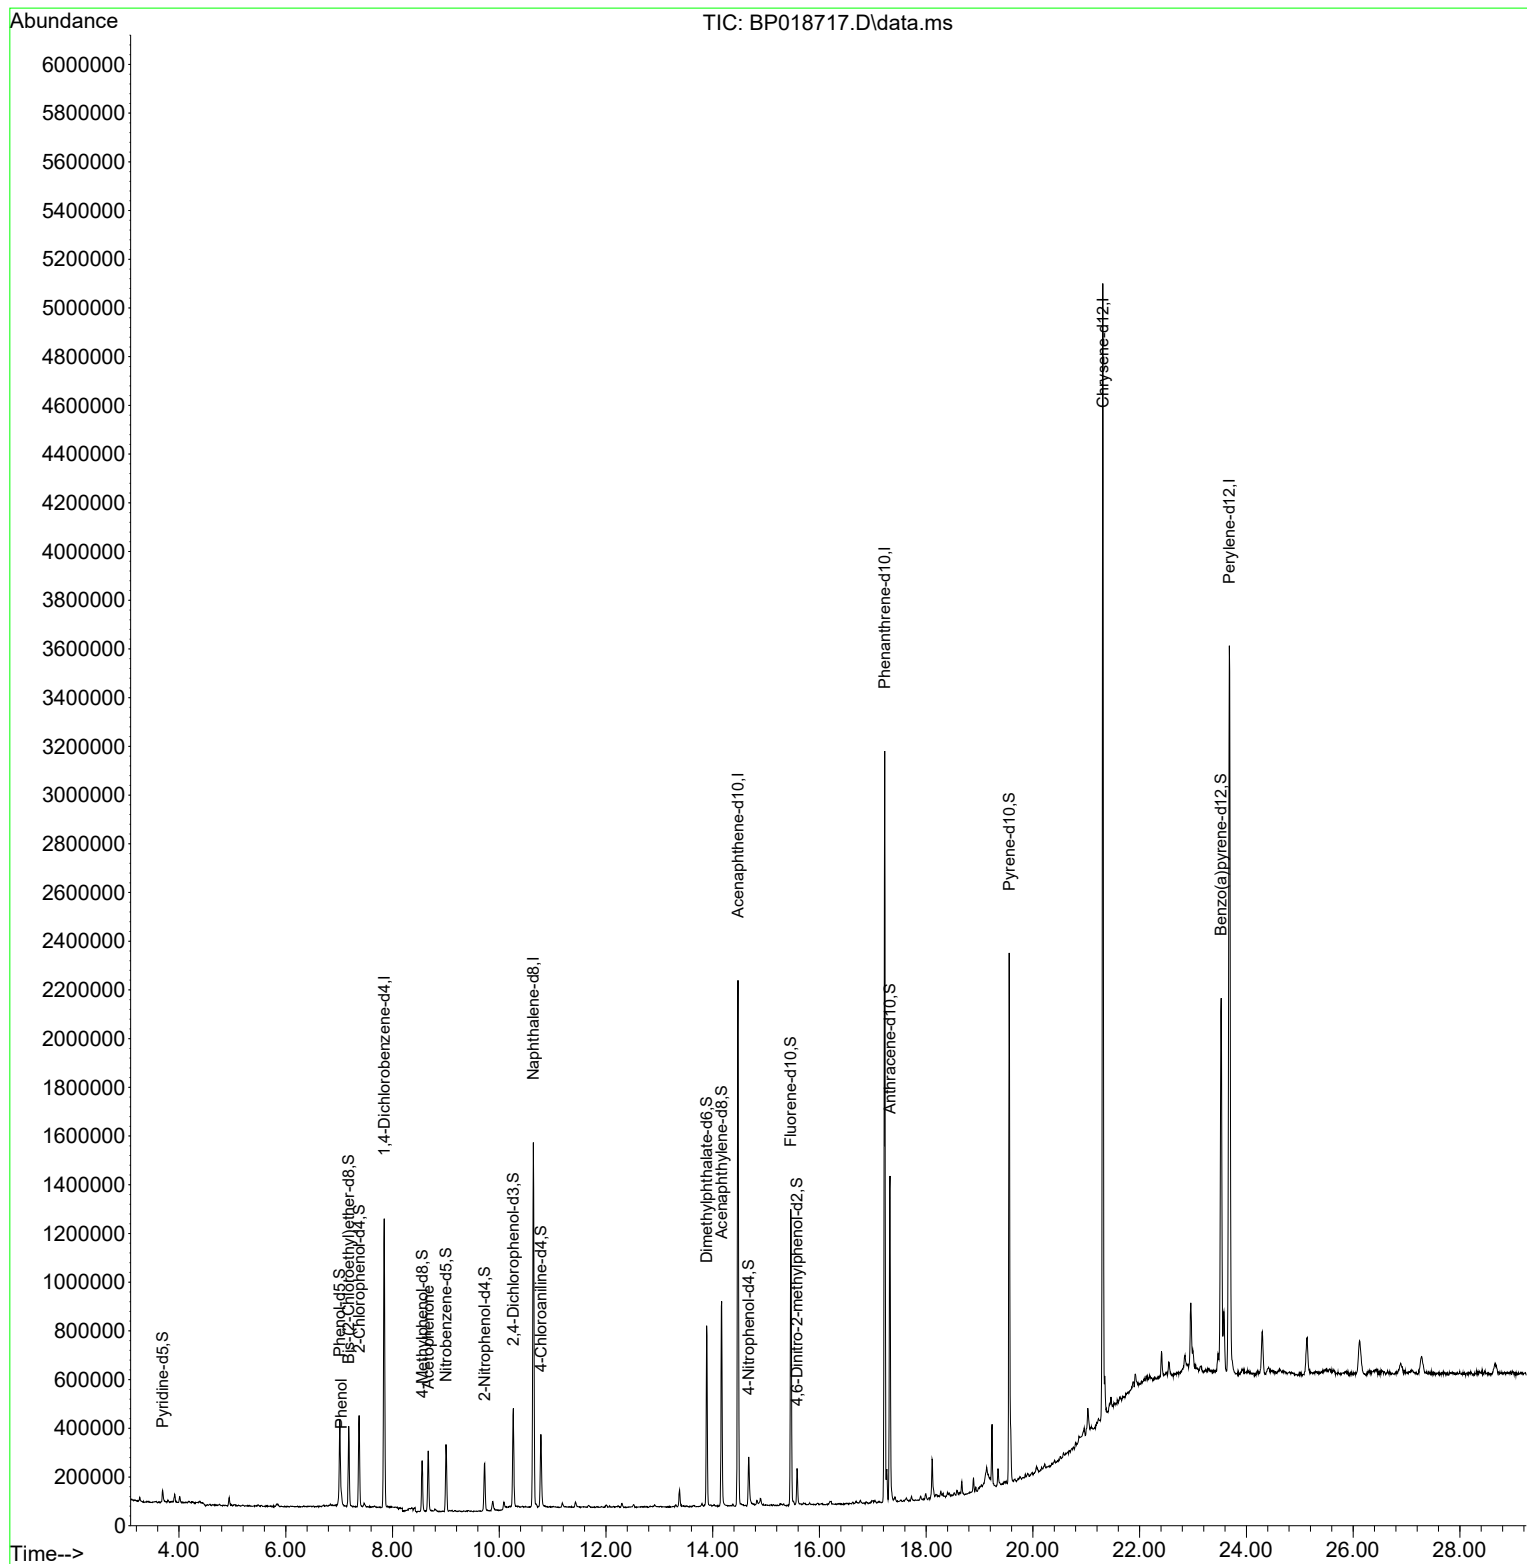


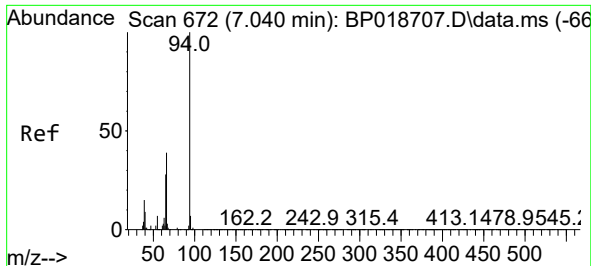

#8
Phenol
Concen: 1.061 ng/ul
RT: 7.040 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP018717.D
Acq: 08 Dec 2023 17:46

Instrument :
BNA_P
ClientSampleId :
C0AB6

Tgt Ion: 94 Resp: 33888
Ion Ratio Lower Upper
94 100
65 30.1 21.0 31.6
66 35.9 28.6 43.0

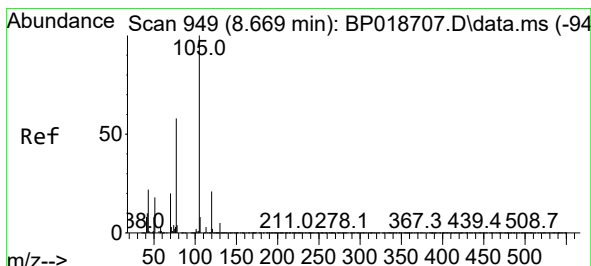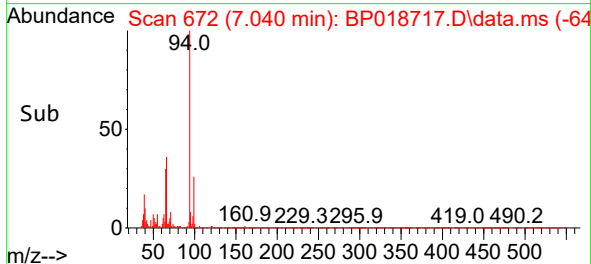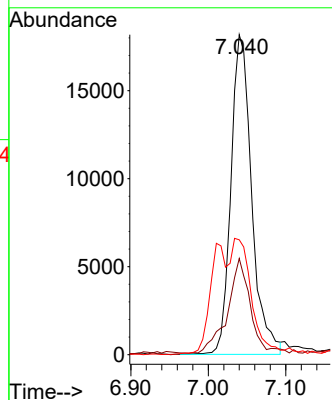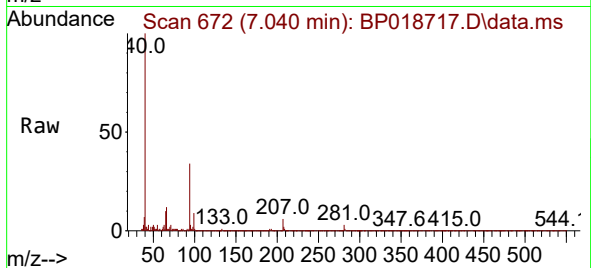

#16
Acetophenone
Concen: 3.397 ng/ul
RT: 8.669 min Scan# 949
Delta R.T. -0.012 min
Lab File: BP018717.D
Acq: 08 Dec 2023 17:46

Tgt Ion: 105 Resp: 133416
Ion Ratio Lower Upper
105 100
77 75.0 59.4 89.0
51 23.9 19.4 29.0

