

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018668.D
 Acq On : 07 Dec 2023 11:09
 Operator : MA/JU
 Sample : PB157420BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK420

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018668.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	39	rVB	97552	124294	1.42%	0.158%
2	3.681	97	101	119	rBV	1100266	1558622	17.82%	1.979%
3	4.011	154	157	162	rVB	20441	26014	0.30%	0.033%
4	5.740	448	451	455	rVB	9732	16452	0.19%	0.021%
5	6.034	499	501	505	rVB	11155	14307	0.16%	0.018%
6	6.322	545	550	553	rBV	9455	17027	0.19%	0.022%
7	6.364	555	557	562	rVB	8938	11739	0.13%	0.015%
8	6.681	600	611	612	rBV	14936	39006	0.45%	0.050%
9	7.011	660	667	674	rBV	1172576	1807498	20.67%	2.295%
10	7.181	690	696	704	rVB	966396	1469542	16.80%	1.866%
11	7.375	720	729	737	rBV	1175229	1848690	21.14%	2.348%
12	7.846	801	809	816	rBV	1219342	1905113	21.79%	2.419%
13	8.558	923	930	941	rBV	1385240	2230545	25.51%	2.833%
14	9.005	999	1006	1018	rVB	1053257	1691460	19.34%	2.148%
15	9.728	1122	1129	1138	rBV	841631	1346294	15.40%	1.710%
16	10.263	1211	1220	1230	rBV	1346644	2218951	25.37%	2.818%
17	10.640	1276	1284	1295	rBV	1530094	2584773	29.56%	3.282%
18	10.781	1297	1308	1319	rBV	1410915	2376068	27.17%	3.017%
19	12.234	1548	1555	1562	rBV2	23186	42126	0.48%	0.053%
20	13.381	1745	1750	1755	rBV4	22488	40196	0.46%	0.051%
21	13.893	1831	1837	1844	rBV	2439157	3360973	38.43%	4.268%
22	14.169	1877	1884	1892	rBV	2775975	3934770	45.00%	4.997%
23	14.475	1929	1936	1945	rBV	2305293	3453580	39.49%	4.386%
24	14.675	1964	1970	1986	rVB	1166390	1784022	20.40%	2.266%
25	14.893	2003	2007	2011	rVB	17064	26369	0.30%	0.033%
26	15.028	2026	2030	2032	rBV	7626	11995	0.14%	0.015%
27	15.051	2032	2034	2037	rVB	10550	11340	0.13%	0.014%
28	15.222	2054	2063	2065	rBV2	7514	16347	0.19%	0.021%
29	15.469	2099	2105	2114	rBV	3040145	4337642	49.60%	5.508%
30	15.534	2114	2116	2118	rVB	13027	12808	0.15%	0.016%
31	15.587	2119	2125	2135	rVV	961095	1329032	15.20%	1.688%
32	15.710	2139	2146	2153	rBV2	19642	47065	0.54%	0.060%
33	16.263	2236	2240	2246	rVB7	7528	11920	0.14%	0.015%
34	17.222	2397	2403	2413	rBV	2991474	4399070	50.31%	5.586%
35	17.322	2414	2420	2431	rVV	3971404	5841373	66.80%	7.418%
36	18.116	2550	2555	2565	rBV4	101380	161672	1.85%	0.205%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018668.D
Acq On : 07 Dec 2023 11:09
Operator : MA/JU
Sample : PB157420BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK420

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.139	2725	2729	2735	rBV2	61647	80725	0.92%	0.103%
38	19.204	2736	2740	2748	rBV	65352	98627	1.13%	0.125%
39	19.351	2761	2765	2773	rBV3	77362	111834	1.28%	0.142%
40	19.563	2795	2801	2807	rBV	5802984	7573235	86.60%	9.617%
41	21.316	3093	3099	3108	rBV	4470675	5689846	65.07%	7.226%
42	23.533	3468	3476	3483	rBV2	4489063	8744745	100.00%	11.105%
43	23.686	3495	3502	3514	rVB	3225519	6337211	72.47%	8.048%




Sum of corrected areas: 78744918

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018668.D
Acq On : 07 Dec 2023 11:09
Operator : MA/JU
Sample : PB157420BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK420

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

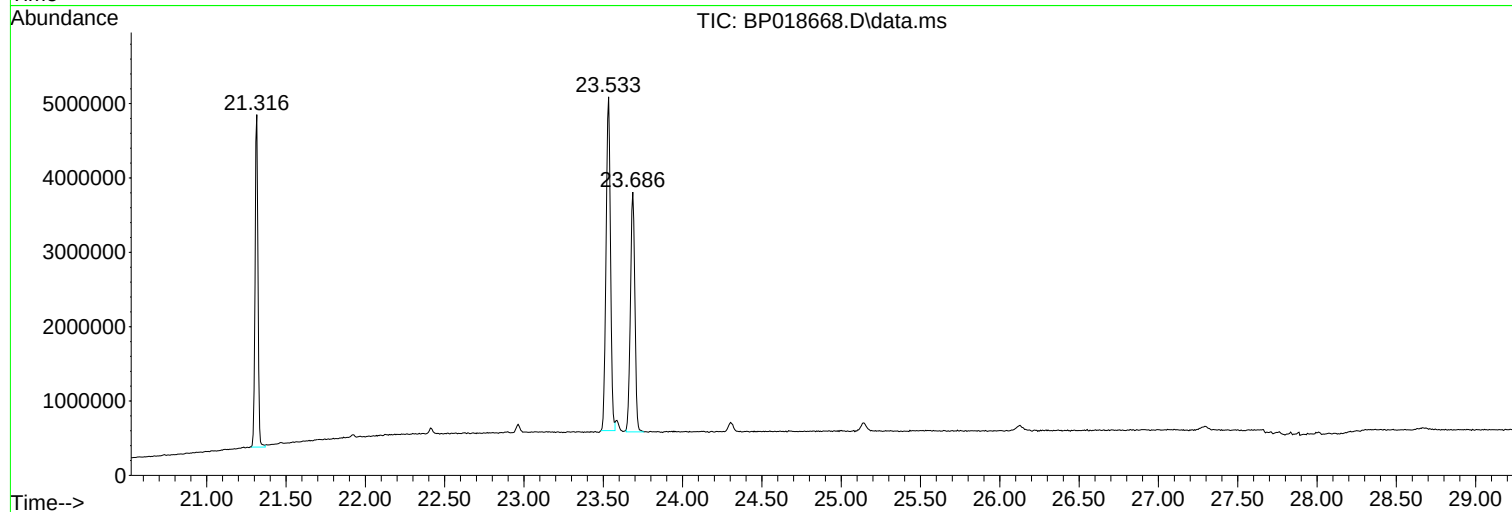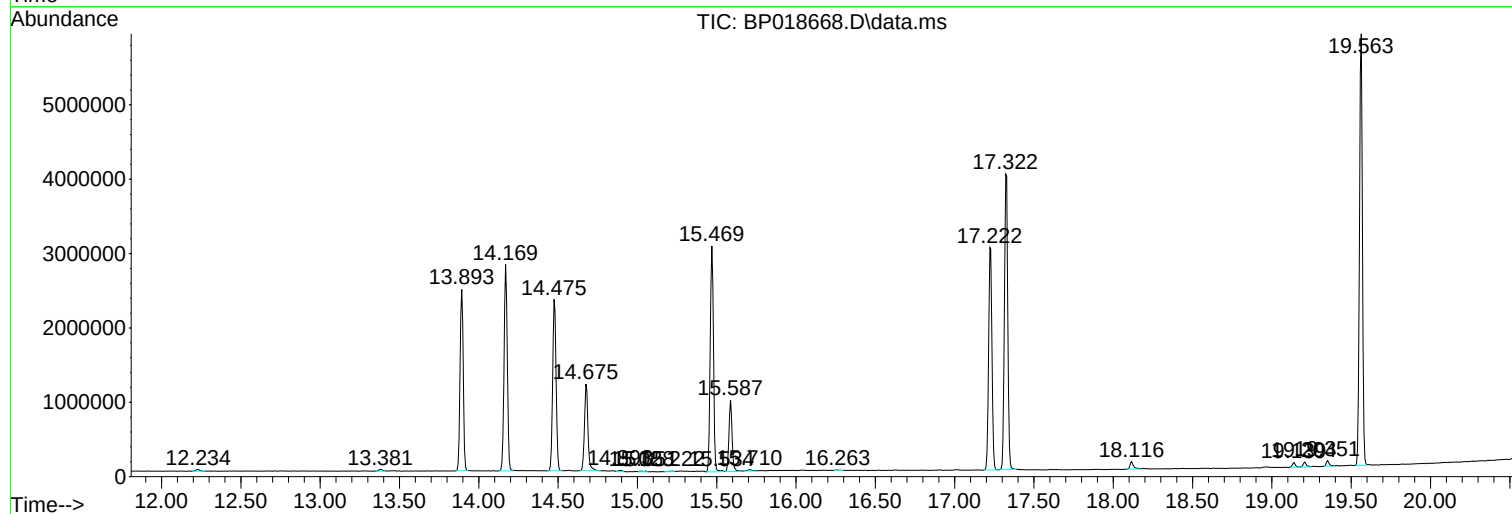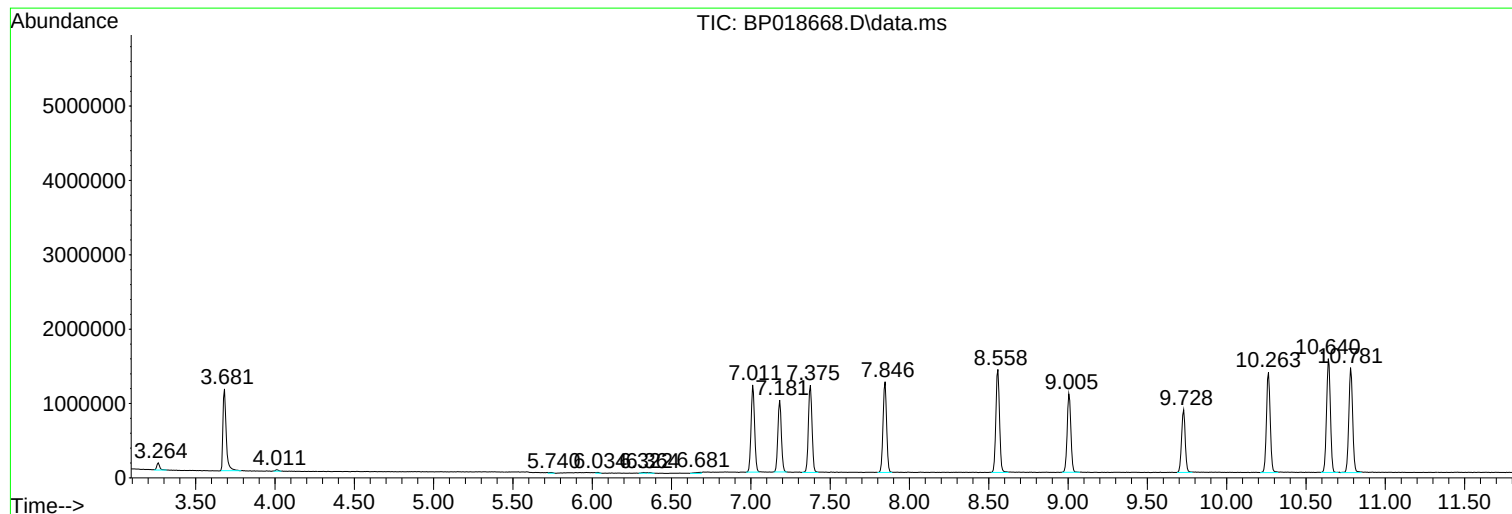

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018668.D
Acq On : 07 Dec 2023 11:09
Operator : MA/JU
Sample : PB157420BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK420

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018668.D
Acq On : 07 Dec 2023 11:09
Operator : MA/JU
Sample : PB157420BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK420

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------