

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018669.D
 Acq On : 07 Dec 2023 11:43
 Operator : MA/JU
 Sample : PB157493BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK493

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	38	rVB	86443	116101	1.39%	0.186%
2	3.681	97	101	118	rBV	1049463	1465001	17.56%	2.342%
3	4.017	154	158	163	rVB2	19543	28876	0.35%	0.046%
4	7.011	658	667	676	rBV	1037336	1674823	20.08%	2.678%
5	7.181	690	696	705	rVB	904845	1383305	16.58%	2.212%
6	7.375	723	729	739	rBV	1111646	1706809	20.46%	2.729%
7	7.846	802	809	819	rVB	1142776	1776297	21.30%	2.840%
8	8.558	924	930	945	rVB	1173157	1865954	22.37%	2.983%
9	8.840	974	978	984	rBV	11016	27633	0.33%	0.044%
10	9.005	997	1006	1013	rBV	858965	1422060	17.05%	2.274%
11	9.075	1013	1018	1021	rVB	11344	18848	0.23%	0.030%
12	9.446	1076	1081	1084	rBV	10649	22691	0.27%	0.036%
13	9.557	1096	1100	1102	rBV	8693	12138	0.15%	0.019%
14	9.728	1122	1129	1137	rBV	686035	1123209	13.47%	1.796%
15	10.263	1212	1220	1228	rBV	931890	1529745	18.34%	2.446%
16	10.640	1277	1284	1293	rVB	1008068	1721087	20.63%	2.752%
17	10.781	1300	1308	1320	rBV	948116	1588282	19.04%	2.539%
18	12.228	1548	1554	1560	rBV3	19307	39765	0.48%	0.064%
19	13.387	1745	1751	1755	rBV5	14979	27197	0.33%	0.043%
20	13.893	1830	1837	1845	rBV	1742734	2352784	28.21%	3.762%
21	14.169	1877	1884	1896	rBV2	1849428	2668769	31.99%	4.267%
22	14.475	1929	1936	1944	rBV	1616152	2337885	28.03%	3.738%
23	14.675	1964	1970	1987	rBV	811494	1290455	15.47%	2.063%
24	15.469	2096	2105	2114	rBV	2444795	3482944	41.76%	5.569%
25	15.587	2118	2125	2136	rBV	779844	1057355	12.68%	1.691%
26	15.704	2141	2145	2154	rVB3	13879	27350	0.33%	0.044%
27	17.222	2396	2403	2412	rBV	2208333	3137325	37.61%	5.016%
28	17.322	2414	2420	2432	rVV2	2773323	4130772	49.52%	6.604%
29	18.116	2550	2555	2562	rBV2	54421	86293	1.03%	0.138%
30	19.133	2725	2728	2735	rVB3	40758	54799	0.66%	0.088%
31	19.204	2736	2740	2748	rVV	44530	64849	0.78%	0.104%
32	19.351	2761	2765	2770	rBV5	49041	66459	0.80%	0.106%
33	19.563	2795	2801	2807	rBV	4158948	5538160	66.39%	8.855%
34	21.316	3093	3099	3104	rBV	3454734	4360179	52.27%	6.971%
35	23.533	3468	3476	3482	rBV2	4347712	8341238	100.00%	13.336%
36	23.686	3495	3502	3514	rVB	3013024	5997750	71.90%	9.589%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018669.D
Acq On : 07 Dec 2023 11:43
Operator : MA/JU
Sample : PB157493BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK493

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 62545187

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018669.D
Acq On : 07 Dec 2023 11:43
Operator : MA/JU
Sample : PB157493BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

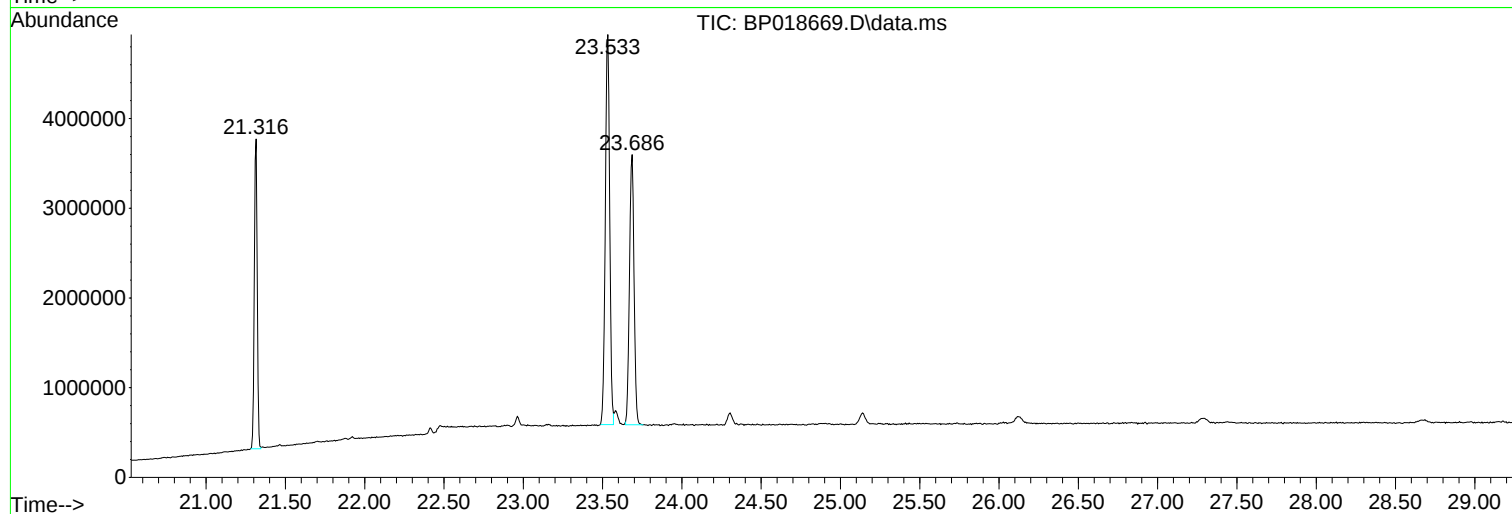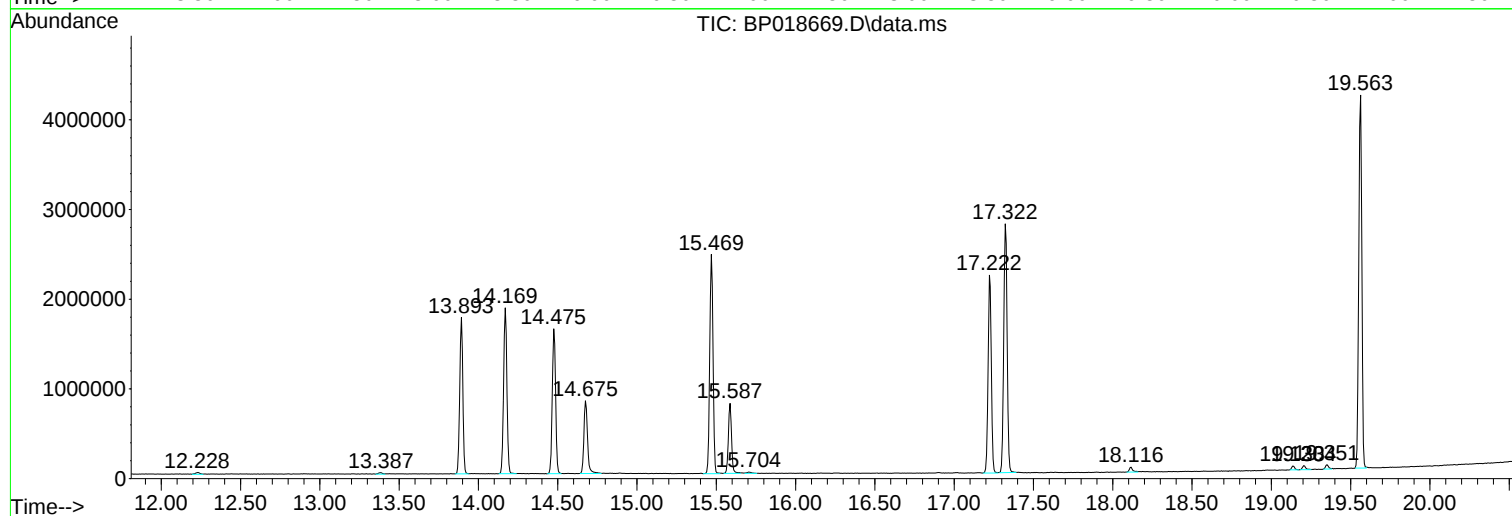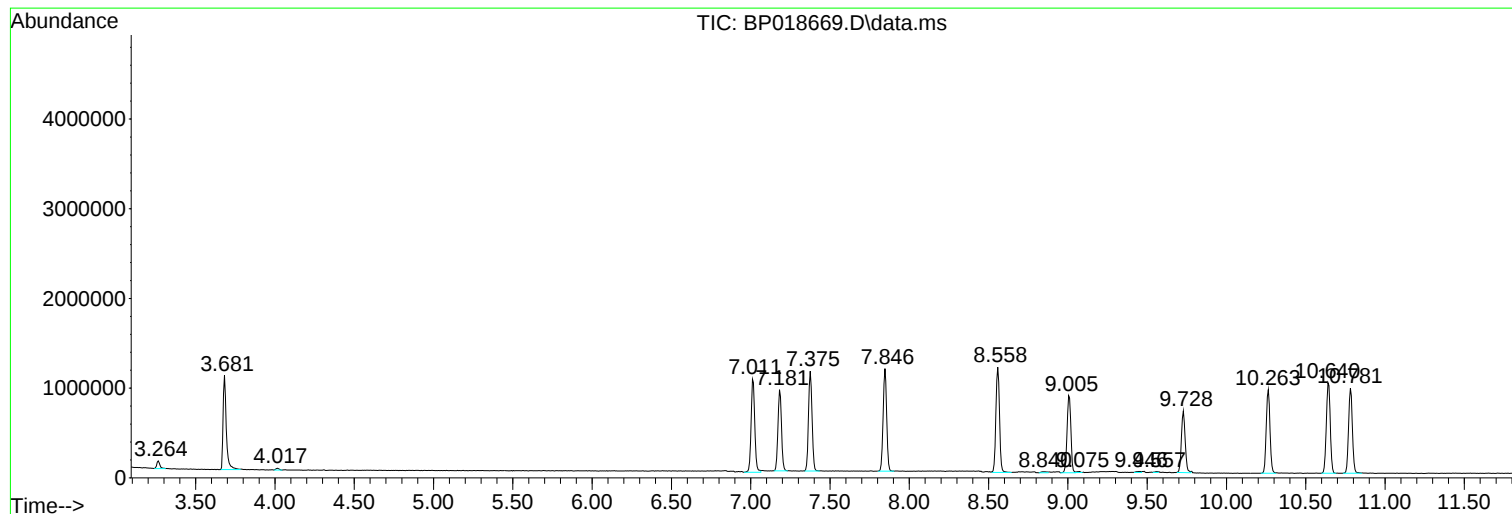

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018669.D
Acq On : 07 Dec 2023 11:43
Operator : MA/JU
Sample : PB157493BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018669.D
Acq On : 07 Dec 2023 11:43
Operator : MA/JU
Sample : PB157493BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc