

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018675.D
 Acq On : 07 Dec 2023 16:19
 Operator : MA/JU
 Sample : PB157408BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK408

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	41	rVB	114742	151349	1.40%	0.162%
2	3.681	97	101	116	rBV	1349031	1918390	17.72%	2.048%
3	4.017	154	158	162	rBV	22028	25029	0.23%	0.027%
4	6.587	587	595	596	rBV	11697	26483	0.24%	0.028%
5	7.016	660	668	676	rBV	1394717	2232909	20.62%	2.384%
6	7.181	690	696	705	rVB	1191219	1805686	16.68%	1.928%
7	7.375	722	729	737	rBV	1433608	2230514	20.60%	2.381%
8	7.846	802	809	818	rVB	1266481	1981239	18.30%	2.115%
9	8.558	923	930	939	rBV	1731104	2744783	25.35%	2.930%
10	9.005	999	1006	1018	rBV	1302321	2096626	19.36%	2.238%
11	9.728	1122	1129	1139	rBV	905808	1500766	13.86%	1.602%
12	9.799	1139	1141	1144	rVB	12448	13067	0.12%	0.014%
13	9.869	1144	1153	1154	rBV	9129	13999	0.13%	0.015%
14	10.175	1200	1205	1206	rBV	7821	10901	0.10%	0.012%
15	10.263	1212	1220	1231	rBV	1530690	2435044	22.49%	2.599%
16	10.640	1277	1284	1295	rVB	1599701	2724613	25.16%	2.909%
17	10.781	1301	1308	1324	rBV	1750803	2934023	27.10%	3.132%
18	12.228	1549	1554	1562	rBV2	34050	53864	0.50%	0.058%
19	13.375	1746	1749	1754	rVB2	23716	34183	0.32%	0.036%
20	13.893	1831	1837	1844	rBV	3064877	4172004	38.53%	4.454%
21	14.169	1877	1884	1893	rBV2	3338600	4954828	45.76%	5.289%
22	14.475	1929	1936	1946	rBV	2535260	3709525	34.26%	3.960%
23	14.675	1964	1970	1987	rBV	1551708	2322429	21.45%	2.479%
24	15.469	2098	2105	2113	rBV	4472861	6329831	58.46%	6.757%
25	15.587	2119	2125	2141	rBV	1359195	1848986	17.08%	1.974%
26	15.704	2142	2145	2154	rVB2	23640	37443	0.35%	0.040%
27	16.898	2346	2348	2355	rVB2	10590	14420	0.13%	0.015%
28	17.222	2397	2403	2410	rBV	3224829	4732792	43.71%	5.052%
29	17.322	2414	2420	2431	rVV2	5257596	7280868	67.24%	7.772%
30	18.110	2550	2554	2560	rBV4	39634	56133	0.52%	0.060%
31	18.434	2607	2609	2616	rVB5	12155	18547	0.17%	0.020%
32	19.134	2724	2728	2733	rBV2	76398	103136	0.95%	0.110%
33	19.204	2736	2740	2747	rBV	76311	115465	1.07%	0.123%
34	19.345	2762	2764	2770	rVB5	27411	32461	0.30%	0.035%
35	19.563	2794	2801	2808	rBV	6971568	9430382	87.09%	10.067%
36	21.310	3093	3098	3104	rBV	4986033	5988247	55.30%	6.393%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018675.D
Acq On : 07 Dec 2023 16:19
Operator : MA/JU
Sample : PB157408BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK408

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	23.527	3468	3475	3483	rBV2	5596617	10828429	100.00%	11.560%
38	23.680	3494	3501	3513	rVB	3320267	6766154	62.49%	7.223%




Sum of corrected areas: 93675548

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018675.D
Acq On : 07 Dec 2023 16:19
Operator : MA/JU
Sample : PB157408BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

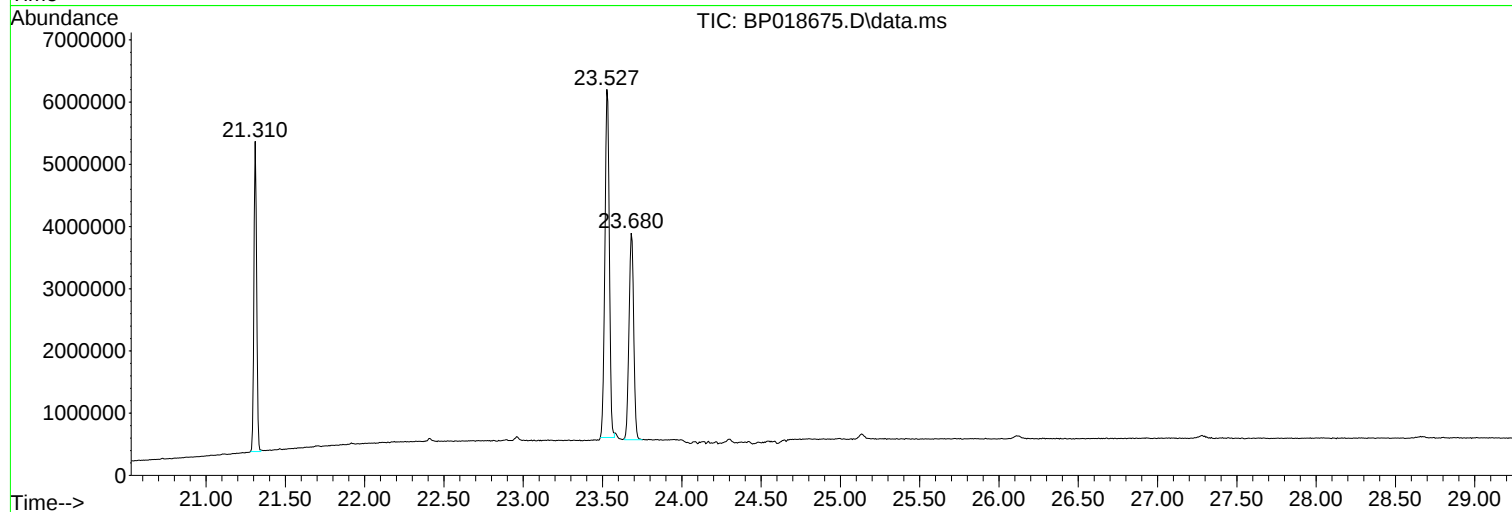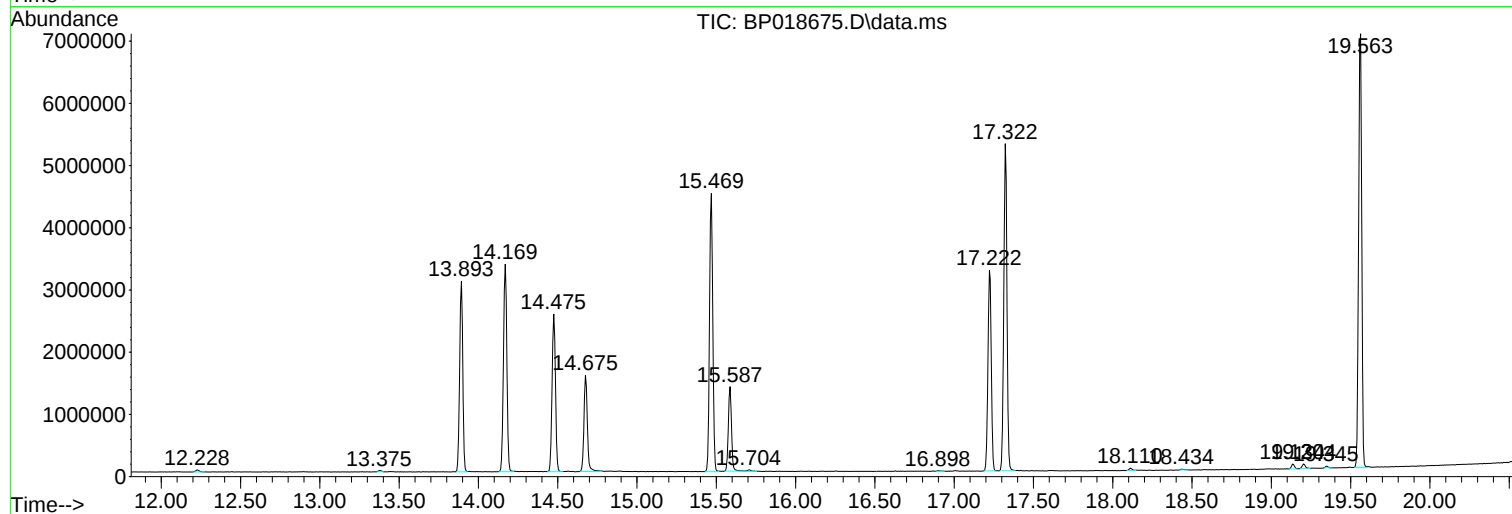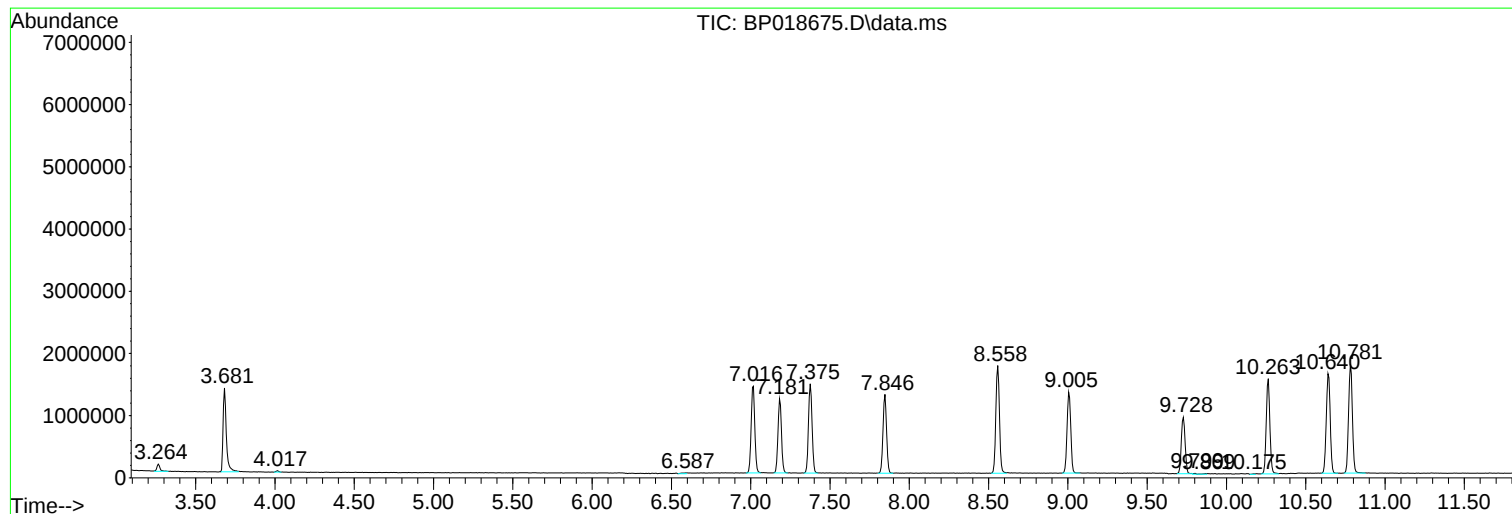

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018675.D
Acq On : 07 Dec 2023 16:19
Operator : MA/JU
Sample : PB157408BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018675.D
Acq On : 07 Dec 2023 16:19
Operator : MA/JU
Sample : PB157408BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc