

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018678.D
 Acq On : 07 Dec 2023 18:01
 Operator : MA/JU
 Sample : 05459-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	28	30	36	rVB2	11602	15426	0.34%	0.061%
2	3.693	99	103	111	rVB	29790	44056	0.97%	0.174%
3	3.922	137	142	147	rVB	27890	40651	0.90%	0.160%
4	4.011	154	157	163	rVB2	15116	21991	0.49%	0.087%
5	4.393	218	222	229	rVB7	7387	10586	0.23%	0.042%
6	4.664	264	268	271	rBV5	3823	7445	0.16%	0.029%
7	4.940	309	315	320	rBV2	25517	42365	0.94%	0.167%
8	5.040	327	332	337	rVB3	3972	7695	0.17%	0.030%
9	5.205	357	360	363	rVB4	4734	5266	0.12%	0.021%
10	5.558	417	420	424	rVB3	4171	5317	0.12%	0.021%
11	5.828	461	466	469	rBV3	8719	17387	0.38%	0.069%
12	5.858	469	471	475	rVB3	8293	9187	0.20%	0.036%
13	6.475	570	576	580	rBV8	2988	6313	0.14%	0.025%
14	6.646	602	605	609	rBV	4320	5698	0.13%	0.022%
15	6.840	634	638	643	rVB3	5014	8981	0.20%	0.035%
16	7.010	658	667	680	rBV2	130543	281595	6.22%	1.111%
17	7.181	689	696	704	rBV	122340	183668	4.06%	0.725%
18	7.375	723	729	735	rBV	136732	213437	4.71%	0.842%
19	7.475	740	746	749	rBV4	12338	21486	0.47%	0.085%
20	7.846	801	809	816	rVB	804977	1245084	27.49%	4.914%
21	8.557	923	930	937	rBV	85799	145819	3.22%	0.576%
22	8.669	943	949	956	rBV	182571	294287	6.50%	1.162%
23	8.793	964	970	973	rBV2	8761	14967	0.33%	0.059%
24	9.004	998	1006	1013	rVV	128476	213361	4.71%	0.842%
25	9.075	1015	1018	1023	rVV3	6007	10656	0.24%	0.042%
26	9.428	1073	1078	1082	rVB6	5489	10969	0.24%	0.043%
27	9.610	1106	1109	1112	rBV2	4018	5204	0.11%	0.021%
28	9.728	1123	1129	1136	rBV	86281	149586	3.30%	0.590%
29	9.875	1148	1154	1161	rBV2	29546	56697	1.25%	0.224%
30	10.087	1184	1190	1196	rBV4	18319	32648	0.72%	0.129%
31	10.204	1206	1210	1213	rBV5	3359	6446	0.14%	0.025%
32	10.263	1213	1220	1228	rVB	148438	237175	5.24%	0.936%
33	10.640	1277	1284	1291	rBV	987743	1677388	37.04%	6.621%
34	10.687	1291	1292	1299	rVV2	12707	17970	0.40%	0.071%
35	10.781	1301	1308	1320	rVB	88302	170943	3.77%	0.675%
36	11.181	1372	1376	1387	rVV9	12959	29395	0.65%	0.116%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018678.D
 Acq On : 07 Dec 2023 18:01
 Operator : MA/JU
 Sample : 05459-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	11.428	1412	1418	1429	rBV	18316	41168	0.91%	0.162%
38	11.675	1454	1460	1464	rBV3	8704	15276	0.34%	0.060%
39	12.069	1523	1527	1530	rBV4	7604	10013	0.22%	0.040%
40	12.222	1547	1553	1558	rVB2	12806	23053	0.51%	0.091%
41	12.304	1561	1567	1571	rBV2	17964	26462	0.58%	0.104%
42	12.404	1581	1584	1588	rVB3	4026	6466	0.14%	0.026%
43	12.522	1597	1604	1610	rVB2	14477	27449	0.61%	0.108%
44	12.916	1665	1671	1676	rVB3	6480	8739	0.19%	0.034%
45	13.022	1684	1689	1692	rVB4	6114	10845	0.24%	0.043%
46	13.310	1733	1738	1744	rVB4	10521	18994	0.42%	0.075%
47	13.381	1744	1750	1755	rBV3	23107	38502	0.85%	0.152%
48	13.634	1789	1793	1794	rBV3	6153	7063	0.16%	0.028%
49	13.792	1816	1820	1821	rBV2	10287	11229	0.25%	0.044%
50	13.851	1827	1830	1831	rBV3	8544	9733	0.21%	0.038%
51	13.887	1831	1836	1845	rVV	294700	427586	9.44%	1.688%
52	13.969	1845	1850	1853	rVB4	8902	13541	0.30%	0.053%
53	14.016	1853	1858	1859	rBV4	4512	6313	0.14%	0.025%
54	14.028	1859	1860	1864	rVV3	8495	8557	0.19%	0.034%
55	14.169	1878	1884	1892	rVB	304989	463566	10.24%	1.830%
56	14.381	1915	1920	1923	rVB5	9187	12592	0.28%	0.050%
57	14.475	1928	1936	1944	rBV	1574741	2295714	50.69%	9.061%
58	14.681	1963	1971	1980	rBV2	57121	113260	2.50%	0.447%
59	14.828	1991	1996	2000	rBV	13117	21926	0.48%	0.087%
60	14.898	2000	2008	2015	rVV6	26647	64498	1.42%	0.255%
61	14.945	2015	2016	2021	rVB4	5873	6312	0.14%	0.025%
62	15.087	2036	2040	2045	rBV3	5861	9589	0.21%	0.038%
63	15.334	2078	2082	2085	rVB3	8320	10586	0.23%	0.042%
64	15.469	2098	2105	2110	rBV	461518	671467	14.83%	2.650%
65	15.516	2110	2113	2118	rVV3	13133	19676	0.43%	0.078%
66	15.581	2120	2124	2134	rVV2	51590	88695	1.96%	0.350%
67	15.734	2148	2150	2154	rVB3	7286	8658	0.19%	0.034%
68	15.822	2161	2165	2172	rVB5	8026	13521	0.30%	0.053%
69	15.881	2174	2175	2182	rBV4	3264	5738	0.13%	0.023%
70	15.963	2186	2189	2193	rVV4	4640	6382	0.14%	0.025%
71	16.051	2198	2204	2209	rVB6	6041	15440	0.34%	0.061%
72	16.216	2225	2232	2236	rBV2	21637	43323	0.96%	0.171%
73	16.763	2319	2325	2329	rBV3	17372	29980	0.66%	0.118%
74	16.986	2360	2363	2370	rBV3	13018	18351	0.41%	0.072%
75	17.045	2370	2373	2375	rVB3	5505	6851	0.15%	0.027%
76	17.139	2387	2389	2394	rVB	3473	5253	0.12%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018678.D
 Acq On : 07 Dec 2023 18:01
 Operator : MA/JU
 Sample : 05459-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	17.222	2397	2403	2409	rVV	2104229	3073688	67.87%	12.132%
78	17.263	2409	2410	2414	rVV	55011	53898	1.19%	0.213%
79	17.322	2414	2420	2431	rVV	500009	740733	16.36%	2.924%
80	17.422	2433	2437	2441	rVB5	22938	32778	0.72%	0.129%
81	17.633	2470	2473	2479	rVB6	4979	6737	0.15%	0.027%
82	17.728	2486	2489	2493	rBV3	16252	19071	0.42%	0.075%
83	17.898	2513	2518	2522	rBV6	10561	17291	0.38%	0.068%
84	17.992	2530	2534	2541	rBV3	13839	26417	0.58%	0.104%
85	18.110	2547	2554	2564	rBV4	109933	204478	4.52%	0.807%
86	18.269	2578	2581	2586	rBV4	10313	17722	0.39%	0.070%
87	18.316	2586	2589	2592	rVB3	11068	14470	0.32%	0.057%
88	18.398	2600	2603	2608	rBV4	13967	22773	0.50%	0.090%
89	18.669	2646	2649	2653	rVB	35972	40266	0.89%	0.159%
90	18.886	2682	2686	2691	rBV2	32262	39822	0.88%	0.157%
91	18.927	2691	2693	2697	rVB3	11933	14293	0.32%	0.056%
92	19.133	2722	2728	2733	rBV8	28297	71586	1.58%	0.283%
93	19.204	2737	2740	2742	rVV3	33395	43444	0.96%	0.171%
94	19.233	2742	2745	2749	rVB	67957	82731	1.83%	0.327%
95	19.345	2760	2764	2770	rBV4	71679	97361	2.15%	0.384%
96	19.557	2795	2800	2813	rVB	833471	1159637	25.61%	4.577%
97	21.027	3048	3050	3058	rVB3	52770	75528	1.67%	0.298%
98	21.310	3093	3098	3103	rBV	3281064	4065248	89.77%	16.046%
99	23.521	3469	3474	3480	rBV2	548035	977680	21.59%	3.859%
100	23.680	3494	3501	3515	rVB	2196830	4528529	100.00%	17.874%




Sum of corrected areas: 25335693

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018678.D
Acq On : 07 Dec 2023 18:01
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

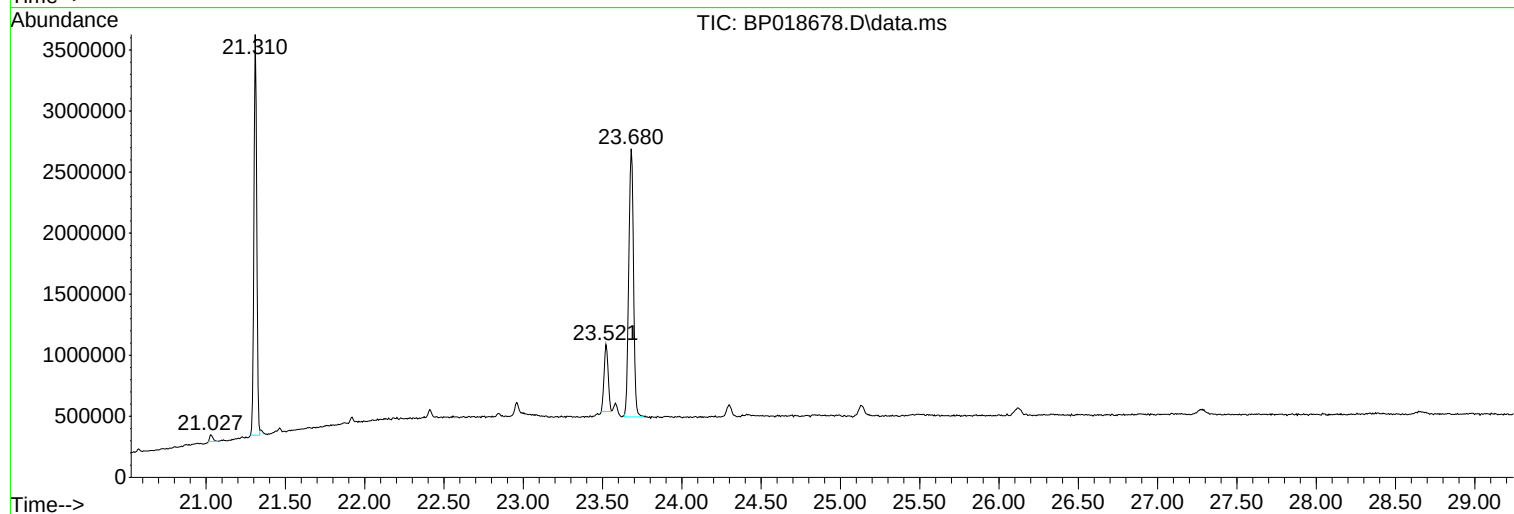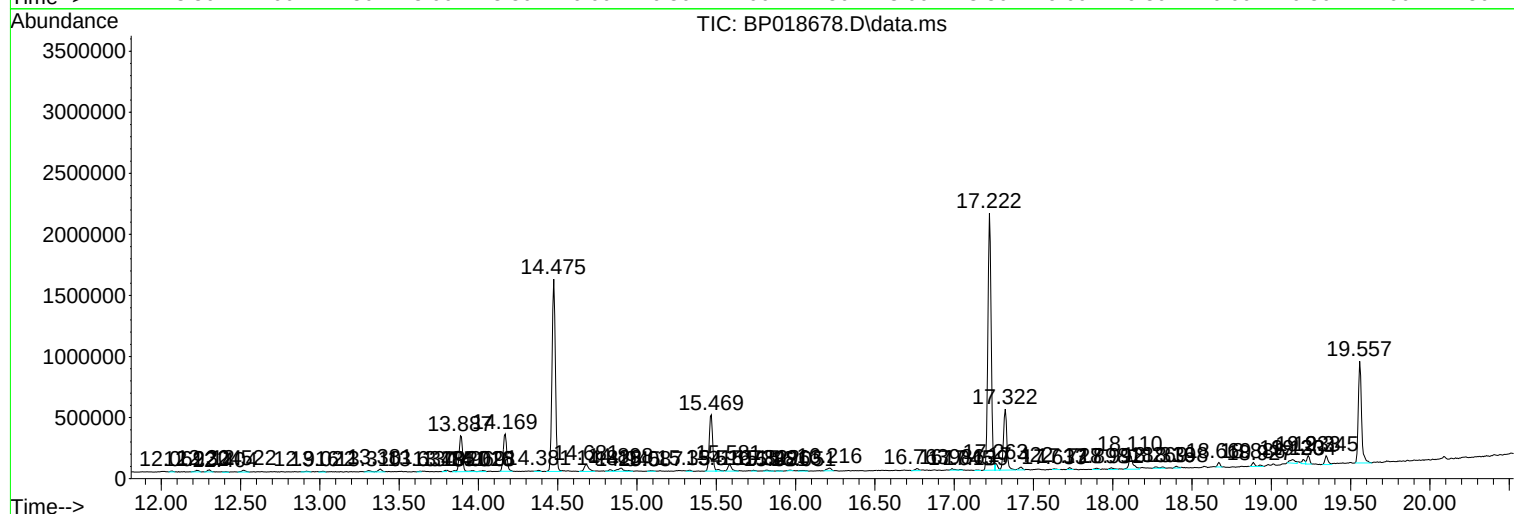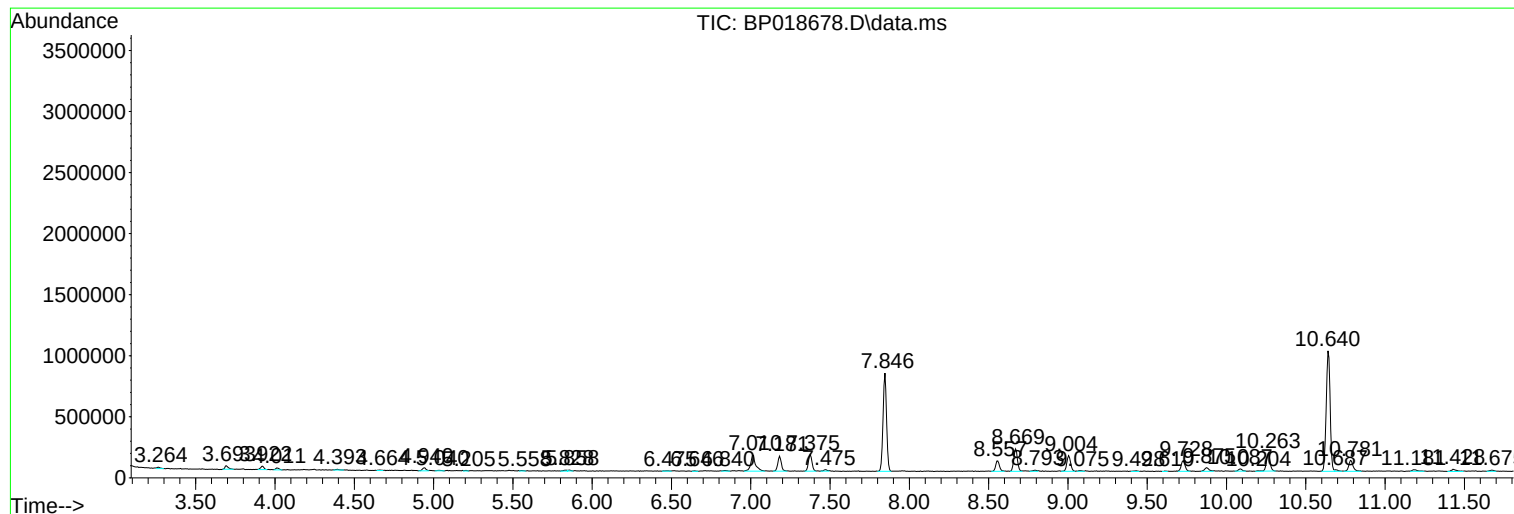

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018678.D
Acq On : 07 Dec 2023 18:01
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018678.D
Acq On : 07 Dec 2023 18:01
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc