

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018681.D
 Acq On : 07 Dec 2023 19:43
 Operator : MA/JU
 Sample : 05459-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	28	30	36	rVB2	17025	22453	0.42%	0.069%
2	3.693	99	103	113	rBV2	47246	72571	1.36%	0.224%
3	3.799	118	121	125	rVB	21636	25509	0.48%	0.079%
4	3.922	137	142	146	rVB2	33161	50011	0.93%	0.155%
5	4.016	154	158	163	rVB2	22748	33786	0.63%	0.104%
6	4.240	194	196	202	rVB2	18350	28302	0.53%	0.087%
7	4.311	204	208	210	rBV	5744	7647	0.14%	0.024%
8	4.393	220	222	225	rVB2	9713	7377	0.14%	0.023%
9	4.516	241	243	245	rBV	5565	5933	0.11%	0.018%
10	4.646	263	265	266	rVB	10014	6029	0.11%	0.019%
11	4.940	310	315	321	rBV2	28379	45240	0.85%	0.140%
12	5.822	462	465	469	rBV3	6271	10799	0.20%	0.033%
13	6.834	634	637	640	rBV3	4064	5980	0.11%	0.018%
14	7.010	658	667	681	rBV2	147272	308962	5.77%	0.955%
15	7.181	689	696	703	rBV	141530	221049	4.13%	0.683%
16	7.375	721	729	737	rBV	163790	264419	4.94%	0.817%
17	7.469	741	745	751	rBV5	9084	15596	0.29%	0.048%
18	7.552	753	759	760	rBV	17490	26238	0.49%	0.081%
19	7.846	802	809	818	rBV	1033817	1601696	29.93%	4.951%
20	8.557	924	930	940	rBV2	97583	168356	3.15%	0.520%
21	8.669	943	949	957	rBV	257037	409876	7.66%	1.267%
22	8.793	966	970	976	rVB3	10783	19964	0.37%	0.062%
23	9.004	1000	1006	1014	rBV	176829	289243	5.40%	0.894%
24	9.728	1123	1129	1136	rBV	115954	194070	3.63%	0.600%
25	9.875	1148	1154	1162	rBV2	40187	80534	1.50%	0.249%
26	10.087	1186	1190	1197	rVB3	27573	46771	0.87%	0.145%
27	10.263	1214	1220	1227	rBV	206169	333955	6.24%	1.032%
28	10.640	1277	1284	1294	rVB	1328758	2192876	40.97%	6.779%
29	10.781	1302	1308	1316	rBV	107224	195427	3.65%	0.604%
30	11.181	1371	1376	1384	rBV7	15169	35335	0.66%	0.109%
31	11.434	1414	1419	1427	rBV3	20971	46753	0.87%	0.145%
32	11.681	1458	1461	1466	rVB2	7556	12450	0.23%	0.038%
33	12.004	1513	1516	1523	rVB3	10031	18624	0.35%	0.058%
34	12.228	1550	1554	1561	rVB2	17551	26913	0.50%	0.083%
35	13.381	1744	1750	1755	rBV2	32893	53490	1.00%	0.165%
36	13.798	1819	1821	1827	rVB4	5084	7965	0.15%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018681.D
 Acq On : 07 Dec 2023 19:43
 Operator : MA/JU
 Sample : 05459-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	13.892	1831	1837	1847	rVB	431578	616472	11.52%	1.906%
38	14.169	1878	1884	1892	rBV	478820	697173	13.03%	2.155%
39	14.475	1929	1936	1944	rBV	2070445	3020812	56.44%	9.338%
40	14.681	1966	1971	1982	rVB	87508	159063	2.97%	0.492%
41	14.834	1993	1997	2002	rBV3	18547	32255	0.60%	0.100%
42	14.898	2004	2008	2015	rVB5	29438	48818	0.91%	0.151%
43	15.469	2098	2105	2111	rBV	729811	1037846	19.39%	3.208%
44	15.586	2120	2125	2138	rVB	83042	133536	2.49%	0.413%
45	16.769	2323	2326	2330	rVB3	14673	19113	0.36%	0.059%
46	17.222	2397	2403	2409	rBV	2773059	3899878	72.86%	12.055%
47	17.263	2409	2410	2414	rVV2	60742	57885	1.08%	0.179%
48	17.322	2414	2420	2432	rVV	798887	1137300	21.25%	3.516%
49	17.416	2432	2436	2443	rVB6	29101	46652	0.87%	0.144%
50	17.892	2515	2517	2522	rVB5	11421	14231	0.27%	0.044%
51	17.992	2531	2534	2539	rVB2	15048	19985	0.37%	0.062%
52	18.110	2550	2554	2564	rBV3	111070	160702	3.00%	0.497%
53	18.575	2631	2633	2639	rBV4	12325	16915	0.32%	0.052%
54	18.669	2645	2649	2654	rVB2	47822	60602	1.13%	0.187%
55	18.886	2682	2686	2690	rVB2	41992	52372	0.98%	0.162%
56	18.933	2690	2694	2697	rBV2	16538	23360	0.44%	0.072%
57	19.204	2737	2740	2742	rBV2	28426	35282	0.66%	0.109%
58	19.233	2742	2745	2749	rVB	76178	90944	1.70%	0.281%
59	19.345	2761	2764	2769	rBV4	60088	75158	1.40%	0.232%
60	19.557	2795	2800	2813	rVB	1316026	1750695	32.71%	5.412%
61	21.027	3048	3050	3057	rVB3	74631	89873	1.68%	0.278%
62	21.310	3093	3098	3103	rBV	4210197	5073245	94.79%	15.682%
63	22.957	3375	3378	3384	rVB2	192596	266466	4.98%	0.824%
64	23.521	3469	3474	3480	rBV	865974	1469170	27.45%	4.541%
65	23.680	3494	3501	3510	rVB	2722728	5352349	100.00%	16.545%




Sum of corrected areas: 32350351

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018681.D
Acq On : 07 Dec 2023 19:43
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

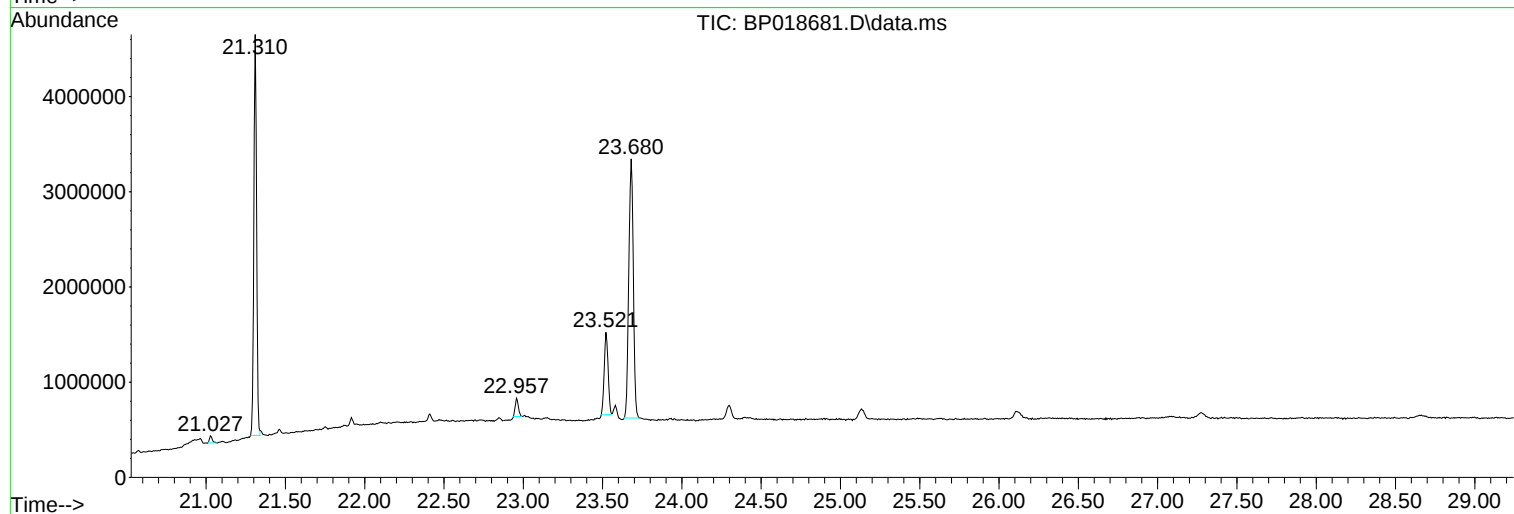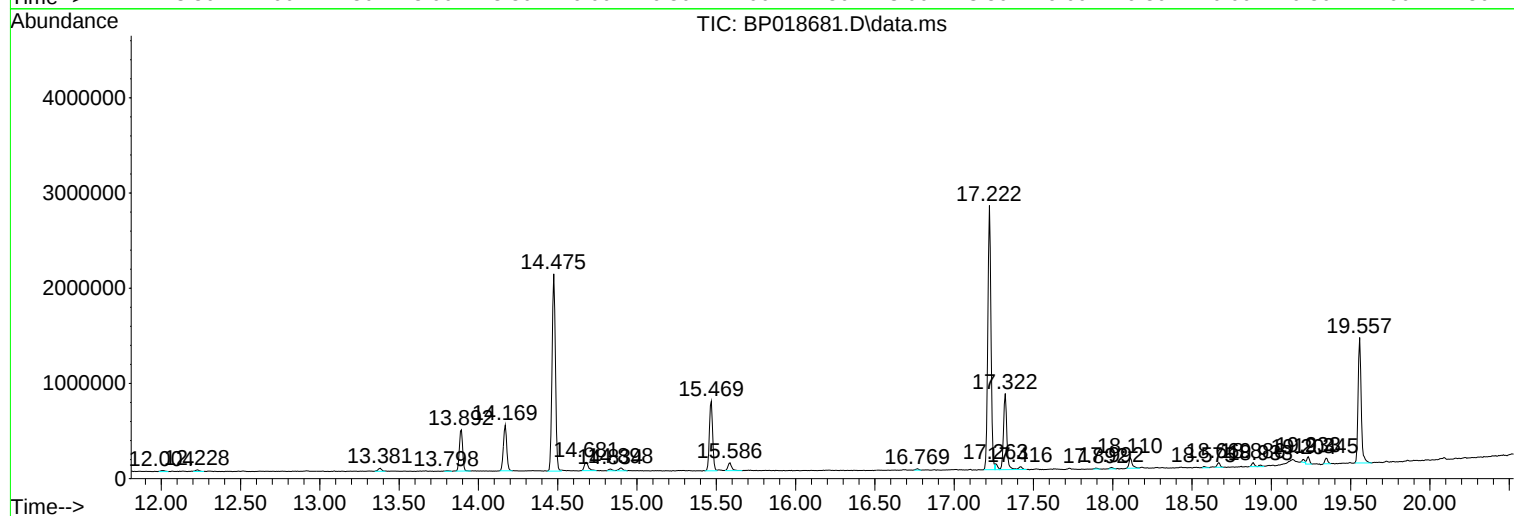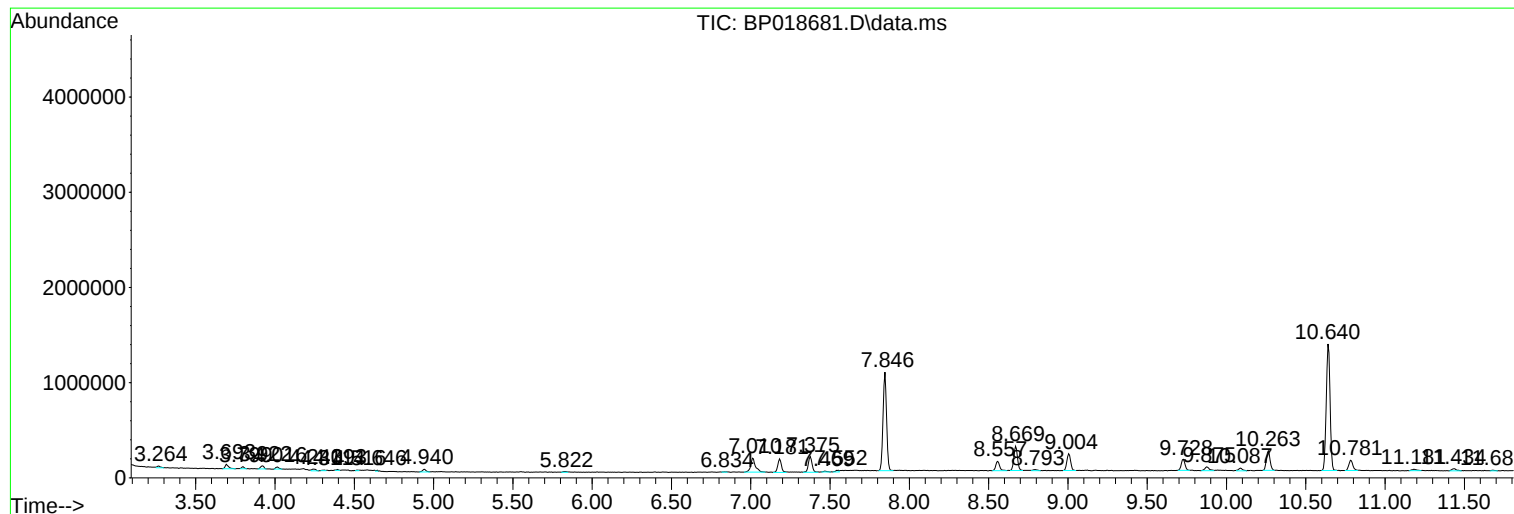

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018681.D
Acq On : 07 Dec 2023 19:43
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018681.D
Acq On : 07 Dec 2023 19:43
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc