

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018682.D
 Acq On : 07 Dec 2023 20:17
 Operator : MA/JU
 Sample : 05459-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	39	rVB3	18505	30913	0.67%	0.113%
2	3.693	99	103	114	rVV	62478	101381	2.20%	0.371%
3	3.793	118	120	125	rVB3	10898	13238	0.29%	0.048%
4	3.922	137	142	148	rVB2	24934	42117	0.92%	0.154%
5	4.017	154	158	163	rVB2	18770	28246	0.61%	0.103%
6	4.940	311	315	319	rBV2	21496	29844	0.65%	0.109%
7	5.481	403	407	410	rVB5	5770	8004	0.17%	0.029%
8	5.546	416	418	425	rVB5	9183	13462	0.29%	0.049%
9	5.828	463	466	468	rBV3	7815	8923	0.19%	0.033%
10	6.069	503	507	509	rBV2	4319	6434	0.14%	0.024%
11	6.322	546	550	553	rBV3	4586	6395	0.14%	0.023%
12	6.758	621	624	625	rBV	3882	4892	0.11%	0.018%
13	6.799	629	631	633	rBV	5084	5552	0.12%	0.020%
14	7.010	659	667	678	rBV2	132008	290798	6.32%	1.063%
15	7.181	691	696	702	rBV	185680	273868	5.96%	1.001%
16	7.375	723	729	735	rBV	175949	270645	5.89%	0.990%
17	7.463	740	744	752	rVB4	22144	56709	1.23%	0.207%
18	7.557	755	760	762	rBV	10387	13211	0.29%	0.048%
19	7.605	766	768	772	rVB2	8602	11647	0.25%	0.043%
20	7.663	772	778	781	rBV3	5574	10997	0.24%	0.040%
21	7.710	781	786	789	rBV2	7144	11596	0.25%	0.042%
22	7.752	789	793	798	rVB2	10791	19401	0.42%	0.071%
23	7.846	798	809	816	rVB	849567	1320656	28.72%	4.828%
24	7.940	819	825	827	rVB	10732	13571	0.30%	0.050%
25	7.981	827	832	834	rBV2	7405	10703	0.23%	0.039%
26	8.034	837	841	842	rBV	10513	12402	0.27%	0.045%
27	8.122	852	856	859	rBV	7771	13427	0.29%	0.049%
28	8.557	923	930	938	rVB2	48894	88423	1.92%	0.323%
29	8.669	943	949	958	rVV	202555	329423	7.16%	1.204%
30	8.793	967	970	975	rVB4	10628	15526	0.34%	0.057%
31	9.004	1000	1006	1014	rBV	182279	295813	6.43%	1.082%
32	9.422	1075	1077	1081	rVB3	7236	10399	0.23%	0.038%
33	9.728	1123	1129	1135	rBV	115263	201726	4.39%	0.738%
34	9.875	1147	1154	1162	rBV2	34566	67930	1.48%	0.248%
35	10.087	1186	1190	1198	rVB4	19568	33982	0.74%	0.124%
36	10.263	1213	1220	1229	rVB	180879	293571	6.38%	1.073%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018682.D
 Acq On : 07 Dec 2023 20:17
 Operator : MA/JU
 Sample : 05459-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	10.640	1276	1284	1292	rBV	1116592	1838754	39.99%	6.723%
38	10.781	1303	1308	1315	rBV	101493	178219	3.88%	0.652%
39	11.181	1370	1376	1384	rBV8	11453	27672	0.60%	0.101%
40	11.428	1414	1418	1425	rBV2	17310	34140	0.74%	0.125%
41	11.681	1456	1461	1466	rBV5	8080	15653	0.34%	0.057%
42	12.004	1514	1516	1520	rVB2	9056	9958	0.22%	0.036%
43	12.228	1550	1554	1559	rBV3	13152	19615	0.43%	0.072%
44	12.298	1562	1566	1571	rVB2	14796	22517	0.49%	0.082%
45	12.522	1600	1604	1609	rVB3	11230	19425	0.42%	0.071%
46	12.751	1642	1643	1649	rVB3	4762	5687	0.12%	0.021%
47	12.910	1668	1670	1673	rBV2	5415	6672	0.15%	0.024%
48	13.075	1696	1698	1703	rBV5	3958	5830	0.13%	0.021%
49	13.381	1746	1750	1756	rVB2	33217	46656	1.01%	0.171%
50	13.798	1818	1821	1826	rBV3	9653	12760	0.28%	0.047%
51	13.887	1831	1836	1844	rVB	352149	510532	11.10%	1.867%
52	14.169	1878	1884	1895	rVB	431505	631155	13.73%	2.308%
53	14.475	1929	1936	1944	rBV	1601284	2345944	51.02%	8.577%
54	14.681	1967	1971	1979	rVB2	49912	97427	2.12%	0.356%
55	14.745	1979	1982	1985	rVV4	5337	8299	0.18%	0.030%
56	14.792	1988	1990	1991	rVB2	8330	5433	0.12%	0.020%
57	14.828	1992	1996	2000	rBV2	17980	24256	0.53%	0.089%
58	14.892	2000	2007	2013	rVB4	19783	43012	0.94%	0.157%
59	14.945	2013	2016	2017	rBV	5816	5035	0.11%	0.018%
60	15.081	2035	2039	2041	rBV2	7033	11685	0.25%	0.043%
61	15.192	2054	2058	2064	rVB2	7543	14767	0.32%	0.054%
62	15.322	2079	2080	2084	rVB2	5066	4967	0.11%	0.018%
63	15.469	2096	2105	2110	rBV	520594	779559	16.95%	2.850%
64	15.581	2120	2124	2131	rVB5	29677	48658	1.06%	0.178%
65	15.692	2141	2143	2147	rVB	10202	11629	0.25%	0.043%
66	15.863	2169	2172	2173	rBV2	6688	6938	0.15%	0.025%
67	16.151	2219	2221	2223	rBV2	8254	8250	0.18%	0.030%
68	16.763	2323	2325	2329	rVB5	11556	13097	0.28%	0.048%
69	17.222	2397	2403	2408	rBV	2137486	3023094	65.75%	11.053%
70	17.263	2408	2410	2414	rVV	69800	84049	1.83%	0.307%
71	17.322	2414	2420	2430	rVB	631946	908921	19.77%	3.323%
72	17.986	2531	2533	2541	rVB4	12931	19122	0.42%	0.070%
73	18.116	2550	2555	2562	rBV3	119617	178933	3.89%	0.654%
74	18.433	2606	2609	2621	rVB6	23383	42102	0.92%	0.154%
75	18.669	2646	2649	2656	rVB2	45940	56140	1.22%	0.205%
76	18.886	2683	2686	2690	rVB	40057	42187	0.92%	0.154%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018682.D
Acq On : 07 Dec 2023 20:17
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

77	19.233	2741	2745	2749	rVB	166055	208711	4.54%	0.763%
78	19.345	2761	2764	2769	rBV3	73587	92248	2.01%	0.337%
79	19.557	2795	2800	2814	rBV2	1166392	1662400	36.15%	6.078%
80	21.310	3092	3098	3103	rBV	3424863	4370233	95.04%	15.978%
81	23.521	3469	3474	3480	rBV2	738373	1285231	27.95%	4.699%
82	23.680	3494	3501	3514	rVB	2271294	4598074	100.00%	16.811%




Sum of corrected areas: 27351471

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018682.D
Acq On : 07 Dec 2023 20:17
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

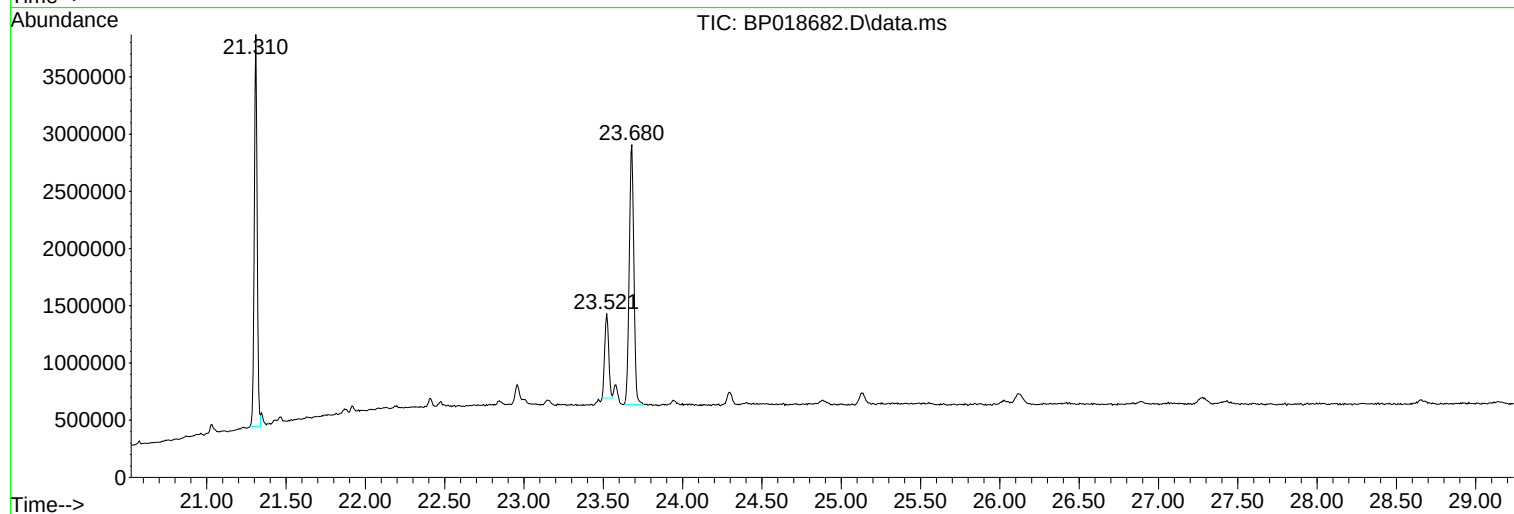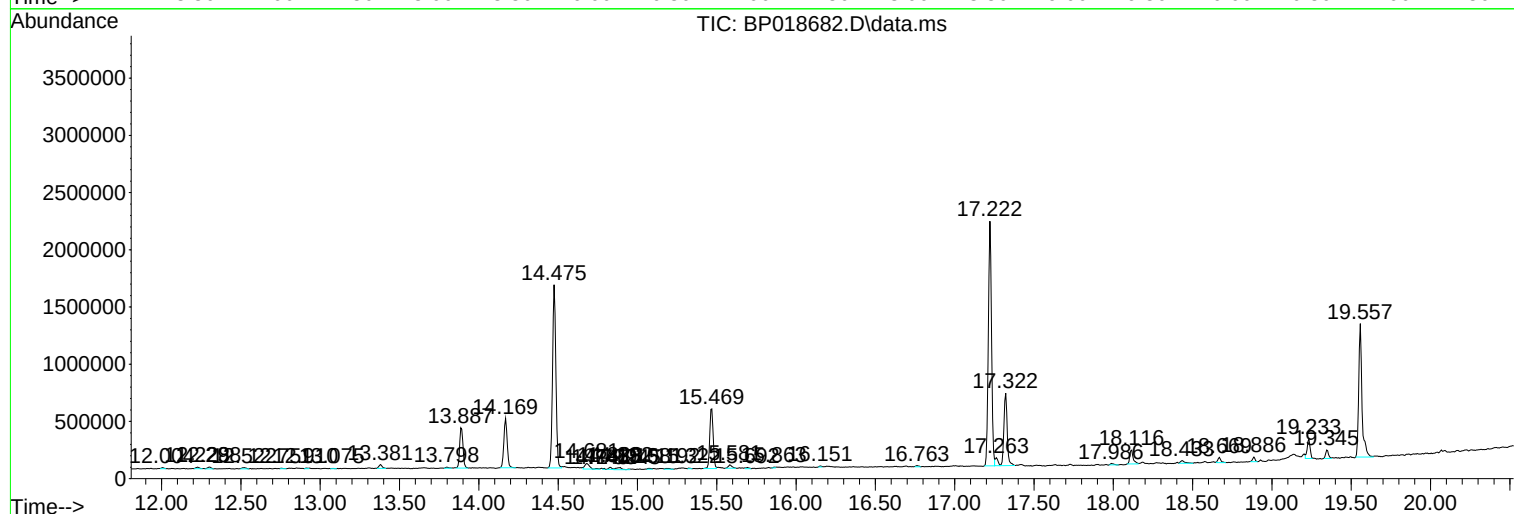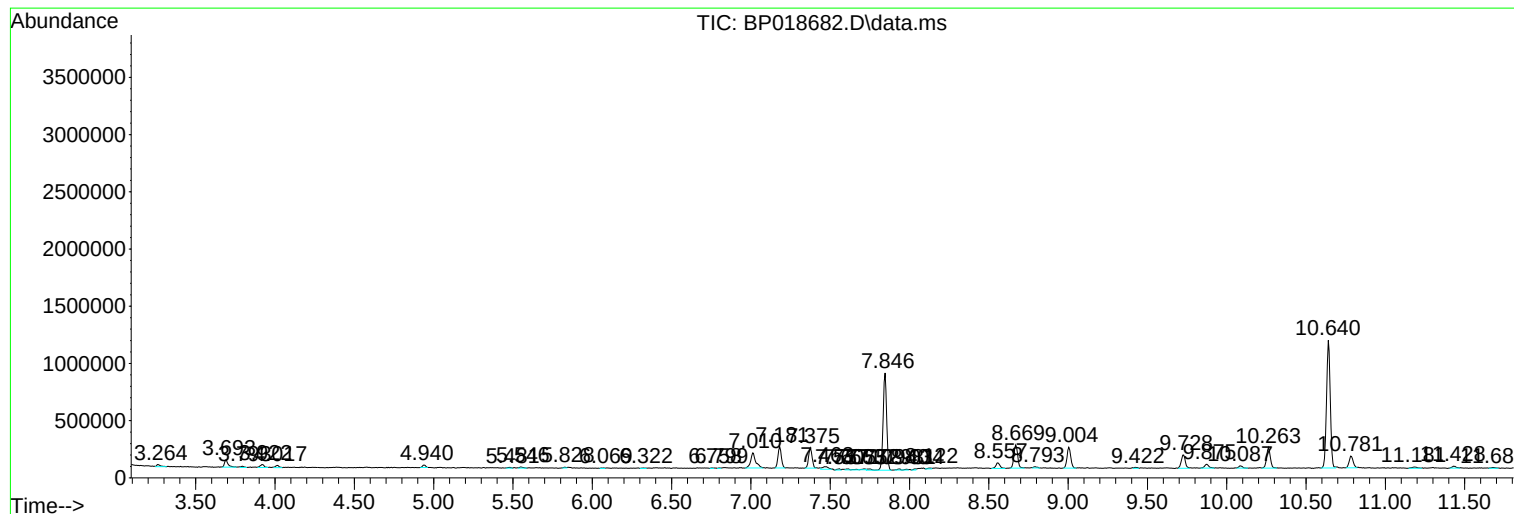

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018682.D
Acq On : 07 Dec 2023 20:17
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018682.D
Acq On : 07 Dec 2023 20:17
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc