

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018689.D
 Acq On : 08 Dec 2023 00:15
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	37	rVB2	22725	35769	0.30%	0.062%
2	3.687	99	102	113	rVB	71565	109784	0.93%	0.190%
3	3.917	137	141	147	rVB2	31986	54825	0.47%	0.095%
4	4.017	153	158	162	rVB	36738	48414	0.41%	0.084%
5	4.240	193	196	201	rVB5	9078	13179	0.11%	0.023%
6	4.393	218	222	227	rVV6	10708	18200	0.15%	0.031%
7	4.458	231	233	241	rVB4	10628	14522	0.12%	0.025%
8	4.940	312	315	320	rVB2	31350	42660	0.36%	0.074%
9	5.470	401	405	410	rBV4	5753	12611	0.11%	0.022%
10	7.011	657	667	681	rVB2	222110	437402	3.72%	0.755%
11	7.181	690	696	703	rBV	244124	365199	3.11%	0.631%
12	7.375	722	729	738	rBV	255891	399599	3.40%	0.690%
13	7.464	738	744	753	rVB4	23459	52487	0.45%	0.091%
14	7.846	799	809	816	rBV	2164564	3402795	28.96%	5.876%
15	8.558	923	930	937	rBV	141414	236450	2.01%	0.408%
16	8.669	943	949	956	rBV	215682	341661	2.91%	0.590%
17	8.799	966	971	977	rVB2	11646	24494	0.21%	0.042%
18	9.005	999	1006	1015	rBV	249238	407152	3.47%	0.703%
19	9.728	1123	1129	1136	rBV2	162243	271546	2.31%	0.469%
20	9.875	1147	1154	1165	rBV2	39040	77031	0.66%	0.133%
21	10.087	1184	1190	1196	rBV2	23913	39370	0.34%	0.068%
22	10.263	1214	1220	1228	rVB	288355	458129	3.90%	0.791%
23	10.640	1276	1284	1291	rBV	2726254	4571023	38.90%	7.894%
24	10.781	1301	1308	1317	rBV	216680	368321	3.13%	0.636%
25	11.181	1369	1376	1381	rBV5	16026	37025	0.32%	0.064%
26	11.434	1415	1419	1428	rBV3	16833	32590	0.28%	0.056%
27	11.669	1454	1459	1463	rBV4	8878	15816	0.13%	0.027%
28	12.228	1546	1554	1560	rBV3	19383	31472	0.27%	0.054%
29	12.304	1562	1567	1572	rVB3	12369	20217	0.17%	0.035%
30	12.522	1599	1604	1608	rVB3	10469	17564	0.15%	0.030%
31	13.381	1744	1750	1756	rVV	32755	52584	0.45%	0.091%
32	13.799	1815	1821	1826	rBV5	11093	20562	0.18%	0.036%
33	13.887	1831	1836	1846	rVB	527832	758732	6.46%	1.310%
34	14.169	1877	1884	1894	rBV	621383	923964	7.86%	1.596%
35	14.475	1928	1936	1946	rBV	4135832	6080127	51.75%	10.500%
36	14.681	1963	1971	1980	rBV	92807	187852	1.60%	0.324%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018689.D
 Acq On : 08 Dec 2023 00:15
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	14.898	2000	2008	2012	rBV6	24066	38971	0.33%	0.067%
38	15.463	2098	2104	2111	rBV	879981	1266376	10.78%	2.187%
39	15.581	2120	2124	2130	rBV	81222	115505	0.98%	0.199%
40	16.622	2299	2301	2306	rVB4	8940	11811	0.10%	0.020%
41	16.687	2308	2312	2315	rBV2	8246	12613	0.11%	0.022%
42	17.004	2363	2366	2371	rVB2	11452	15196	0.13%	0.026%
43	17.222	2397	2403	2409	rBV	5365028	7768100	66.12%	13.415%
44	17.263	2409	2410	2414	rVV	65671	59142	0.50%	0.102%
45	17.322	2414	2420	2430	rVV	932525	1335884	11.37%	2.307%
46	17.416	2433	2436	2442	rVB3	19306	26891	0.23%	0.046%
47	17.728	2484	2489	2493	rBV4	17916	33488	0.29%	0.058%
48	17.904	2515	2519	2522	rVB3	19488	25783	0.22%	0.045%
49	17.992	2530	2534	2540	rBV4	19726	36484	0.31%	0.063%
50	18.116	2548	2555	2563	rBV2	148205	249909	2.13%	0.432%
51	18.275	2579	2582	2586	rBV4	12722	16071	0.14%	0.028%
52	18.316	2586	2589	2592	rVB4	13741	17983	0.15%	0.031%
53	18.669	2646	2649	2657	rVB	45853	59212	0.50%	0.102%
54	18.886	2683	2686	2690	rVB	38909	44813	0.38%	0.077%
55	19.204	2737	2740	2742	rBV	32082	39525	0.34%	0.068%
56	19.234	2742	2745	2753	rVB	113536	147109	1.25%	0.254%
57	19.345	2761	2764	2768	rBV3	57561	76715	0.65%	0.132%
58	19.557	2795	2800	2814	rBV	1604567	2152309	18.32%	3.717%
59	21.028	3047	3050	3059	rBV3	103248	180523	1.54%	0.312%
60	21.310	3093	3098	3109	rVB	8482908	10424805	88.73%	18.003%
61	23.522	3468	3474	3480	rBV2	1080893	2021089	17.20%	3.490%
62	23.686	3493	3502	3514	rVB	5751361	11749363	100.00%	20.290%




Sum of corrected areas: 57906798

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018689.D
Acq On : 08 Dec 2023 00:15
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

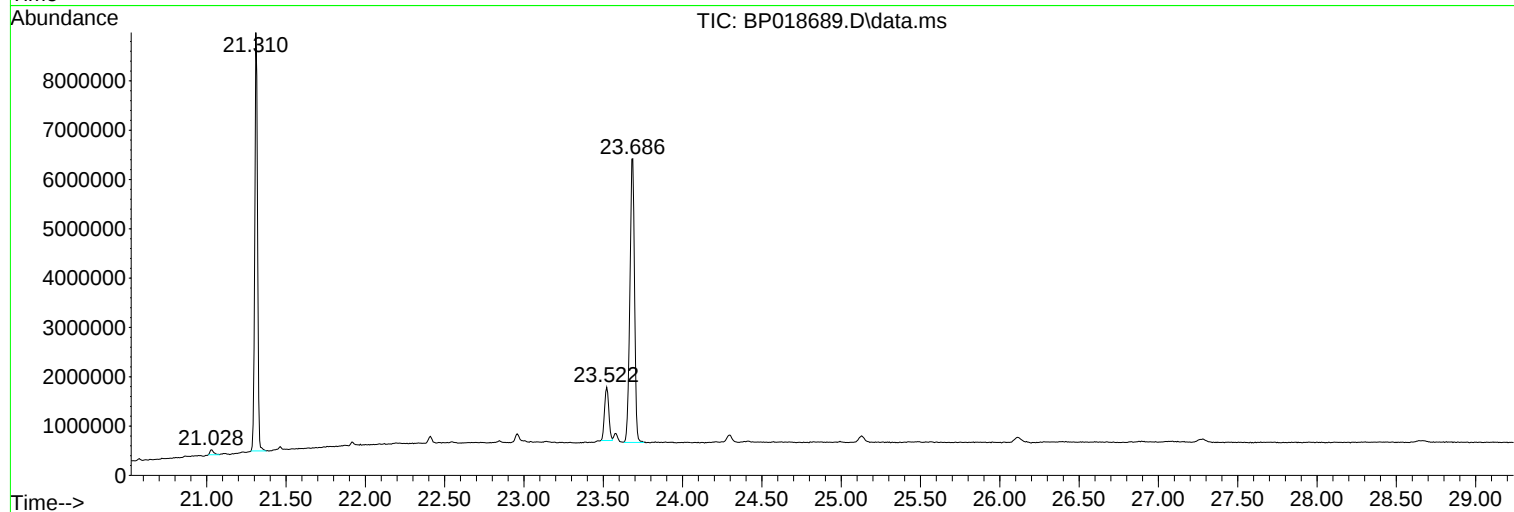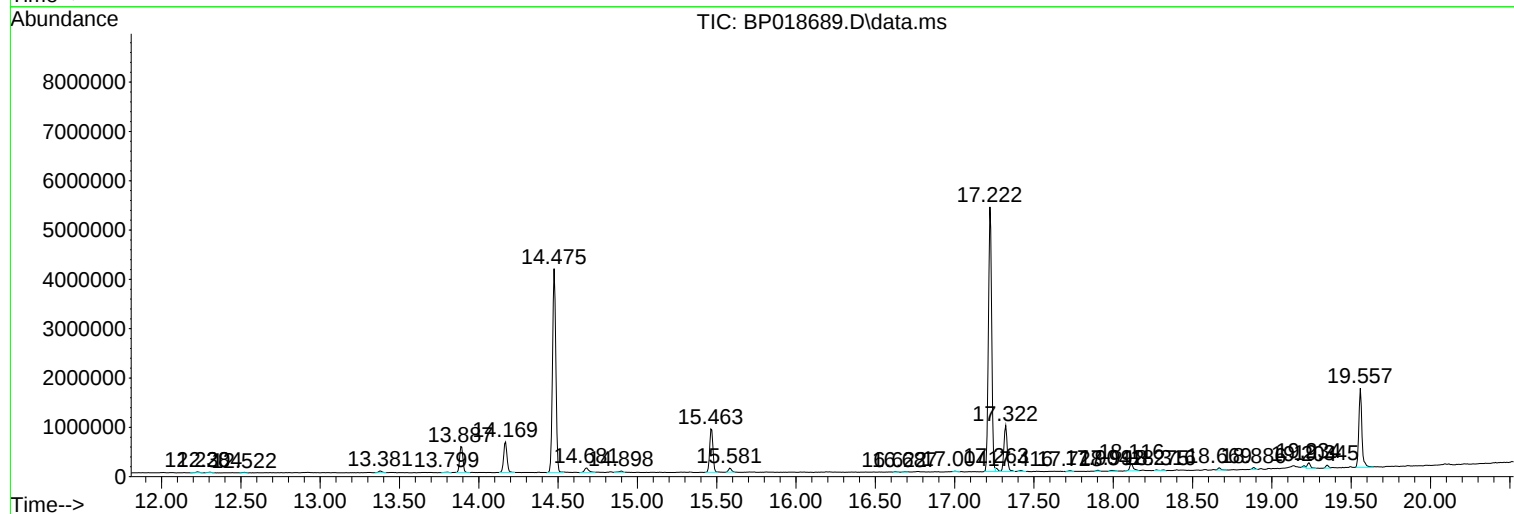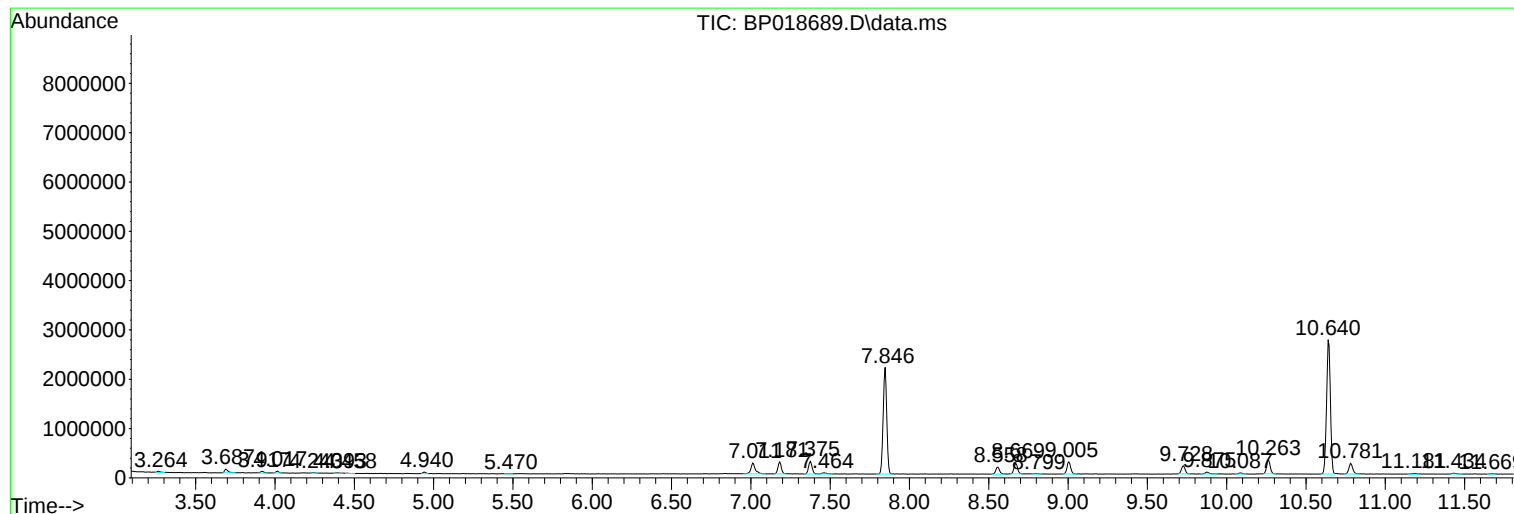

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018689.D
Acq On : 08 Dec 2023 00:15
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018689.D
Acq On : 08 Dec 2023 00:15
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc