

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018693.D
 Acq On : 08 Dec 2023 03:04
 Operator : MA/JU
 Sample : PB157493BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK493

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	26	30	35	rVB	93529	112432	1.26%	0.146%
2	3.681	97	101	119	rBV	1068175	1550203	17.39%	2.007%
3	4.010	154	157	162	rVB2	19025	25015	0.28%	0.032%
4	5.875	471	474	475	rBV	9879	10162	0.11%	0.013%
5	7.010	661	667	677	rVB	1138948	1758564	19.73%	2.277%
6	7.181	690	696	707	rVB	961448	1437956	16.13%	1.862%
7	7.375	722	729	739	rBV	1157663	1789061	20.07%	2.317%
8	7.845	802	809	816	rVB	1192945	1860341	20.87%	2.409%
9	8.216	869	872	876	rVB	7908	11269	0.13%	0.015%
10	8.422	903	907	909	rBV5	8037	13462	0.15%	0.017%
11	8.557	922	930	940	rBV	1329727	2163041	24.26%	2.801%
12	9.004	999	1006	1016	rVB	1009287	1609471	18.05%	2.084%
13	9.728	1121	1129	1138	rBV	749483	1240662	13.92%	1.607%
14	10.263	1210	1220	1229	rBV	1272784	2130324	23.90%	2.759%
15	10.639	1276	1284	1292	rBV	1529533	2480715	27.83%	3.212%
16	10.781	1299	1308	1321	rBV	1343248	2263670	25.39%	2.931%
17	12.228	1549	1554	1560	rVB3	21773	38015	0.43%	0.049%
18	13.380	1745	1750	1755	rVB3	19174	34437	0.39%	0.045%
19	13.892	1830	1837	1845	rBV	2200750	3051244	34.23%	3.951%
20	13.992	1852	1854	1862	rVB3	5921	9937	0.11%	0.013%
21	14.169	1877	1884	1894	rBV	2576560	3706558	41.58%	4.800%
22	14.475	1929	1936	1944	rBV	2231941	3266682	36.64%	4.230%
23	14.675	1964	1970	1986	rBV	1101822	1694213	19.00%	2.194%
24	15.469	2098	2105	2116	rBV	3194637	4761284	53.41%	6.166%
25	15.586	2118	2125	2136	rBV	917433	1252547	14.05%	1.622%
26	15.704	2141	2145	2150	rVB4	16976	27478	0.31%	0.036%
27	17.221	2396	2403	2413	rBV	3110572	4260689	47.79%	5.517%
28	17.321	2413	2420	2434	rBV	4116072	5648154	63.35%	7.314%
29	17.610	2465	2469	2471	rBV3	6358	9717	0.11%	0.013%
30	18.110	2551	2554	2558	rVB3	19063	24150	0.27%	0.031%
31	18.239	2574	2576	2578	rBV2	11578	13580	0.15%	0.018%
32	18.280	2579	2583	2584	rVV2	10608	14051	0.16%	0.018%
33	19.133	2724	2728	2733	rBV4	59195	77880	0.87%	0.101%
34	19.198	2736	2739	2743	rVV	53671	71803	0.81%	0.093%
35	19.557	2794	2800	2809	rBV	5992121	7633614	85.62%	9.885%
36	21.309	3093	3098	3104	rBV	4763732	5776726	64.80%	7.481%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018693.D
Acq On : 08 Dec 2023 03:04
Operator : MA/JU
Sample : PB157493BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK493

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	23.527	3467	3475	3481	rBV2	4572482	8915237	100.00%	11.545%
38	23.680	3494	3501	3514	rVB	3244094	6478292	72.67%	8.389%




Sum of corrected areas: 77222636

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018693.D
Acq On : 08 Dec 2023 03:04
Operator : MA/JU
Sample : PB157493BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

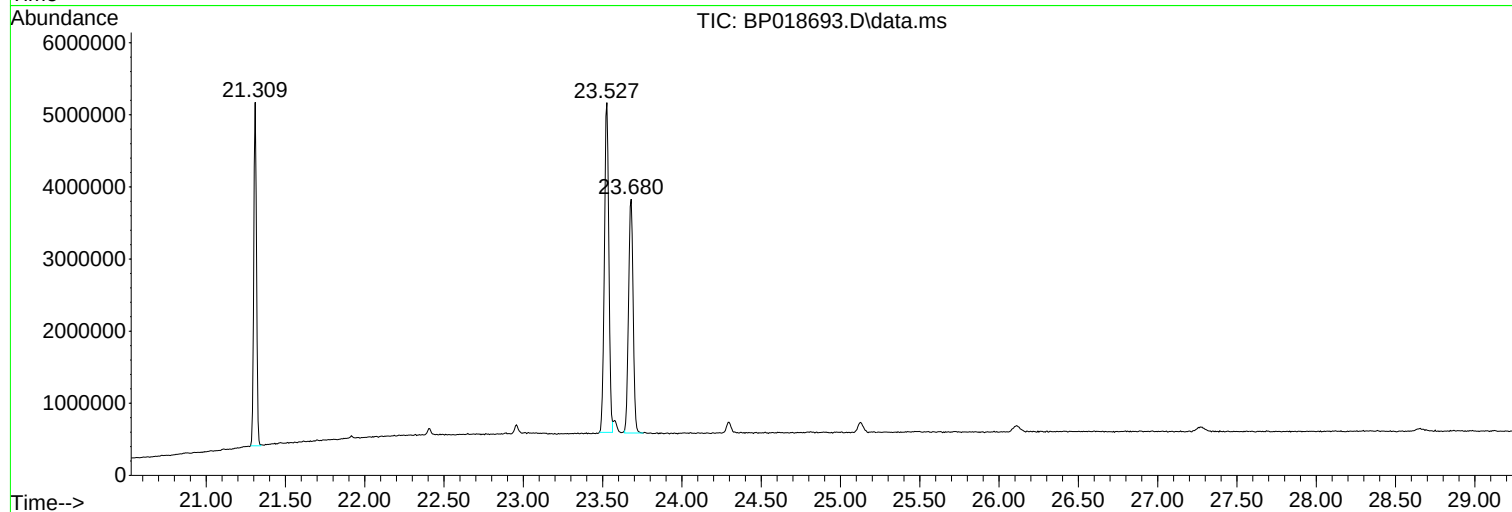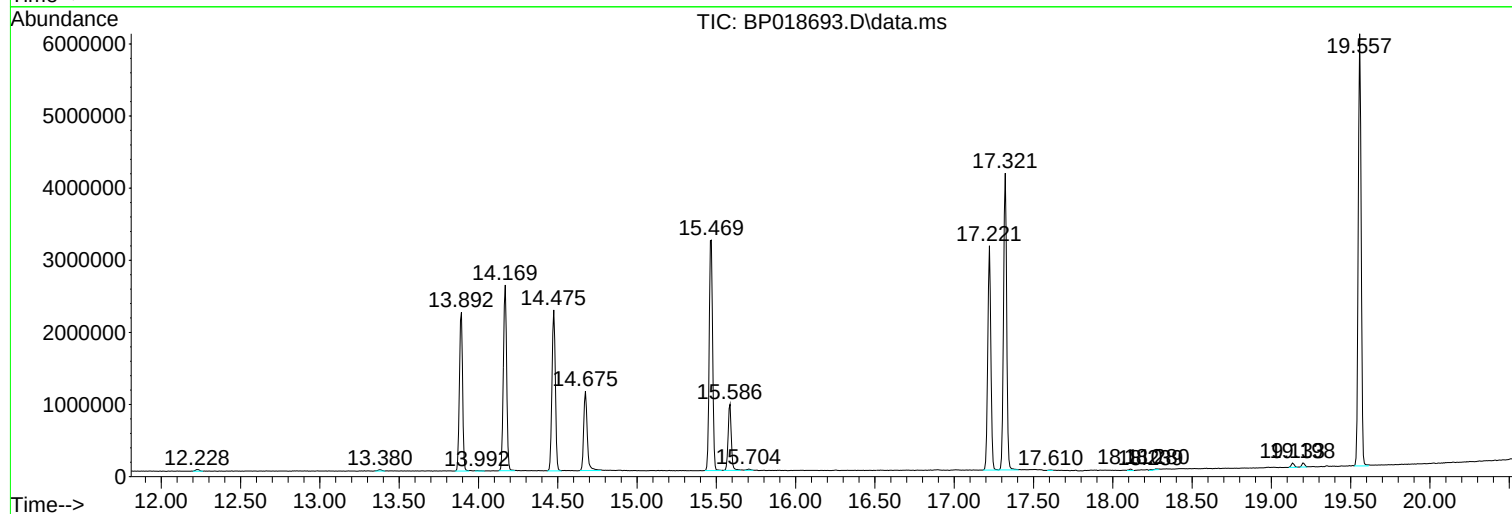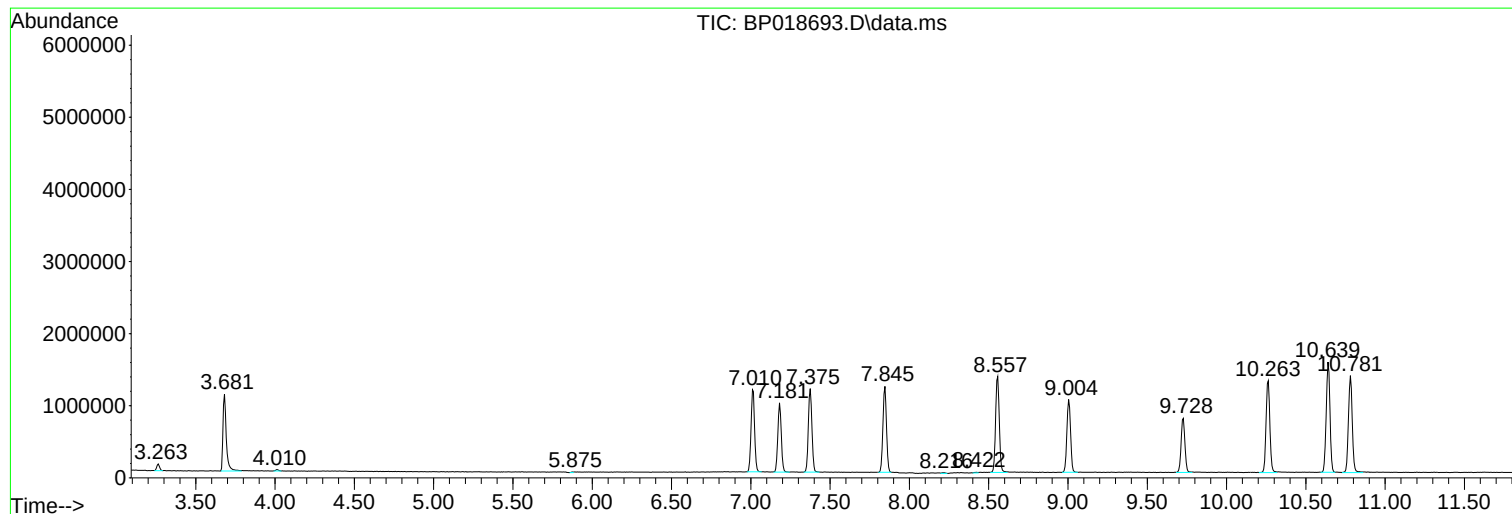

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018693.D
Acq On : 08 Dec 2023 03:04
Operator : MA/JU
Sample : PB157493BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018693.D
Acq On : 08 Dec 2023 03:04
Operator : MA/JU
Sample : PB157493BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc