

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018701.D
 Acq On : 08 Dec 2023 07:35
 Operator : MA/JU
 Sample : 05497-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018701.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	34	rVB2	11245	15486	0.34%	0.056%
2	3.693	99	103	111	rBV	39316	61248	1.33%	0.221%
3	3.793	118	120	124	rVB3	6867	7576	0.17%	0.027%
4	3.869	130	133	135	rBV3	3837	4904	0.11%	0.018%
5	3.922	137	142	148	rVB	25954	40056	0.87%	0.144%
6	4.016	154	158	163	rVB2	16267	25874	0.56%	0.093%
7	4.240	195	196	200	rVB3	6046	7614	0.17%	0.027%
8	4.758	280	284	286	rBV3	5098	6939	0.15%	0.025%
9	4.940	310	315	319	rBV2	21161	33054	0.72%	0.119%
10	5.205	355	360	362	rBV4	4137	5221	0.11%	0.019%
11	5.481	400	407	408	rBV5	4729	7161	0.16%	0.026%
12	5.552	416	419	426	rVB4	4804	7887	0.17%	0.028%
13	5.828	462	466	468	rBV4	8755	13807	0.30%	0.050%
14	5.928	482	483	488	rVB2	4473	5354	0.12%	0.019%
15	6.452	569	572	575	rBV3	4780	5719	0.12%	0.021%
16	6.834	635	637	643	rVB4	5459	7219	0.16%	0.026%
17	7.010	658	667	681	rVB2	141610	310173	6.76%	1.118%
18	7.181	690	696	706	rVB	143249	217675	4.74%	0.785%
19	7.375	723	729	739	rBV	162750	259531	5.65%	0.936%
20	7.469	742	745	750	rBV4	9164	13830	0.30%	0.050%
21	7.652	773	776	783	rVB5	3827	7795	0.17%	0.028%
22	7.846	802	809	818	rVB	823014	1306796	28.47%	4.712%
23	8.557	922	930	938	rBV	70275	117289	2.56%	0.423%
24	8.669	943	949	960	rVB	228148	362764	7.90%	1.308%
25	8.781	965	968	969	rBV2	7127	5735	0.12%	0.021%
26	9.004	998	1006	1014	rBV	161120	256597	5.59%	0.925%
27	9.069	1014	1017	1021	rVB4	3441	4725	0.10%	0.017%
28	9.416	1070	1076	1080	rBV4	4435	9842	0.21%	0.035%
29	9.722	1122	1128	1136	rVB	102497	179418	3.91%	0.647%
30	9.875	1147	1154	1162	rBV2	39314	80299	1.75%	0.290%
31	9.963	1165	1169	1174	rVV4	5176	10535	0.23%	0.038%
32	10.028	1177	1180	1185	rBV5	2802	5127	0.11%	0.018%
33	10.087	1185	1190	1198	rVV3	23867	40222	0.88%	0.145%
34	10.210	1206	1211	1212	rBV2	4576	5637	0.12%	0.020%
35	10.263	1214	1220	1228	rVV	178129	300141	6.54%	1.082%
36	10.640	1276	1284	1291	rBV	1041602	1714089	37.34%	6.181%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018701.D
 Acq On : 08 Dec 2023 07:35
 Operator : MA/JU
 Sample : 05497-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	10.693	1292	1293	1299	rVB2	10709	8998	0.20%	0.032%
38	10.781	1302	1308	1315	rBV	92043	165205	3.60%	0.596%
39	11.181	1372	1376	1382	rVV5	11522	23585	0.51%	0.085%
40	11.428	1410	1418	1426	rBV	17683	38966	0.85%	0.141%

41	11.740	1467	1471	1475	rBV	3152	6198	0.14%	0.022%
42	12.004	1513	1516	1520	rVB4	7747	12498	0.27%	0.045%
43	12.304	1561	1567	1574	rVB3	11227	22523	0.49%	0.081%
44	12.522	1598	1604	1609	rVB2	11850	20195	0.44%	0.073%
45	12.822	1650	1655	1656	rBV3	3428	5551	0.12%	0.020%

46	12.910	1668	1670	1677	rVB2	8878	13543	0.30%	0.049%
47	13.304	1735	1737	1742	rVB3	6585	8205	0.18%	0.030%
48	13.381	1742	1750	1756	rBV2	58455	98161	2.14%	0.354%
49	13.645	1787	1795	1796	rBV5	6054	13197	0.29%	0.048%
50	13.751	1808	1813	1814	rBV	4119	5682	0.12%	0.020%

51	13.798	1814	1821	1826	rVV7	11379	23312	0.51%	0.084%
52	13.845	1826	1829	1830	rVV4	6217	6221	0.14%	0.022%
53	13.886	1831	1836	1845	rVV	355886	501650	10.93%	1.809%
54	13.969	1845	1850	1852	rVB2	5565	6524	0.14%	0.024%
55	14.028	1858	1860	1863	rVB2	5211	4959	0.11%	0.018%

56	14.169	1876	1884	1893	rBV	392268	603215	13.14%	2.175%
57	14.381	1917	1920	1923	rVB	7737	9198	0.20%	0.033%
58	14.475	1929	1936	1943	rBV	1602158	2313303	50.40%	8.342%
59	14.681	1964	1971	1979	rBV2	63342	123708	2.70%	0.446%
60	14.828	1992	1996	2001	rBV3	13903	23274	0.51%	0.084%

61	14.875	2001	2004	2005	rVV2	8906	10496	0.23%	0.038%
62	14.898	2005	2008	2014	rVB5	20166	30304	0.66%	0.109%
63	15.328	2078	2081	2084	rVB5	6969	9449	0.21%	0.034%
64	15.463	2097	2104	2110	rBV	557934	823255	17.94%	2.969%
65	15.510	2110	2112	2118	rVV4	10784	16764	0.37%	0.060%

66	15.581	2118	2124	2132	rVV2	46690	76428	1.67%	0.276%
67	15.816	2162	2164	2171	rVB4	4919	8152	0.18%	0.029%
68	15.963	2187	2189	2194	rVB3	4118	4820	0.11%	0.017%
69	16.192	2224	2228	2229	rBV4	7147	9067	0.20%	0.033%
70	16.310	2242	2248	2249	rBV4	3264	4960	0.11%	0.018%

71	16.622	2298	2301	2305	rVB3	6110	8279	0.18%	0.030%
72	16.686	2309	2312	2317	rVV3	6945	11107	0.24%	0.040%
73	16.769	2321	2326	2332	rBV6	11929	20532	0.45%	0.074%
74	16.986	2360	2363	2365	rBV3	8131	10124	0.22%	0.037%
75	17.039	2369	2372	2375	rVB2	7288	9119	0.20%	0.033%

76	17.116	2384	2385	2388	rBV3	6200	4942	0.11%	0.018%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018701.D
 Acq On : 08 Dec 2023 07:35
 Operator : MA/JU
 Sample : 05497-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	17.222	2395	2403	2408	rBV	2267347	3135535	68.31%	11.307%
78	17.263	2408	2410	2414	rVV	101457	121978	2.66%	0.440%
79	17.322	2414	2420	2430	rVV	634158	923846	20.13%	3.331%
80	17.416	2434	2436	2441	rVB5	16121	22901	0.50%	0.083%
81	17.627	2470	2472	2475	rVB3	7356	8291	0.18%	0.030%
82	17.727	2485	2489	2494	rBV5	16096	24694	0.54%	0.089%
83	17.898	2515	2518	2521	rVB5	10973	12127	0.26%	0.044%
84	17.986	2529	2533	2538	rBV2	22147	37674	0.82%	0.136%
85	18.110	2548	2554	2563	rBV2	154922	241699	5.27%	0.872%
86	18.269	2578	2581	2586	rBV6	11676	21322	0.46%	0.077%
87	18.398	2601	2603	2606	rBV4	9420	10061	0.22%	0.036%
88	18.574	2630	2633	2637	rBV2	13568	17183	0.37%	0.062%
89	18.669	2645	2649	2658	rVB3	46116	66799	1.46%	0.241%
90	18.886	2682	2686	2690	rBV	47560	57337	1.25%	0.207%
91	18.933	2690	2694	2697	rBV3	18270	23033	0.50%	0.083%
92	19.233	2741	2745	2754	rVB	195981	250373	5.45%	0.903%
93	19.345	2761	2764	2772	rBV2	70792	89442	1.95%	0.323%
94	19.557	2795	2800	2813	rBV2	1060934	1568703	34.18%	5.657%
95	21.027	3047	3050	3057	rBV5	77180	117257	2.55%	0.423%
96	21.310	3092	3098	3103	rBV	3404316	4484726	97.70%	16.172%
97	23.521	3468	3474	3480	rBV2	691580	1327797	28.93%	4.788%
98	23.680	3493	3501	3509	rBV	2251011	4590093	100.00%	16.552%


Sum of corrected areas: 27731879

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018701.D
Acq On : 08 Dec 2023 07:35
Operator : MA/JU
Sample : 05497-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

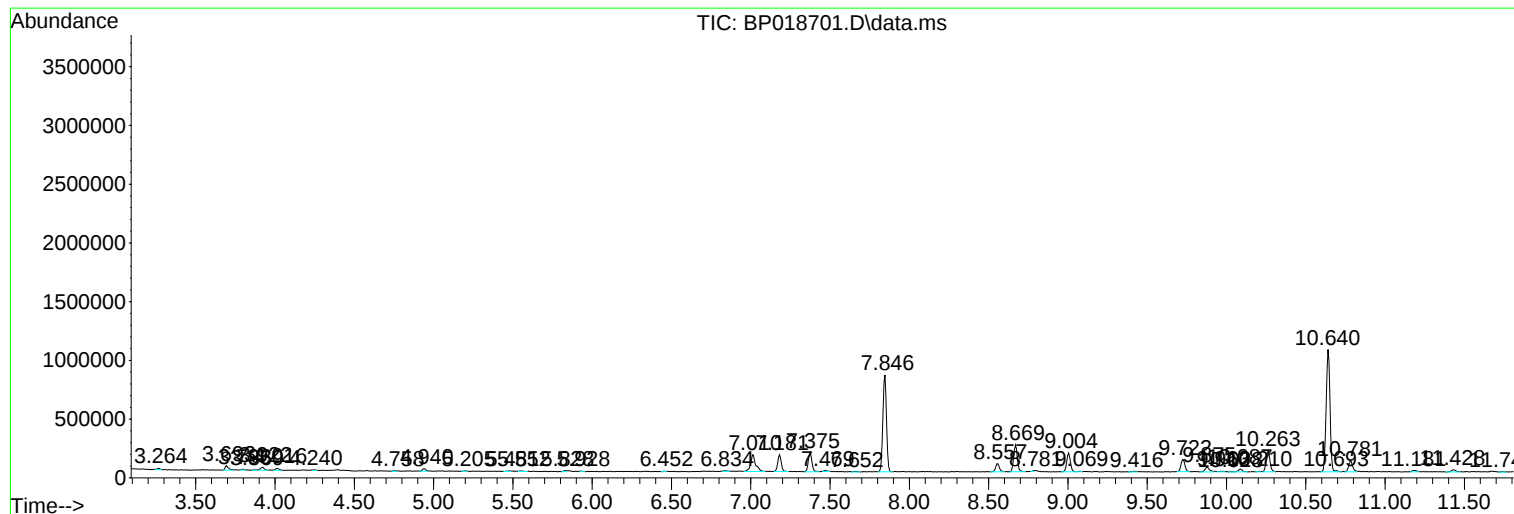

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018701.D
Acq On : 08 Dec 2023 07:35
Operator : MA/JU
Sample : 05497-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018701.D
Acq On : 08 Dec 2023 07:35
Operator : MA/JU
Sample : 05497-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------