

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018705.D
 Acq On : 08 Dec 2023 10:24
 Operator : MA/JU
 Sample : PB157408BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK408

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018705.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	36	rVB	80675	108064	1.05%	0.142%
2	3.681	97	101	121	rVB	1011374	1486025	14.47%	1.956%
3	4.017	153	158	164	rVB3	15987	32542	0.32%	0.043%
4	4.346	211	214	218	rVB2	18964	25147	0.24%	0.033%
5	5.117	338	345	346	rBV	8232	14344	0.14%	0.019%
6	5.387	383	391	394	rBV	9552	18873	0.18%	0.025%
7	5.446	395	401	404	rVV2	9502	23997	0.23%	0.032%
8	5.499	407	410	412	rVV	10337	13313	0.13%	0.018%
9	7.011	661	667	676	rBV	1118937	1762895	17.16%	2.320%
10	7.181	690	696	704	rVB	913448	1383118	13.47%	1.820%
11	7.375	722	729	738	rBV	1141162	1761238	17.15%	2.318%
12	7.846	802	809	817	rBV	805701	1274233	12.41%	1.677%
13	8.187	865	867	870	rVB	10232	10497	0.10%	0.014%
14	8.434	904	909	910	rBV	8003	10891	0.11%	0.014%
15	8.558	922	930	939	rBV	1123722	1844248	17.96%	2.427%
16	8.699	946	954	955	rBV	11739	22604	0.22%	0.030%
17	9.005	999	1006	1014	rBV	1053004	1673683	16.29%	2.203%
18	9.728	1121	1129	1137	rBV	810910	1326862	12.92%	1.746%
19	10.263	1212	1220	1230	rBV	1393264	2285540	22.25%	3.008%
20	10.640	1277	1284	1294	rVB	1061980	1740233	16.94%	2.290%
21	10.781	1301	1308	1320	rVB	1453246	2410344	23.47%	3.172%
22	12.222	1550	1553	1557	rBV2	26503	33742	0.33%	0.044%
23	12.310	1565	1568	1572	rVB	14580	17902	0.17%	0.024%
24	12.716	1634	1637	1639	rBV	8678	13916	0.14%	0.018%
25	13.381	1746	1750	1754	rVB2	12761	18841	0.18%	0.025%
26	13.893	1830	1837	1843	rBV	2529943	3549414	34.56%	4.672%
27	14.169	1877	1884	1891	rBV	2876820	4252821	41.41%	5.598%
28	14.475	1929	1936	1945	rVB	1574686	2347469	22.85%	3.090%
29	14.675	1964	1970	1986	rBV	1391150	2056817	20.03%	2.707%
30	15.463	2098	2104	2113	rBV	3752893	5540495	53.94%	7.292%
31	15.587	2119	2125	2136	rBV	1075378	1518811	14.79%	1.999%
32	15.704	2143	2145	2150	rVB2	22704	25287	0.25%	0.033%
33	16.898	2344	2348	2354	rBV3	9866	15707	0.15%	0.021%
34	17.222	2397	2403	2411	rBV	2101018	3052391	29.72%	4.018%
35	17.322	2413	2420	2432	rVV	4973767	6769855	65.91%	8.910%
36	18.110	2551	2554	2559	rVB6	18355	25821	0.25%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018705.D
Acq On : 08 Dec 2023 10:24
Operator : MA/JU
Sample : PB157408BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK408

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.133	2724	2728	2732	rBV2	72437	94569	0.92%	0.124%
38	19.204	2736	2740	2745	rVV	66252	88425	0.86%	0.116%
39	19.557	2794	2800	2809	rBV	6894862	8941351	87.05%	11.769%
40	21.310	3093	3098	3104	rBV	3165464	3871688	37.69%	5.096%
41	23.527	3467	3475	3490	rVB2	5061569	10271201	100.00%	13.519%
42	23.680	3494	3501	3514	rVB	2179003	4241183	41.29%	5.582%




Sum of corrected areas: 75976397

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018705.D
Acq On : 08 Dec 2023 10:24
Operator : MA/JU
Sample : PB157408BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

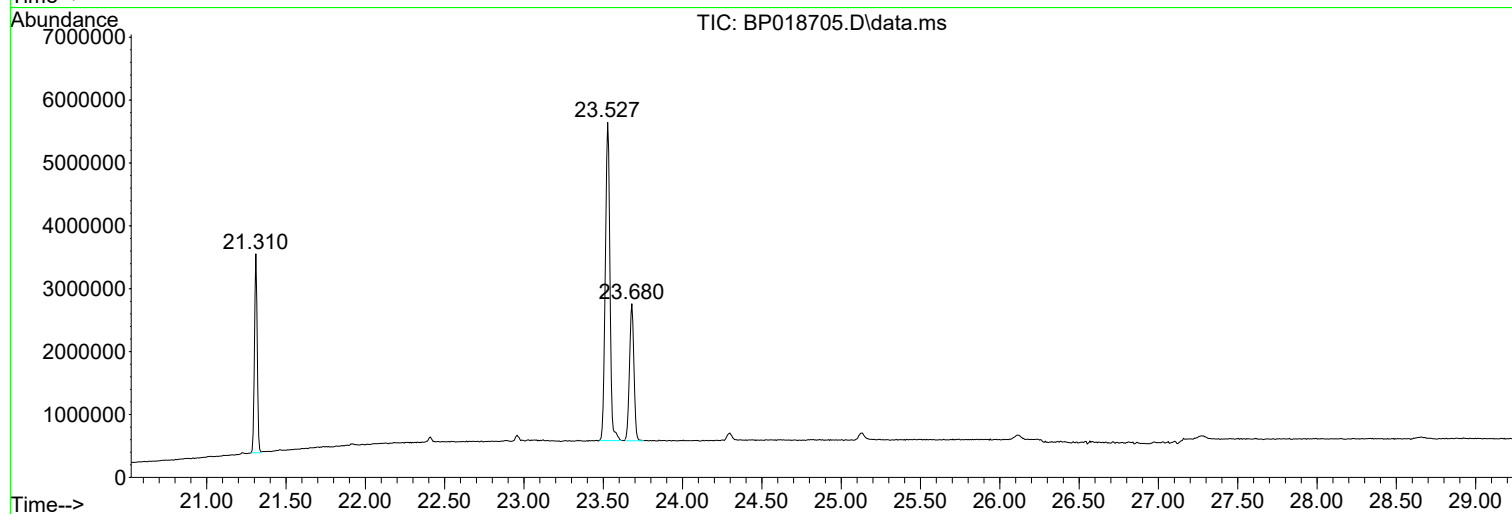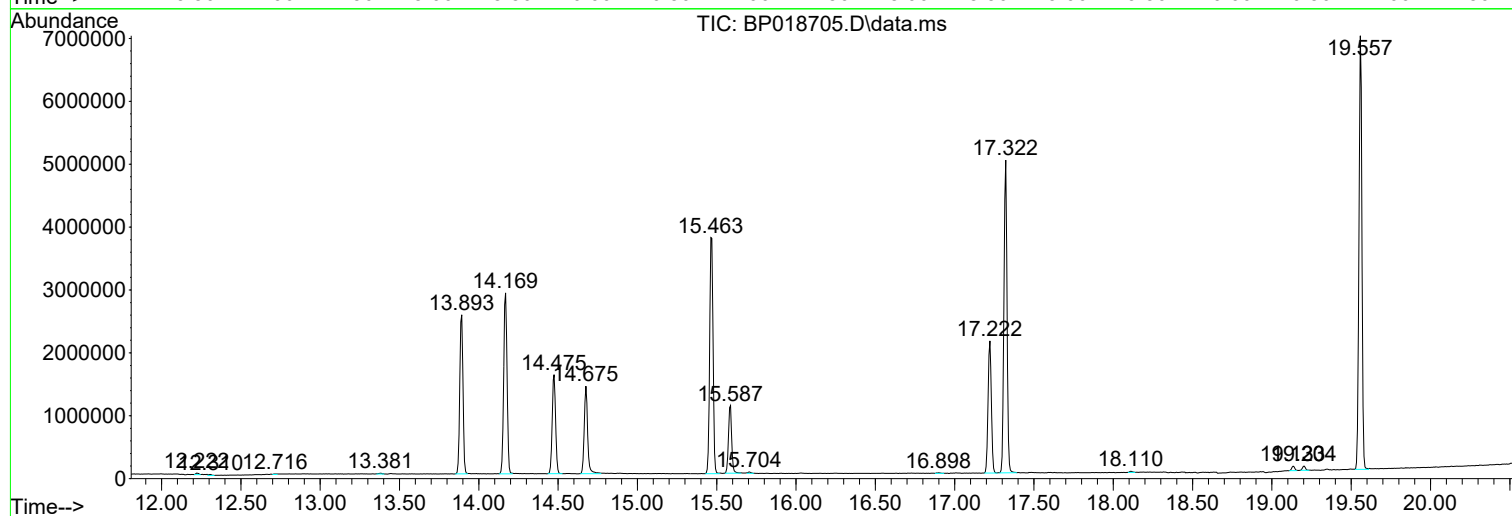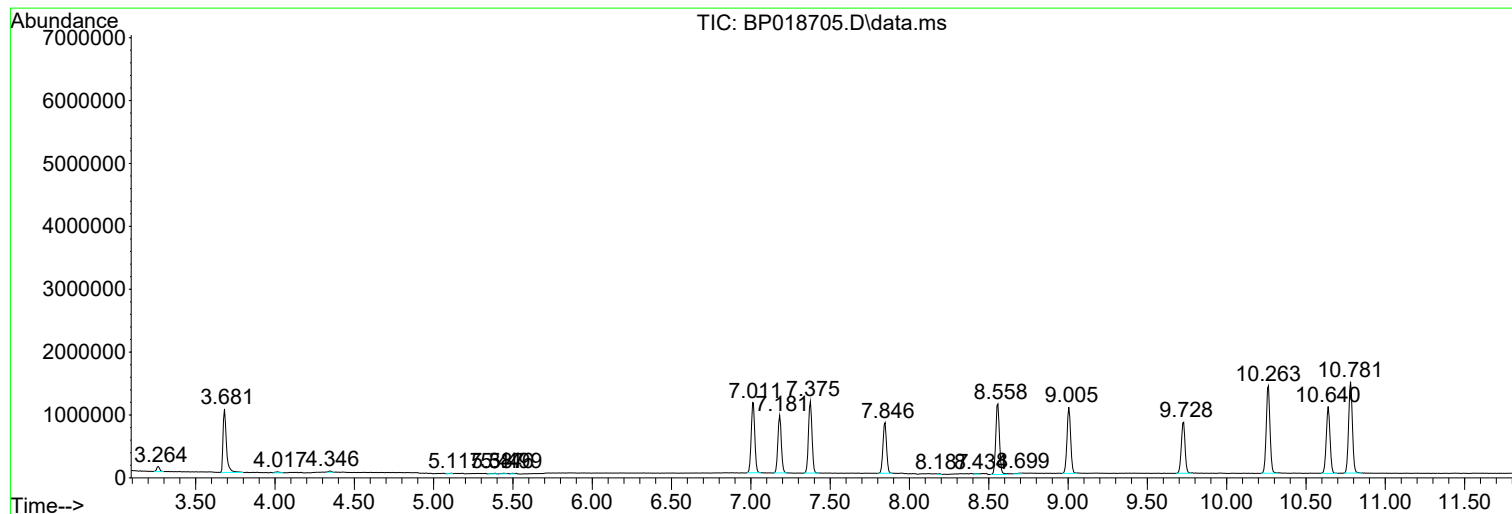

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018705.D
Acq On : 08 Dec 2023 10:24
Operator : MA/JU
Sample : PB157408BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018705.D
Acq On : 08 Dec 2023 10:24
Operator : MA/JU
Sample : PB157408BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------