

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018706.D
 Acq On : 08 Dec 2023 10:58
 Operator : MA/JU
 Sample : 05497-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	35	rVB2	21172	24795	0.41%	0.046%
2	3.693	99	103	116	rVV	56554	91408	1.52%	0.170%
3	3.799	118	121	125	rVB	17792	21610	0.36%	0.040%
4	3.922	137	142	146	rVB	32462	51027	0.85%	0.095%
5	4.017	154	158	163	rBV2	27603	40391	0.67%	0.075%
6	4.940	308	315	319	rBV3	22577	36078	0.60%	0.067%
7	5.028	326	330	335	rBV5	8233	15435	0.26%	0.029%
8	5.481	404	407	412	rVB3	7518	12034	0.20%	0.022%
9	5.852	461	470	477	rBV6	17277	33585	0.56%	0.063%
10	6.658	598	607	608	rBV	19557	43847	0.73%	0.082%
11	7.011	659	667	683	rVB	512994	917735	15.21%	1.709%
12	7.181	689	696	703	rBV	498741	759280	12.59%	1.414%
13	7.375	722	729	736	rBV	541166	850617	14.10%	1.584%
14	7.469	740	745	753	rVB4	22970	47840	0.79%	0.089%
15	7.846	801	809	817	rVB	1156316	1834758	30.42%	3.416%
16	7.952	825	827	830	rBV4	6804	9089	0.15%	0.017%
17	8.552	923	929	937	rBV	434024	686473	11.38%	1.278%
18	8.669	943	949	957	rVB	297061	469906	7.79%	0.875%
19	8.799	967	971	977	rBV3	13782	27713	0.46%	0.052%
20	9.005	999	1006	1014	rBV	541281	871477	14.45%	1.623%
21	9.069	1014	1017	1021	rVB5	10446	15769	0.26%	0.029%
22	9.246	1045	1047	1049	rBV	6949	6808	0.11%	0.013%
23	9.722	1122	1128	1137	rBV	391332	641999	10.64%	1.195%
24	9.881	1147	1155	1161	rBV2	49305	99426	1.65%	0.185%
25	10.081	1185	1189	1197	rVB2	29315	51489	0.85%	0.096%
26	10.257	1212	1219	1230	rVB	632720	1039749	17.24%	1.936%
27	10.640	1276	1284	1290	rBV	1536418	2551128	42.29%	4.750%
28	10.687	1290	1292	1298	rVB	48986	70116	1.16%	0.131%
29	10.781	1300	1308	1317	rBV	501184	875687	14.52%	1.630%
30	11.181	1372	1376	1382	rBV3	18684	30842	0.51%	0.057%
31	11.428	1414	1418	1426	rVB2	24267	44905	0.74%	0.084%
32	11.669	1456	1459	1468	rVB4	13949	30417	0.50%	0.057%
33	12.010	1511	1517	1520	rBV	12460	21784	0.36%	0.041%
34	12.069	1522	1527	1530	rVB2	13642	19784	0.33%	0.037%
35	12.298	1561	1566	1574	rVB	51595	86077	1.43%	0.160%
36	12.516	1599	1603	1609	rVB	40857	62121	1.03%	0.116%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018706.D
 Acq On : 08 Dec 2023 10:58
 Operator : MA/JU
 Sample : 05497-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	12.910	1667	1670	1675	rVB4	6445	10310	0.17%	0.019%
38	13.016	1685	1688	1693	rBV3	8976	13468	0.22%	0.025%
39	13.304	1733	1737	1743	rVB5	24498	37956	0.63%	0.071%
40	13.375	1743	1749	1756	rBV	71292	122255	2.03%	0.228%
41	13.634	1790	1793	1796	rBV3	11841	20703	0.34%	0.039%
42	13.798	1816	1821	1826	rBV2	30788	51018	0.85%	0.095%
43	13.845	1826	1829	1831	rVV	21945	28029	0.46%	0.052%
44	13.887	1831	1836	1844	rVV	1174416	1629138	27.01%	3.033%
45	13.963	1846	1849	1852	rVB3	16915	19595	0.32%	0.036%
46	14.034	1857	1861	1866	rVB3	15086	19256	0.32%	0.036%
47	14.169	1877	1884	1897	rVB	1404768	2077278	34.44%	3.868%
48	14.375	1916	1919	1925	rVB2	20878	31329	0.52%	0.058%
49	14.475	1928	1936	1943	rVV	2366916	3427569	56.82%	6.382%
50	14.540	1943	1947	1951	rVB3	14746	25031	0.41%	0.047%
51	14.675	1964	1970	1981	rBV	274215	471840	7.82%	0.879%
52	14.828	1992	1996	1999	rBV2	28188	38931	0.65%	0.072%
53	14.875	1999	2004	2006	rBV	33138	48538	0.80%	0.090%
54	15.145	2046	2050	2053	rVB4	11707	16535	0.27%	0.031%
55	15.257	2063	2069	2073	rBV4	19085	36086	0.60%	0.067%
56	15.328	2078	2081	2084	rVB	20866	24274	0.40%	0.045%
57	15.410	2093	2095	2097	rBV	6392	6227	0.10%	0.012%
58	15.463	2097	2104	2110	rVV	1864853	2703913	44.82%	5.034%
59	15.516	2110	2113	2119	rVV4	37437	59316	0.98%	0.110%
60	15.581	2119	2124	2132	rVV	215938	308227	5.11%	0.574%
61	15.810	2160	2163	2171	rVB2	20638	36785	0.61%	0.068%
62	15.957	2185	2188	2196	rVB3	19814	43908	0.73%	0.082%
63	16.192	2224	2228	2229	rBV	28960	33937	0.56%	0.063%
64	16.763	2321	2325	2330	rBV4	16923	34263	0.57%	0.064%
65	16.875	2341	2344	2350	rVB4	20406	32758	0.54%	0.061%
66	16.986	2360	2363	2368	rVB4	19693	30988	0.51%	0.058%
67	17.222	2397	2403	2407	rBV	3229881	4400677	72.95%	8.194%
68	17.263	2407	2410	2414	rVV	280864	380299	6.30%	0.708%
69	17.322	2414	2420	2431	rVB	1981343	2955933	49.00%	5.504%
70	17.628	2469	2472	2479	rVB	30615	42420	0.70%	0.079%
71	17.728	2486	2489	2495	rVB4	30368	40725	0.68%	0.076%
72	17.898	2515	2518	2522	rVB5	16422	23085	0.38%	0.043%
73	17.986	2531	2533	2540	rVB4	13770	21576	0.36%	0.040%
74	18.110	2547	2554	2557	rBV3	161573	259564	4.30%	0.483%
75	18.275	2578	2582	2586	rBV2	40223	71337	1.18%	0.133%
76	18.310	2586	2588	2592	rVB	37117	41115	0.68%	0.077%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018706.D
 Acq On : 08 Dec 2023 10:58
 Operator : MA/JU
 Sample : 05497-04
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	18.398	2600	2603	2606	rBV2	28157	31111	0.52%	0.058%
78	18.528	2623	2625	2629	rVB5	23564	24674	0.41%	0.046%
79	18.575	2629	2633	2637	rBV2	41378	63816	1.06%	0.119%
80	18.669	2645	2649	2656	rVB3	55712	74050	1.23%	0.138%
81	18.886	2682	2686	2690	rVB	54821	63680	1.06%	0.119%
82	18.980	2699	2702	2704	rBV3	24904	32816	0.54%	0.061%
83	19.233	2740	2745	2750	rVB	371472	493248	8.18%	0.918%
84	19.345	2761	2764	2769	rVB4	72228	73833	1.22%	0.137%
85	19.557	2794	2800	2812	rBV	3107997	4520071	74.93%	8.416%
86	21.027	3047	3050	3057	rBV4	115357	194324	3.22%	0.362%
87	21.310	3092	3098	3102	rBV	4571067	5813915	96.38%	10.825%
88	21.345	3102	3104	3110	rVB	198314	224009	3.71%	0.417%
89	23.527	3468	3475	3480	rBV2	2078454	3896737	64.60%	7.255%
90	23.680	3494	3501	3513	rVB	3049150	6032243	100.00%	11.232%




Sum of corrected areas: 53707918

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018706.D
Acq On : 08 Dec 2023 10:58
Operator : MA/JU
Sample : 05497-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

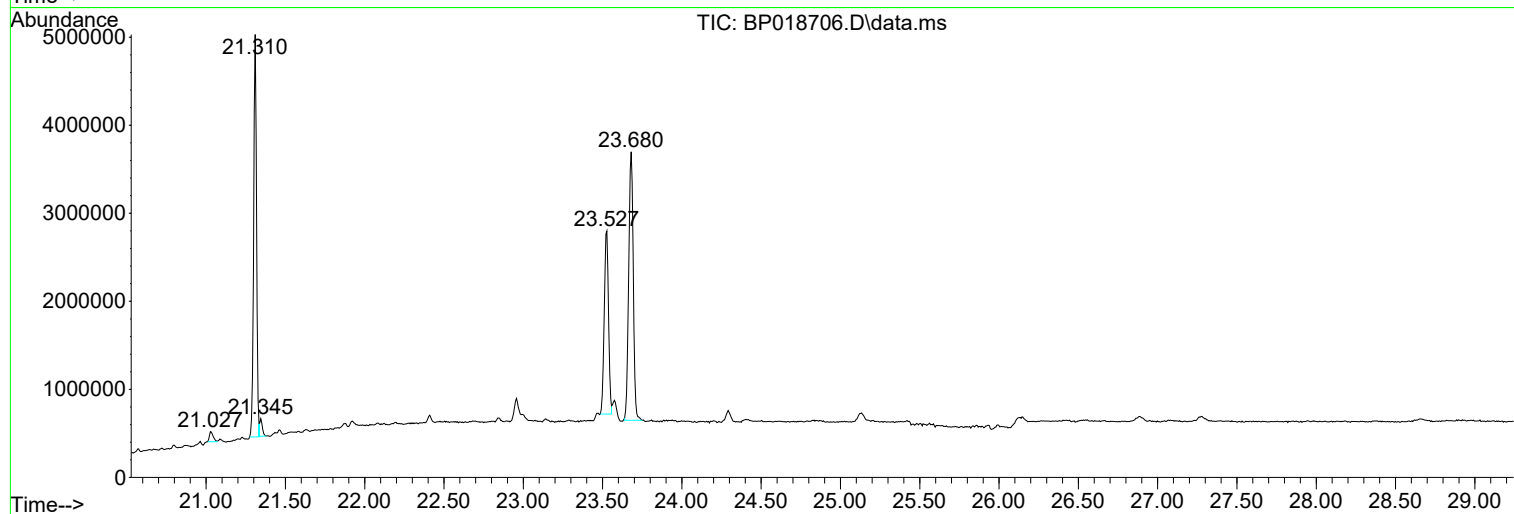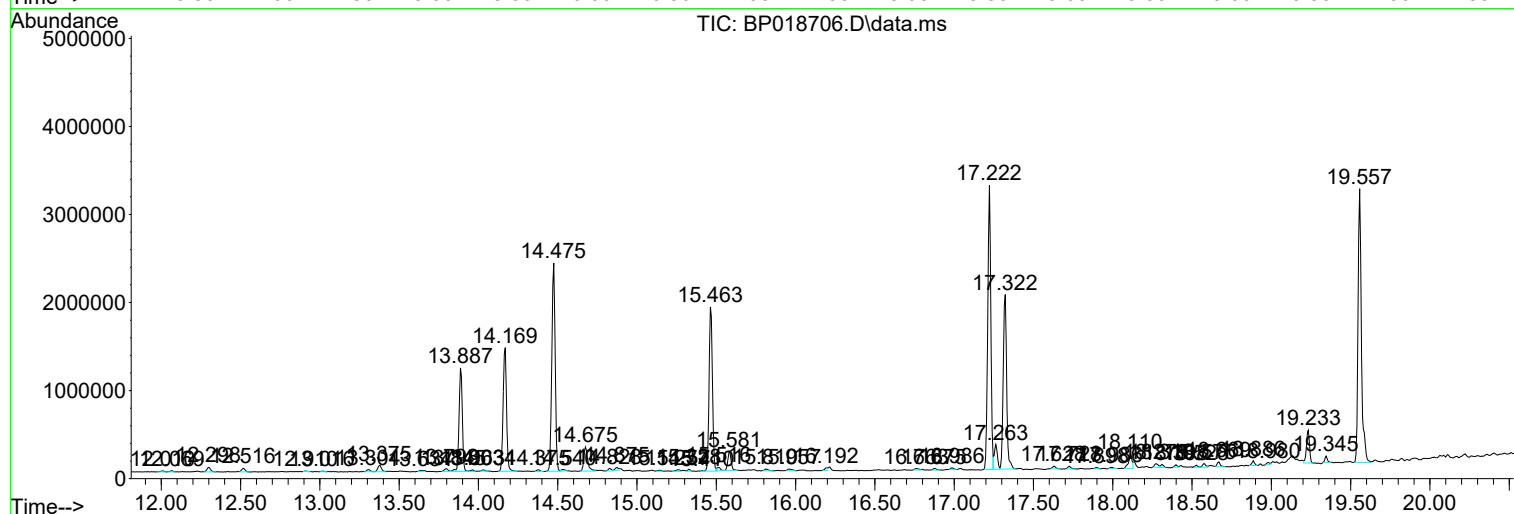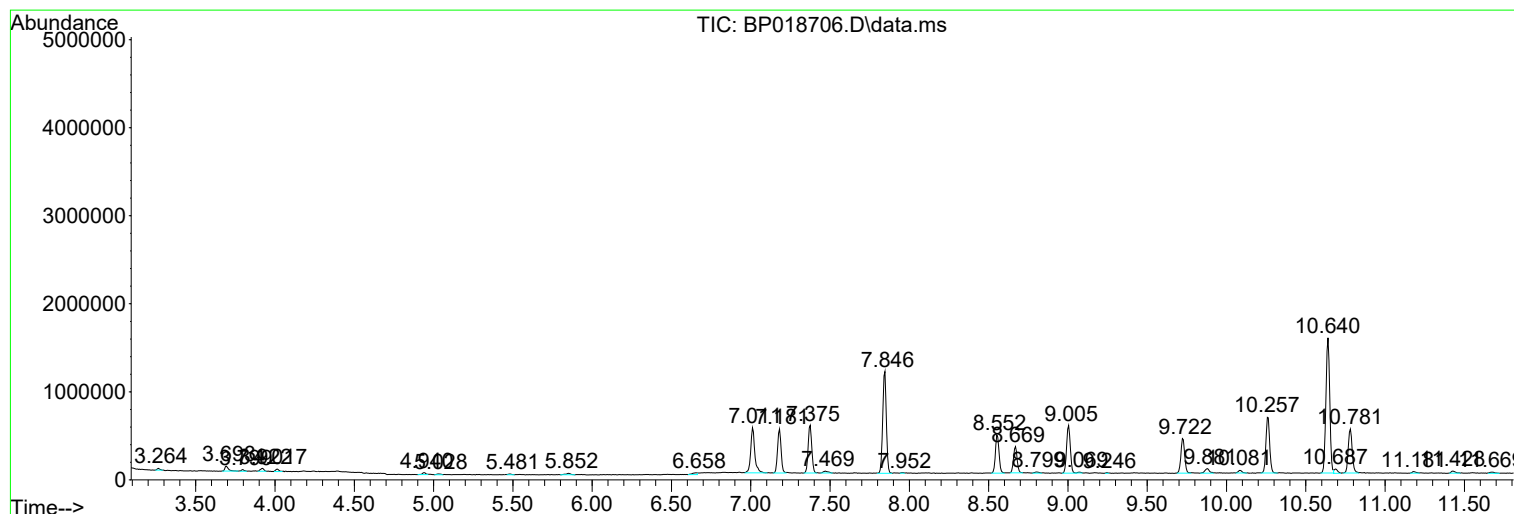

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018706.D
Acq On : 08 Dec 2023 10:58
Operator : MA/JU
Sample : 05497-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018706.D
Acq On : 08 Dec 2023 10:58
Operator : MA/JU
Sample : 05497-04
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc