

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018708.D
 Acq On : 08 Dec 2023 12:40
 Operator : MA/JU
 Sample : PB157521BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK521

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018708.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	35	rVB	57936	70712	0.95%	0.141%
2	3.681	97	101	114	rBV	710816	1036782	13.90%	2.066%
3	4.017	153	158	163	rVB4	12108	19920	0.27%	0.040%
4	4.346	210	214	220	rBV3	11940	18029	0.24%	0.036%
5	7.010	659	667	681	rVB	772347	1211220	16.24%	2.413%
6	7.181	690	696	704	rVB	612438	918210	12.31%	1.829%
7	7.375	722	729	737	rVB	774425	1202782	16.13%	2.396%
8	7.846	801	809	816	rBV	498058	799018	10.71%	1.592%
9	8.552	922	929	938	rBV	922136	1482572	19.88%	2.954%
10	9.005	998	1006	1014	rBV	678113	1103158	14.79%	2.198%
11	9.722	1119	1128	1140	rBV	531823	890236	11.94%	1.774%
12	10.257	1210	1219	1231	rBV	920998	1508385	20.23%	3.005%
13	10.640	1276	1284	1294	rVB	618372	1024881	13.74%	2.042%
14	10.781	1300	1308	1316	rBV	924753	1559251	20.91%	3.107%
15	12.222	1549	1553	1562	rVB2	17039	29274	0.39%	0.058%
16	13.375	1744	1749	1755	rVB6	8905	15323	0.21%	0.031%
17	13.445	1755	1761	1765	rBV5	5433	8284	0.11%	0.017%
18	13.887	1830	1836	1843	rBV	1624214	2281487	30.60%	4.546%
19	14.169	1876	1884	1892	rBV	1835206	2672764	35.84%	5.325%
20	14.475	1929	1936	1944	rBV	906695	1356621	18.19%	2.703%
21	14.675	1961	1970	1989	rBV	870501	1371763	18.40%	2.733%
22	15.463	2097	2104	2112	rBV	2481319	3542899	47.51%	7.059%
23	15.581	2118	2124	2138	rBV	730744	1025784	13.76%	2.044%
24	15.710	2141	2146	2150	rVB4	11128	19265	0.26%	0.038%
25	17.222	2397	2403	2411	rBV	1243695	1795573	24.08%	3.577%
26	17.322	2413	2420	2432	rBV	2979603	4386855	58.83%	8.740%
27	18.116	2550	2555	2559	rBV2	14479	20854	0.28%	0.042%
28	19.133	2724	2728	2732	rBV3	49501	61198	0.82%	0.122%
29	19.198	2736	2739	2743	rBV2	42581	60968	0.82%	0.121%
30	19.557	2794	2800	2807	rBV	4637501	5962762	79.96%	11.880%
31	21.310	3093	3098	3105	rBV	1878555	2474142	33.18%	4.929%
32	23.521	3467	3474	3483	rBV2	3796314	7457049	100.00%	14.857%
33	23.674	3494	3500	3508	rVB	1395795	2802921	37.59%	5.585%




Sum of corrected areas: 50190942

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018708.D
Acq On : 08 Dec 2023 12:40
Operator : MA/JU
Sample : PB157521BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK521

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

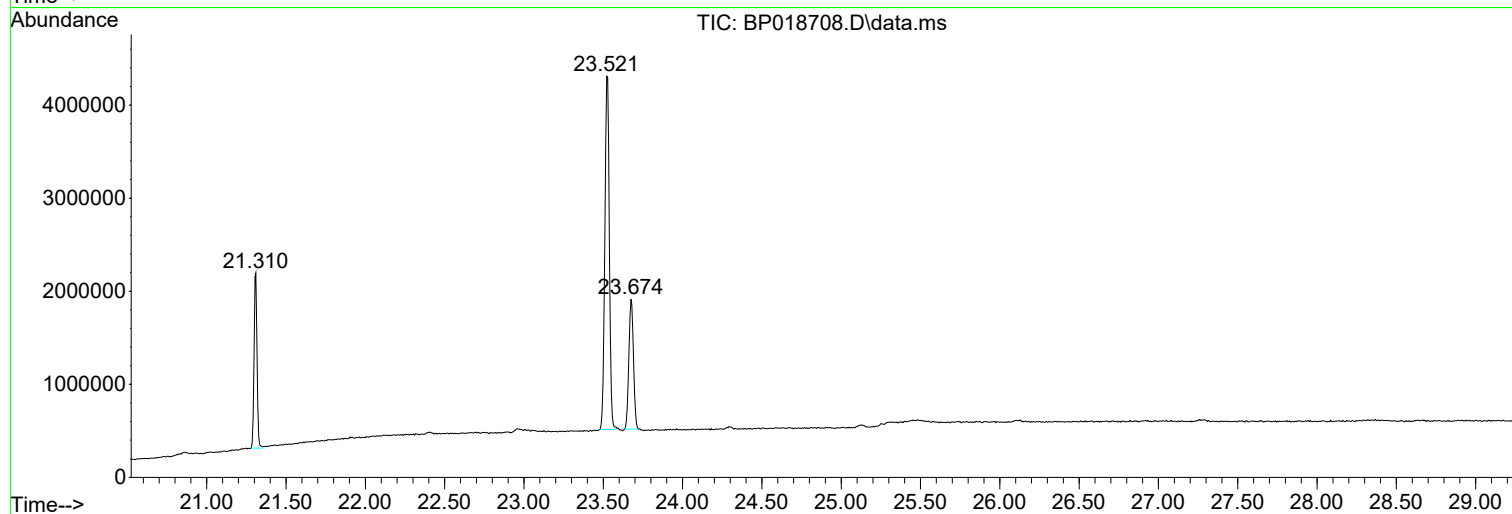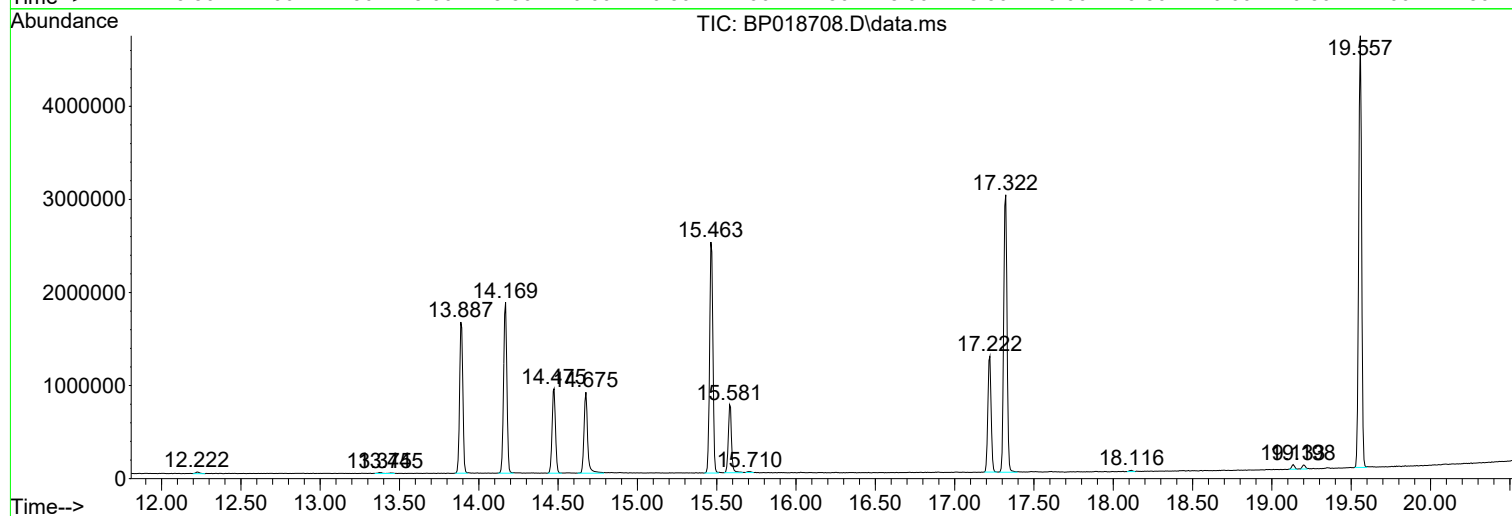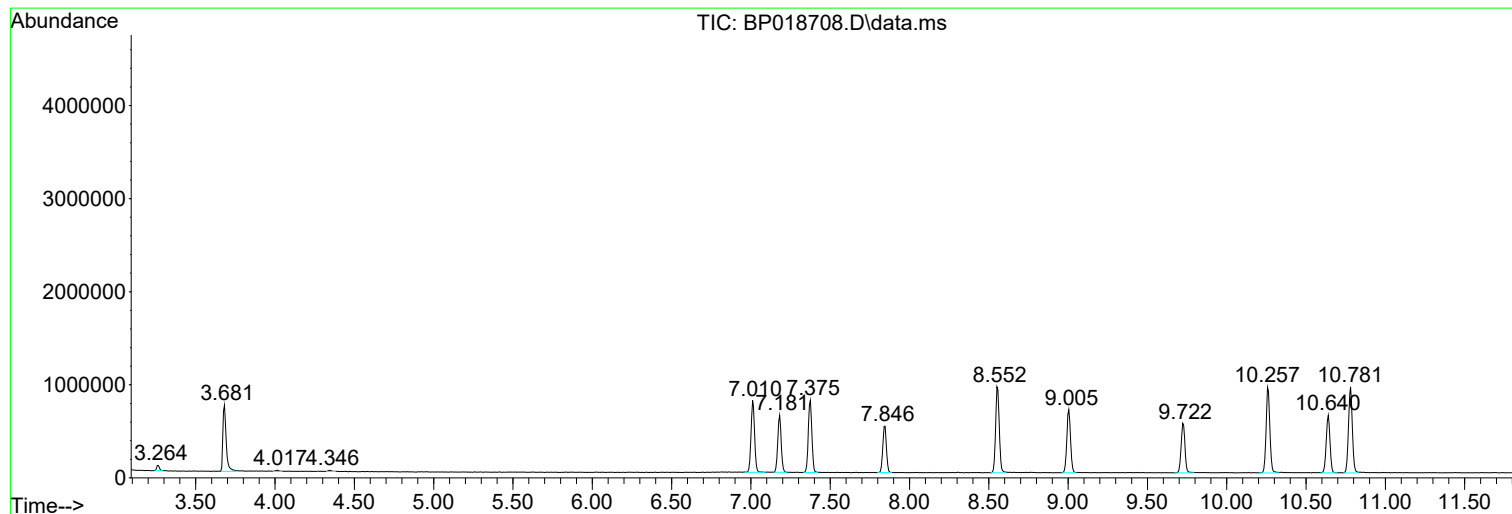

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018708.D
Acq On : 08 Dec 2023 12:40
Operator : MA/JU
Sample : PB157521BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK521

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018708.D
Acq On : 08 Dec 2023 12:40
Operator : MA/JU
Sample : PB157521BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK521

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc