

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018709.D
 Acq On : 08 Dec 2023 13:14
 Operator : MA/JU
 Sample : 05459-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018709.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	101	103	109	rBV	20902	32082	0.92%	0.117%
2	3.916	135	141	145	rBV	23930	39725	1.13%	0.145%
3	4.016	154	158	163	rVB3	21279	37989	1.09%	0.139%
4	4.093	170	171	172	rVB	11385	4019	0.11%	0.015%
5	4.111	172	174	178	rVB	17660	15615	0.45%	0.057%
6	4.393	219	222	225	rVB4	5296	5945	0.17%	0.022%
7	4.634	260	263	266	rBV4	2760	3769	0.11%	0.014%
8	4.699	269	274	276	rBV5	3542	4234	0.12%	0.015%
9	4.858	298	301	304	rVB2	4790	3745	0.11%	0.014%
10	4.940	308	315	320	rVV2	15944	25765	0.74%	0.094%
11	5.093	338	341	343	rVB	4031	3874	0.11%	0.014%
12	5.181	352	356	357	rBV4	3382	3868	0.11%	0.014%
13	5.269	367	371	375	rVB4	3051	5028	0.14%	0.018%
14	5.481	400	407	410	rBV8	4317	7517	0.21%	0.027%
15	5.822	462	465	466	rBV3	5250	4939	0.14%	0.018%
16	5.840	466	468	475	rVB4	4967	8982	0.26%	0.033%
17	6.099	503	512	513	rBV	16549	28564	0.82%	0.104%
18	6.828	634	636	638	rBV	4934	4338	0.12%	0.016%
19	7.010	659	667	683	rVB	287591	496173	14.17%	1.812%
20	7.181	690	696	703	rBV	231110	353311	10.09%	1.290%
21	7.375	722	729	737	rBV	268486	423127	12.09%	1.545%
22	7.469	741	745	748	rBV3	6028	9458	0.27%	0.035%
23	7.846	802	809	817	rVB	686374	1066674	30.47%	3.895%
24	7.952	824	827	828	rBV2	3768	3919	0.11%	0.014%
25	8.552	924	929	940	rBV	279096	454896	12.99%	1.661%
26	8.669	943	949	955	rVB	140382	223432	6.38%	0.816%
27	9.004	1000	1006	1013	rBV	250293	405811	11.59%	1.482%
28	9.169	1032	1034	1038	rBV3	3490	4911	0.14%	0.018%
29	9.240	1044	1046	1047	rBV2	4524	4148	0.12%	0.015%
30	9.540	1095	1097	1100	rVV	4473	5175	0.15%	0.019%
31	9.569	1100	1102	1106	rVB	3919	4730	0.14%	0.017%
32	9.669	1115	1119	1120	rBV2	3863	4607	0.13%	0.017%
33	9.722	1122	1128	1138	rVB2	169862	291256	8.32%	1.064%
34	9.869	1148	1153	1160	rBV2	18792	39827	1.14%	0.145%
35	10.087	1185	1190	1194	rVV3	12604	23399	0.67%	0.085%
36	10.263	1214	1220	1232	rBV	303462	510863	14.59%	1.866%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018709.D
 Acq On : 08 Dec 2023 13:14
 Operator : MA/JU
 Sample : 05459-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	10.440	1249	1250	1256	rVB	4531	6177	0.18%	0.023%
38	10.640	1277	1284	1291	rBV	860219	1420388	40.58%	5.187%
39	10.781	1301	1308	1317	rBV	270965	465327	13.29%	1.699%
40	10.904	1327	1329	1334	rVB2	5688	7700	0.22%	0.028%
41	11.181	1373	1376	1382	rVB7	7583	13683	0.39%	0.050%
42	11.434	1414	1419	1425	rBV2	11383	19760	0.56%	0.072%
43	11.675	1455	1460	1466	rBV8	8720	16714	0.48%	0.061%
44	12.004	1514	1516	1519	rBV4	4485	5703	0.16%	0.021%
45	12.063	1524	1526	1531	rBV3	6520	9954	0.28%	0.036%
46	12.222	1551	1553	1557	rVB2	10150	13323	0.38%	0.049%
47	12.298	1562	1566	1574	rVB2	15035	26537	0.76%	0.097%
48	12.522	1600	1604	1608	rVB	13086	18218	0.52%	0.067%
49	12.904	1667	1669	1672	rBV3	3879	4220	0.12%	0.015%
50	13.016	1686	1688	1695	rVB4	5969	8062	0.23%	0.029%
51	13.304	1734	1737	1743	rVB4	9334	11208	0.32%	0.041%
52	13.381	1746	1750	1755	rVB4	15307	23975	0.68%	0.088%
53	13.798	1819	1821	1826	rVB3	11274	12419	0.35%	0.045%
54	13.887	1831	1836	1844	rVV	541729	765178	21.86%	2.794%
55	13.963	1847	1849	1856	rVB3	8934	12000	0.34%	0.044%
56	14.169	1877	1884	1898	rBV	644042	969942	27.71%	3.542%
57	14.475	1929	1936	1945	rBV	1293706	1904402	54.40%	6.955%
58	14.675	1965	1970	1981	rBV	161220	302007	8.63%	1.103%
59	14.828	1993	1996	1999	rBV5	7974	11809	0.34%	0.043%
60	14.898	2005	2008	2014	rVB5	19225	28984	0.83%	0.106%
61	15.086	2038	2040	2042	rBV2	4847	4649	0.13%	0.017%
62	15.463	2098	2104	2111	rBV	909457	1311961	37.48%	4.791%
63	15.581	2119	2124	2133	rVB	123397	178970	5.11%	0.654%
64	16.210	2224	2231	2237	rBV5	17830	36831	1.05%	0.135%
65	16.875	2342	2344	2345	rBV2	6100	5437	0.16%	0.020%
66	17.222	2396	2403	2408	rBV	1819903	2518037	71.93%	9.196%
67	17.322	2414	2420	2431	rBV	1024452	1481201	42.31%	5.409%
68	17.722	2485	2488	2493	rBV2	13463	19417	0.55%	0.071%
69	17.857	2509	2511	2513	rBV2	6942	5475	0.16%	0.020%
70	18.110	2550	2554	2562	rVB4	62641	95196	2.72%	0.348%
71	18.886	2682	2686	2691	rVB2	24451	32548	0.93%	0.119%
72	19.227	2742	2744	2748	rVB	48963	58609	1.67%	0.214%
73	19.345	2761	2764	2769	rBV3	35013	41743	1.19%	0.152%
74	19.557	2794	2800	2812	rBV	1559809	2123558	60.66%	7.755%
75	21.310	3093	3098	3103	rBV	2602134	3264924	93.27%	11.923%
76	23.521	3468	3474	3481	rBV2	1095007	2060419	58.86%	7.524%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018709.D
Acq On : 08 Dec 2023 13:14
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

77 23.674 3494 3500 3510 rVB 1727511 3500608 100.00% 12.784%




Sum of corrected areas: 27382988

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018709.D
Acq On : 08 Dec 2023 13:14
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

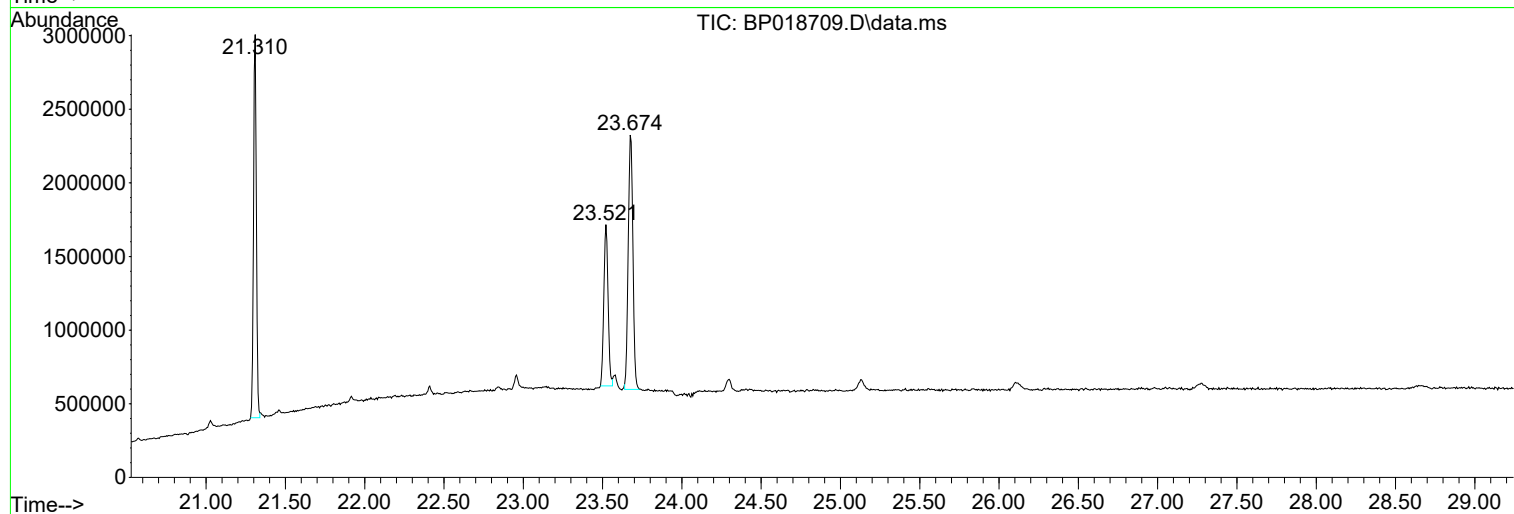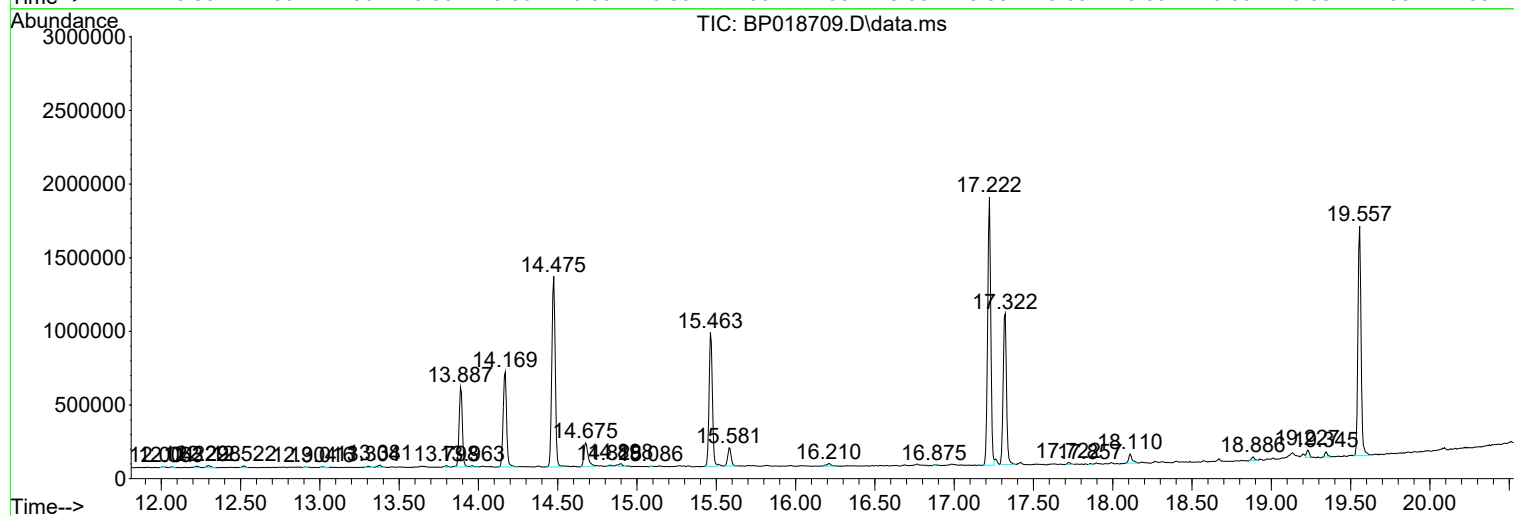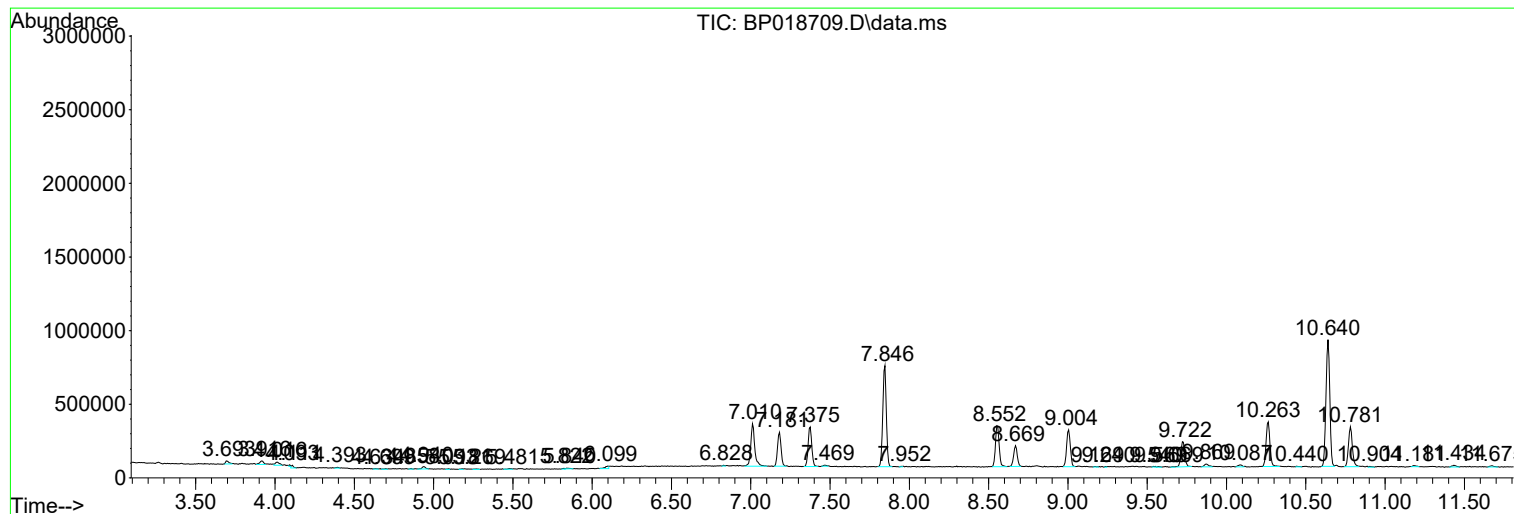

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018709.D
Acq On : 08 Dec 2023 13:14
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018709.D
Acq On : 08 Dec 2023 13:14
Operator : MA/JU
Sample : 05459-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------