

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018710.D
 Acq On : 08 Dec 2023 13:48
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	34	rVB2	12642	17389	0.63%	0.093%
2	3.693	99	103	112	rVB	42569	67608	2.43%	0.362%
3	3.917	137	141	146	rVB2	21836	34031	1.22%	0.182%
4	4.175	182	185	186	rBV2	6597	6948	0.25%	0.037%
5	4.387	219	221	226	rVB5	4787	5797	0.21%	0.031%
6	4.634	262	263	266	rBV2	3887	4013	0.14%	0.021%
7	4.934	311	314	320	rBV	11235	14202	0.51%	0.076%
8	5.416	393	396	398	rBV4	4224	4764	0.17%	0.025%
9	5.540	415	417	421	rBV5	2880	3814	0.14%	0.020%
10	5.781	456	458	460	rBV2	3136	3324	0.12%	0.018%
11	5.828	462	466	468	rBV3	2713	4099	0.15%	0.022%
12	5.940	483	485	488	rVB2	3179	3400	0.12%	0.018%
13	5.975	488	491	492	rBV2	4088	3273	0.12%	0.018%
14	6.834	633	637	638	rBV2	4229	5370	0.19%	0.029%
15	6.875	642	644	648	rVB3	2613	3253	0.12%	0.017%
16	6.916	648	651	653	rBV	3884	4286	0.15%	0.023%
17	7.010	657	667	677	rBV	160165	277247	9.97%	1.483%
18	7.181	689	696	707	rVB	145000	229937	8.27%	1.230%
19	7.375	722	729	739	rBV	170948	277525	9.98%	1.485%
20	7.469	739	745	748	rBV5	10211	18183	0.65%	0.097%
21	7.657	776	777	782	rVB3	3386	3725	0.13%	0.020%
22	7.722	785	788	790	rBV	3085	3263	0.12%	0.017%
23	7.769	792	796	798	rVB	2638	3367	0.12%	0.018%
24	7.846	798	809	817	rBV	403154	630391	22.67%	3.372%
25	8.346	892	894	900	rVB4	2562	4034	0.15%	0.022%
26	8.557	923	930	938	rBV	139966	235613	8.47%	1.260%
27	8.669	941	949	955	rVV	84208	135297	4.87%	0.724%
28	8.799	969	971	976	rVB2	3903	4498	0.16%	0.024%
29	9.004	999	1006	1012	rBV	162268	258598	9.30%	1.383%
30	9.422	1075	1077	1081	rVB3	5301	5221	0.19%	0.028%
31	9.546	1094	1098	1100	rBV4	3216	4497	0.16%	0.024%
32	9.722	1122	1128	1136	rBV	112294	188630	6.78%	1.009%
33	9.869	1148	1153	1161	rBV4	12695	28912	1.04%	0.155%
34	10.087	1186	1190	1195	rVB3	8342	13497	0.49%	0.072%
35	10.210	1208	1211	1213	rBV2	3824	3951	0.14%	0.021%
36	10.263	1213	1220	1228	rVV	184739	311635	11.21%	1.667%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018710.D
 Acq On : 08 Dec 2023 13:48
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	10.428	1246	1248	1251	rVB4	2739	3268	0.12%	0.017%
38	10.463	1251	1254	1255	rBV2	3276	3844	0.14%	0.021%
39	10.640	1276	1284	1291	rBV	483943	808425	29.08%	4.325%
40	10.687	1291	1292	1296	rVB2	4996	5388	0.19%	0.029%

41	10.728	1296	1299	1302	rBV3	2946	3309	0.12%	0.018%
42	10.781	1302	1308	1319	rBV	157349	277197	9.97%	1.483%
43	11.028	1347	1350	1352	rVB4	3111	3506	0.13%	0.019%
44	11.046	1352	1353	1355	rBV	3606	3633	0.13%	0.019%
45	11.169	1367	1374	1375	rBV3	5472	8931	0.32%	0.048%

46	11.440	1415	1420	1424	rVB6	5805	9099	0.33%	0.049%
47	11.675	1458	1460	1463	rVV	4610	5634	0.20%	0.030%
48	11.998	1512	1515	1518	rBV2	4111	5652	0.20%	0.030%
49	12.063	1524	1526	1533	rVB4	2678	3703	0.13%	0.020%
50	12.228	1550	1554	1560	rVB4	7401	12984	0.47%	0.069%

51	12.298	1562	1566	1571	rVB3	7079	11272	0.41%	0.060%
52	12.440	1586	1590	1592	rBV5	2551	4173	0.15%	0.022%
53	12.516	1600	1603	1608	rVB4	4495	8304	0.30%	0.044%
54	12.598	1613	1617	1621	rVB	3071	5026	0.18%	0.027%
55	12.910	1668	1670	1676	rVB5	4014	6802	0.24%	0.036%

56	13.040	1689	1692	1696	rVB2	2624	3584	0.13%	0.019%
57	13.081	1696	1699	1702	rBV2	2758	4213	0.15%	0.023%
58	13.169	1711	1714	1718	rVB2	3617	3981	0.14%	0.021%
59	13.381	1742	1750	1755	rBV3	18303	31566	1.14%	0.169%
60	13.557	1777	1780	1782	rBV2	3383	3295	0.12%	0.018%

61	13.757	1811	1814	1818	rBV2	2423	3938	0.14%	0.021%
62	13.798	1818	1821	1824	rVB2	3879	5539	0.20%	0.030%
63	13.887	1830	1836	1846	rBV	351846	478033	17.19%	2.557%
64	14.163	1875	1883	1893	rBV	383034	589874	21.22%	3.156%
65	14.322	1908	1910	1914	rVB5	2893	3503	0.13%	0.019%

66	14.475	1928	1936	1944	rBV	711144	1058999	38.09%	5.665%
67	14.675	1963	1970	1980	rBV2	81684	166557	5.99%	0.891%
68	14.839	1994	1998	2000	rBV3	4445	6467	0.23%	0.035%
69	14.892	2004	2007	2013	rVB7	9122	15540	0.56%	0.083%
70	15.222	2060	2063	2067	rBV2	3472	5676	0.20%	0.030%

71	15.334	2078	2082	2086	rVB6	3263	5595	0.20%	0.030%
72	15.463	2094	2104	2115	rBV	565649	821088	29.53%	4.392%
73	15.581	2120	2124	2131	rVV2	77139	108285	3.89%	0.579%
74	15.704	2143	2145	2148	rVB3	3924	3521	0.13%	0.019%
75	16.039	2200	2202	2205	rVB3	3634	3341	0.12%	0.018%

76	16.122	2215	2216	2219	rBV2	3326	3700	0.13%	0.020%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018710.D
 Acq On : 08 Dec 2023 13:48
 Operator : MA/JU
 Sample : 05459-18
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	16.181	2223	2226	2231	rBV3	3603	6548	0.24%	0.035%
78	16.286	2241	2244	2245	rBV3	2588	3260	0.12%	0.017%
79	16.481	2275	2277	2282	rBV5	2659	3428	0.12%	0.018%
80	16.628	2299	2302	2308	rBV2	3739	5520	0.20%	0.030%
81	16.686	2308	2312	2315	rBV4	5010	7245	0.26%	0.039%
82	16.986	2362	2363	2366	rBV3	4376	3723	0.13%	0.020%
83	17.222	2396	2403	2408	rBV	1002676	1446148	52.01%	7.736%
84	17.263	2408	2410	2414	rVV2	23628	27616	0.99%	0.148%
85	17.322	2414	2420	2431	rVB	627861	921695	33.15%	4.931%
86	17.575	2460	2463	2464	rBV4	3428	4075	0.15%	0.022%
87	17.722	2486	2488	2493	rBV4	6776	10588	0.38%	0.057%
88	17.898	2515	2518	2522	rBV5	9930	12060	0.43%	0.065%
89	17.992	2530	2534	2538	rBV6	8323	13310	0.48%	0.071%
90	18.039	2540	2542	2543	rBV2	3775	3701	0.13%	0.020%
91	18.110	2550	2554	2564	rBV3	71163	101186	3.64%	0.541%
92	18.180	2564	2566	2570	rVV	5445	4603	0.17%	0.025%
93	18.669	2646	2649	2652	rVB4	14216	15108	0.54%	0.081%
94	18.886	2683	2686	2689	rVB2	14080	16181	0.58%	0.087%
95	19.227	2742	2744	2750	rVB	43581	50874	1.83%	0.272%
96	19.345	2761	2764	2769	rBV5	31970	42301	1.52%	0.226%
97	19.557	2795	2800	2809	rBV	1108235	1498780	53.90%	8.018%
98	21.310	3093	3098	3103	rBV	2043797	2610204	93.88%	13.963%
99	23.521	3468	3474	3481	rBV2	948143	1764678	63.47%	9.440%
100	23.674	3494	3500	3511	rVB	1361295	2780420	100.00%	14.874%




Sum of corrected areas: 18693289

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018710.D
Acq On : 08 Dec 2023 13:48
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

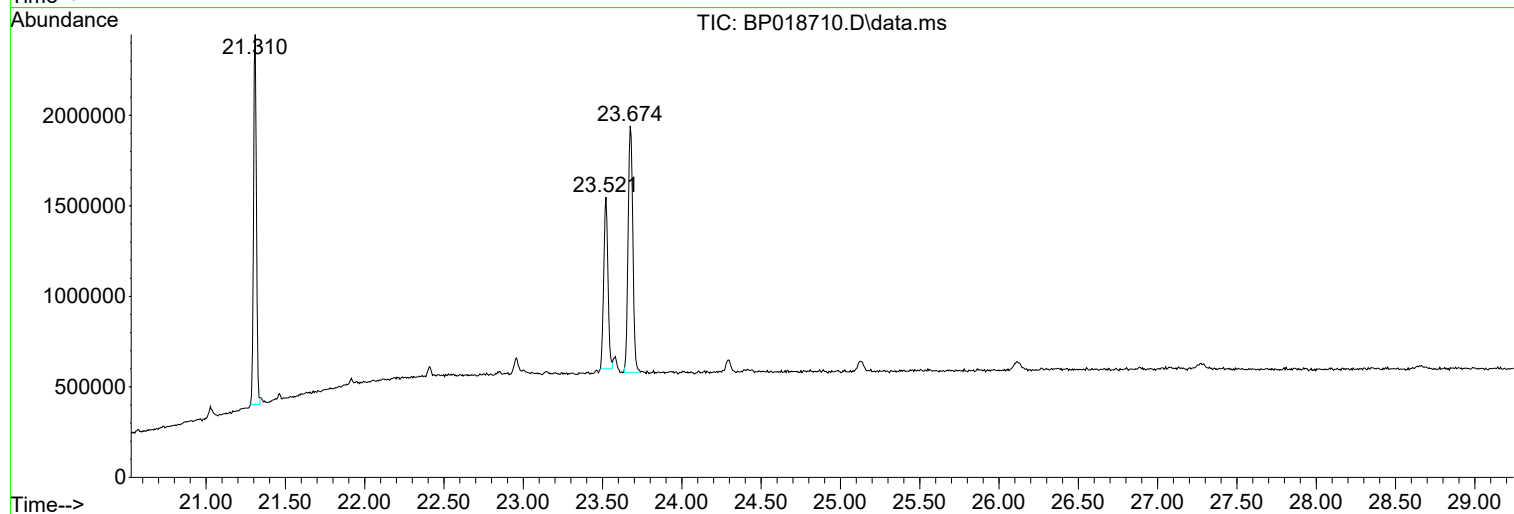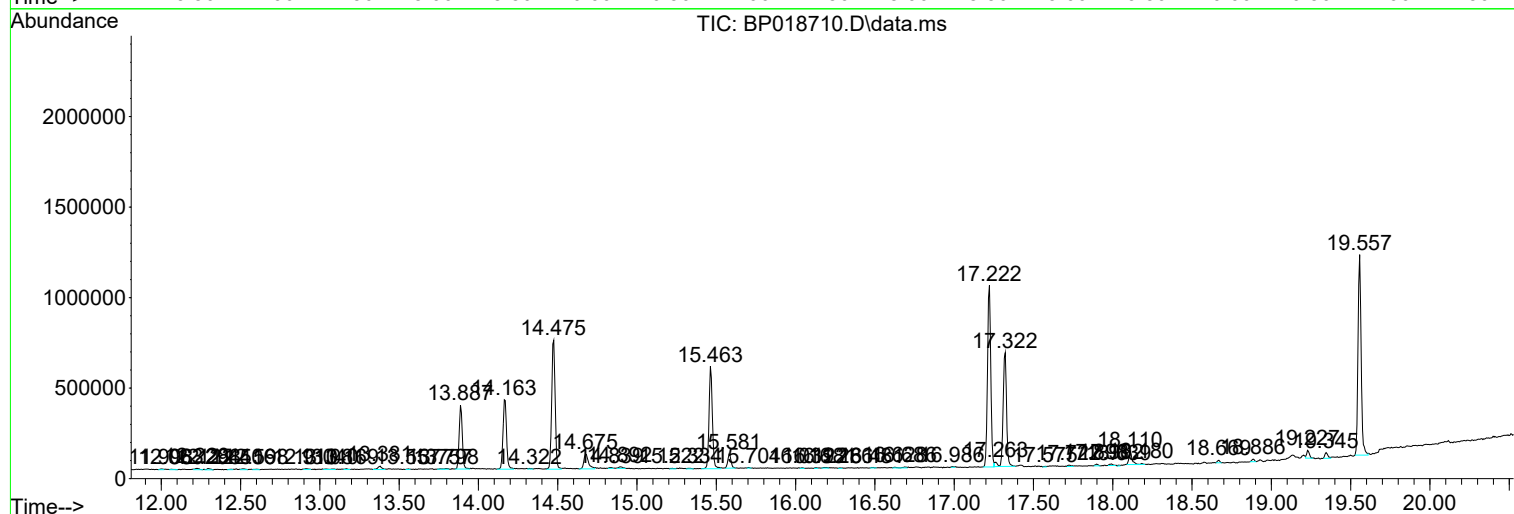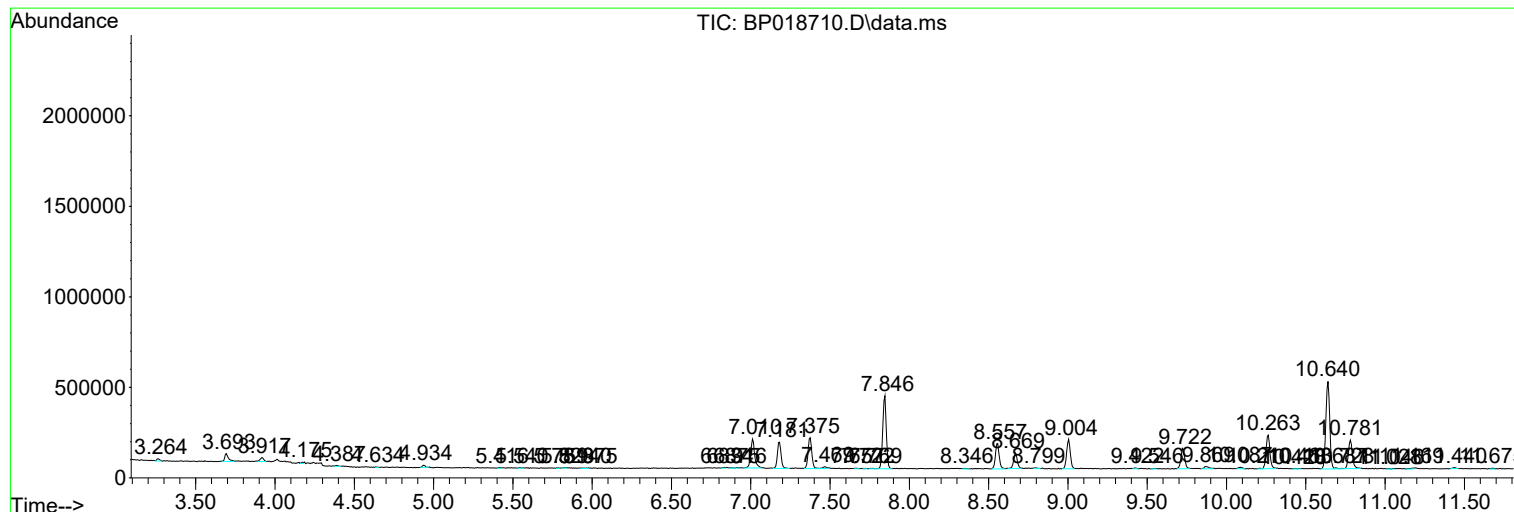

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018710.D
Acq On : 08 Dec 2023 13:48
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018710.D
Acq On : 08 Dec 2023 13:48
Operator : MA/JU
Sample : 05459-18
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------