

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018712.D
 Acq On : 08 Dec 2023 14:56
 Operator : MA/JU
 Sample : 05459-12
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018712.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	100	103	108	rBV	29397	39977	1.44%	0.179%
2	3.793	118	120	124	rVB3	15799	16483	0.59%	0.074%
3	3.917	138	141	147	rVB	25280	34175	1.23%	0.153%
4	4.011	154	157	161	rBV	17484	19160	0.69%	0.086%
5	4.811	292	293	296	rBV	4849	5100	0.18%	0.023%
6	4.940	311	315	321	rBV2	22438	35456	1.28%	0.158%
7	5.775	454	457	458	rBV3	8530	7413	0.27%	0.033%
8	6.187	525	527	528	rBV2	4516	3180	0.11%	0.014%
9	6.299	544	546	550	rBV	3648	3811	0.14%	0.017%
10	7.011	660	667	680	rVB	239817	436165	15.71%	1.948%
11	7.181	689	696	702	rBV	217392	334530	12.05%	1.494%
12	7.275	710	712	716	rBV3	3977	3472	0.13%	0.016%
13	7.375	722	729	736	rBV	253819	399314	14.39%	1.783%
14	7.469	741	745	749	rVB7	7846	11878	0.43%	0.053%
15	7.511	750	752	754	rVB3	3717	2807	0.10%	0.013%
16	7.581	761	764	768	rVB	5791	7878	0.28%	0.035%
17	7.616	768	770	773	rBV	6252	6491	0.23%	0.029%
18	7.652	773	776	780	rVB2	4891	5639	0.20%	0.025%
19	7.705	780	785	786	rBV2	6223	7660	0.28%	0.034%
20	7.734	786	790	791	rBV	6344	9346	0.34%	0.042%
21	7.846	802	809	816	rBV	586020	932948	33.61%	4.167%
22	8.140	858	859	863	rBV2	3665	3656	0.13%	0.016%
23	8.287	882	884	886	rBV3	3139	3035	0.11%	0.014%
24	8.428	906	908	911	rBV3	4715	4410	0.16%	0.020%
25	8.505	919	921	923	rBV	3986	3581	0.13%	0.016%
26	8.552	923	929	942	rVV	204810	346168	12.47%	1.546%
27	8.669	942	949	957	rBV	150005	244587	8.81%	1.092%
28	8.787	967	969	976	rVB6	6584	13210	0.48%	0.059%
29	9.005	999	1006	1013	rBV	218408	357143	12.87%	1.595%
30	9.175	1031	1035	1036	rBV4	3765	4540	0.16%	0.020%
31	9.299	1055	1056	1058	rBV2	3322	2965	0.11%	0.013%
32	9.493	1087	1089	1092	rVB2	3392	2934	0.11%	0.013%
33	9.722	1122	1128	1137	rBV	144289	241079	8.68%	1.077%
34	9.869	1149	1153	1161	rBV2	19300	34446	1.24%	0.154%
35	10.087	1186	1190	1195	rVB4	13076	20869	0.75%	0.093%
36	10.263	1213	1220	1229	rBV	263765	445155	16.04%	1.988%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018712.D
 Acq On : 08 Dec 2023 14:56
 Operator : MA/JU
 Sample : 05459-12
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	10.640	1276	1284	1296	rBV	712464	1217106	43.85%	5.436%
38	10.781	1302	1308	1316	rBV	199250	343921	12.39%	1.536%
39	10.981	1340	1342	1345	rBV	4738	4672	0.17%	0.021%
40	11.181	1374	1376	1383	rVB6	8632	11882	0.43%	0.053%
41	11.434	1416	1419	1427	rVB3	10465	21369	0.77%	0.095%
42	11.710	1464	1466	1470	rVB	12328	16878	0.61%	0.075%
43	11.763	1472	1475	1479	rVB	5286	8113	0.29%	0.036%
44	11.834	1479	1487	1489	rBV4	4273	7694	0.28%	0.034%
45	11.857	1489	1491	1493	rVV2	4836	5009	0.18%	0.022%
46	11.899	1496	1498	1502	rVB	6211	5864	0.21%	0.026%
47	11.975	1509	1511	1514	rBV	4070	3484	0.13%	0.016%
48	12.010	1514	1517	1520	rVB2	8445	10206	0.37%	0.046%
49	12.040	1520	1522	1523	rVB	8393	4576	0.16%	0.020%
50	12.057	1523	1525	1531	rVB	10470	15515	0.56%	0.069%
51	12.163	1533	1543	1547	rBV	12442	40145	1.45%	0.179%
52	12.228	1547	1554	1560	rBV2	22494	66395	2.39%	0.297%
53	13.375	1745	1749	1756	rBV3	17521	28640	1.03%	0.128%
54	13.798	1819	1821	1822	rBV2	3803	3148	0.11%	0.014%
55	13.887	1830	1836	1842	rBV	469635	653486	23.54%	2.919%
56	14.163	1878	1883	1891	rBV2	516824	777396	28.01%	3.472%
57	14.475	1929	1936	1944	rBV	1017705	1512529	54.49%	6.755%
58	14.675	1965	1970	1979	rBV	129690	228693	8.24%	1.021%
59	14.834	1993	1997	2002	rBV7	8875	16816	0.61%	0.075%
60	14.898	2005	2008	2012	rVB5	14730	17554	0.63%	0.078%
61	15.463	2098	2104	2112	rBV	789161	1144798	41.24%	5.113%
62	15.581	2120	2124	2130	rVB	96927	132529	4.77%	0.592%
63	16.769	2323	2326	2329	rVB4	9036	9660	0.35%	0.043%
64	17.222	2397	2403	2409	rBV	1423638	2000353	72.06%	8.934%
65	17.322	2414	2420	2430	rVV	868280	1275916	45.97%	5.699%
66	17.422	2433	2437	2441	rVB4	14032	21145	0.76%	0.094%
67	18.110	2550	2554	2564	rBV3	65828	90854	3.27%	0.406%
68	18.881	2682	2685	2690	rBV	29671	39459	1.42%	0.176%
69	19.233	2742	2745	2750	rVB2	45538	58584	2.11%	0.262%
70	19.345	2761	2764	2768	rBV3	40582	50548	1.82%	0.226%
71	19.557	2794	2800	2812	rBV	1462737	1962874	70.71%	8.767%
72	21.310	3093	3098	3103	rBV	2266746	2775821	100.00%	12.398%
73	23.521	3468	3474	3481	rBV2	796555	1495154	53.86%	6.678%
74	23.674	3494	3500	3509	rVB	1153506	2260647	81.44%	10.097%

Sum of corrected areas: 22390094




Instrument :
BNA_P
ClientSampleId :
C0AJ7

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018712.D
Acq On : 08 Dec 2023 14:56
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

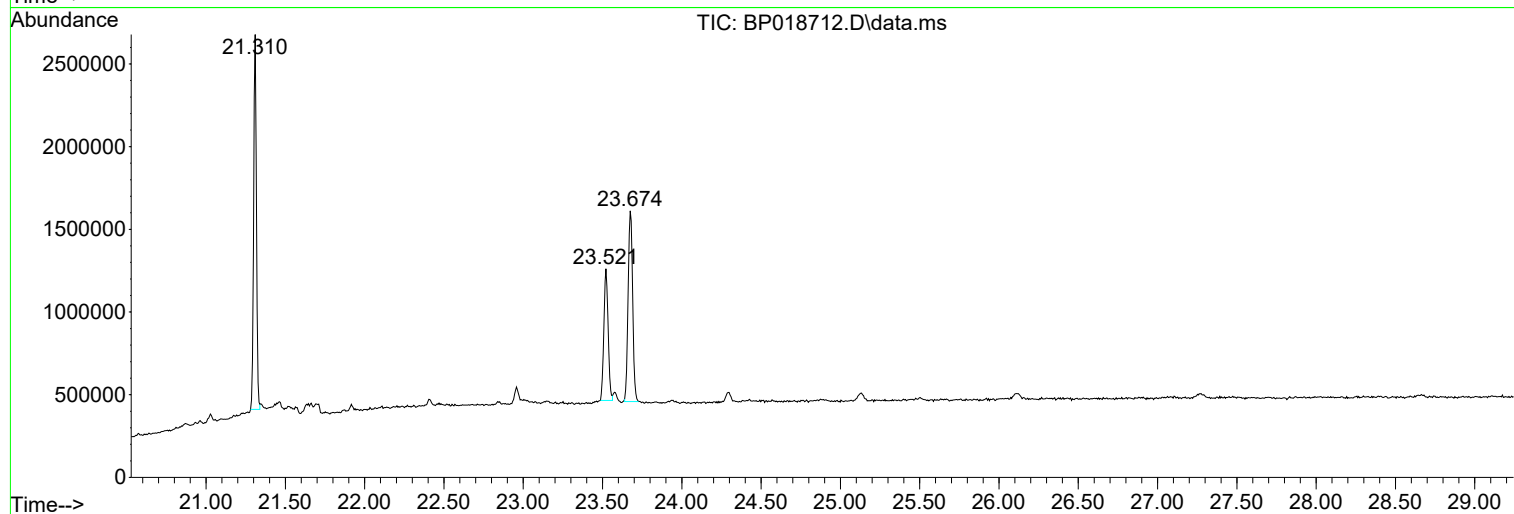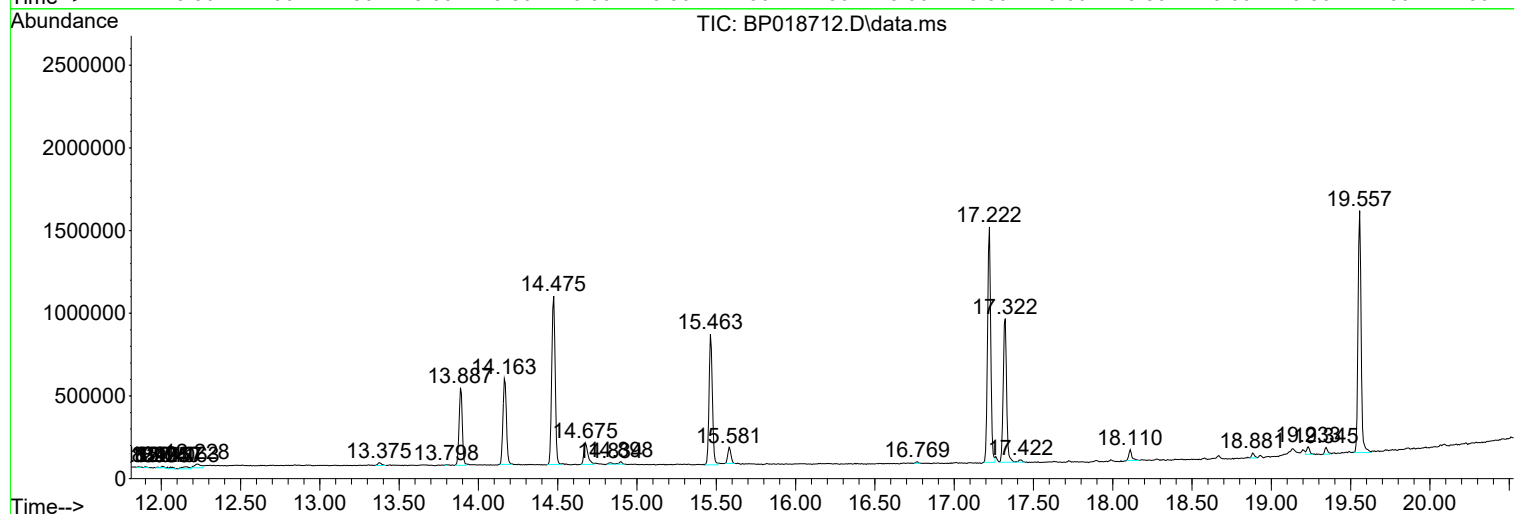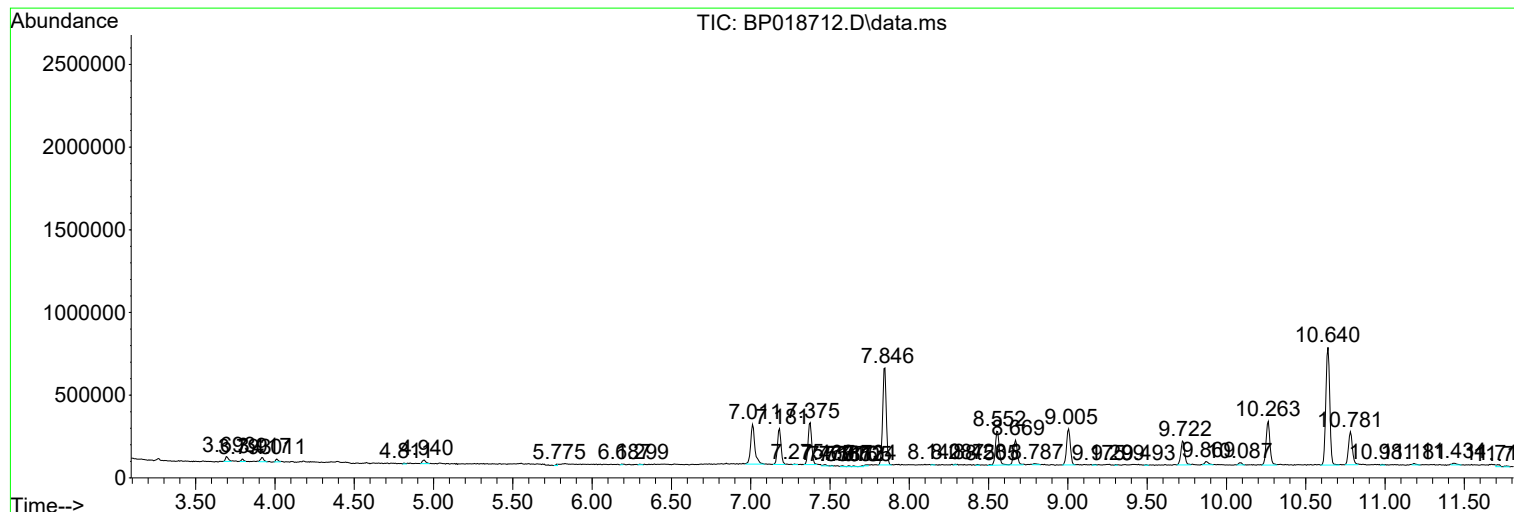

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018712.D
Acq On : 08 Dec 2023 14:56
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018712.D
Acq On : 08 Dec 2023 14:56
Operator : MA/JU
Sample : 05459-12
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------