

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018713.D
 Acq On : 08 Dec 2023 15:30
 Operator : MA/JU
 Sample : 05459-16
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	36	rVB2	9272	11196	0.45%	0.056%
2	3.605	86	88	89	rBV2	4475	3829	0.16%	0.019%
3	3.693	100	103	108	rBV2	32591	54110	2.19%	0.270%
4	3.799	118	121	125	rVB5	5977	7765	0.31%	0.039%
5	3.917	136	141	149	rVB3	17582	32942	1.33%	0.164%
6	4.011	154	157	160	rVB3	9379	10959	0.44%	0.055%
7	4.940	309	315	320	rBV3	14994	25656	1.04%	0.128%
8	5.475	403	406	411	rVB4	3980	5000	0.20%	0.025%
9	5.546	417	418	422	rVB4	4090	3720	0.15%	0.019%
10	5.828	462	466	468	rVV4	4328	6078	0.25%	0.030%
11	5.852	468	470	474	rVB4	2596	3532	0.14%	0.018%
12	6.252	534	538	542	rBV2	4794	3938	0.16%	0.020%
13	6.393	559	562	564	rBV3	4310	5192	0.21%	0.026%
14	6.793	628	630	634	rVB3	2506	3358	0.14%	0.017%
15	6.840	634	638	640	rBV5	4496	6736	0.27%	0.034%
16	7.011	659	667	684	rVB	186140	338493	13.71%	1.689%
17	7.181	687	696	702	rBV	171835	263859	10.69%	1.317%
18	7.375	722	729	737	rBV	190520	300185	12.16%	1.498%
19	7.463	741	744	748	rBV3	7988	14203	0.58%	0.071%
20	7.534	753	756	760	rBV5	2117	3383	0.14%	0.017%
21	7.846	801	809	816	rBV	444757	704102	28.53%	3.514%
22	8.216	865	872	874	rVV2	1849	3868	0.16%	0.019%
23	8.263	877	880	882	rVB	4013	3423	0.14%	0.017%
24	8.552	924	929	940	rVB	155078	253157	10.26%	1.263%
25	8.669	942	949	955	rBV	112601	182857	7.41%	0.912%
26	8.793	966	970	974	rBV5	5988	9074	0.37%	0.045%
27	9.005	999	1006	1015	rBV	190689	315856	12.80%	1.576%
28	9.181	1033	1036	1039	rVB2	3306	4040	0.16%	0.020%
29	9.422	1074	1077	1081	rVB4	3778	3893	0.16%	0.019%
30	9.587	1104	1105	1108	rBV2	3987	4033	0.16%	0.020%
31	9.628	1108	1112	1116	rVB5	3056	5010	0.20%	0.025%
32	9.663	1116	1118	1119	rBV2	3231	3224	0.13%	0.016%
33	9.722	1121	1128	1136	rVV	133551	222502	9.01%	1.110%
34	9.810	1139	1143	1146	rVB4	2427	4028	0.16%	0.020%
35	9.875	1149	1154	1159	rBV3	15542	23956	0.97%	0.120%
36	10.087	1185	1190	1194	rBV4	13442	20227	0.82%	0.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018713.D
 Acq On : 08 Dec 2023 15:30
 Operator : MA/JU
 Sample : 05459-16
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	10.140	1197	1199	1203	rVB3	2906	3699	0.15%	0.018%
38	10.193	1203	1208	1209	rBV2	4871	5258	0.21%	0.026%
39	10.263	1213	1220	1227	rBV	223351	371107	15.03%	1.852%
40	10.440	1247	1250	1252	rBV	2761	3736	0.15%	0.019%
41	10.469	1253	1255	1259	rVB	2925	3275	0.13%	0.016%
42	10.640	1276	1284	1290	rBV	574347	925552	37.50%	4.619%
43	10.781	1300	1308	1321	rBV	182145	325163	13.17%	1.623%
44	11.063	1355	1356	1360	rVB2	3270	3200	0.13%	0.016%
45	11.110	1360	1364	1366	rBV2	4983	5455	0.22%	0.027%
46	11.187	1372	1377	1381	rBV7	3714	6580	0.27%	0.033%
47	11.440	1413	1420	1424	rBV3	9299	22439	0.91%	0.112%
48	11.681	1458	1461	1465	rVB5	4026	5079	0.21%	0.025%
49	11.857	1488	1491	1493	rVB2	3057	3593	0.15%	0.018%
50	12.010	1515	1517	1520	rVV3	4478	5592	0.23%	0.028%
51	12.181	1543	1546	1548	rBV4	2924	3323	0.13%	0.017%
52	12.222	1548	1553	1560	rVB5	7616	15135	0.61%	0.076%
53	12.298	1560	1566	1571	rBV3	8958	16702	0.68%	0.083%
54	12.434	1584	1589	1590	rBV3	2779	3361	0.14%	0.017%
55	12.516	1599	1603	1607	rBV3	6462	11730	0.48%	0.059%
56	12.722	1634	1638	1640	rVB3	2682	3222	0.13%	0.016%
57	12.916	1670	1671	1677	rVB3	2852	4149	0.17%	0.021%
58	13.310	1736	1738	1740	rVV2	6072	5090	0.21%	0.025%
59	13.375	1744	1749	1753	rVV2	18303	29647	1.20%	0.148%
60	13.434	1757	1759	1763	rVV3	4399	5555	0.23%	0.028%
61	13.487	1766	1768	1770	rVV2	4632	3455	0.14%	0.017%
62	13.657	1794	1797	1800	rVB3	4116	5309	0.22%	0.026%
63	13.710	1803	1806	1810	rBV2	3073	5123	0.21%	0.026%
64	13.798	1816	1821	1826	rBV7	3979	7729	0.31%	0.039%
65	13.887	1829	1836	1843	rBV	421683	581220	23.55%	2.900%
66	14.163	1876	1883	1895	rBV	487427	746459	30.24%	3.725%
67	14.245	1895	1897	1902	rVB6	3191	4544	0.18%	0.023%
68	14.292	1902	1905	1909	rBV5	2275	4462	0.18%	0.022%
69	14.475	1928	1936	1944	rBV	810152	1248720	50.59%	6.231%
70	14.622	1958	1961	1964	rVB3	3627	4400	0.18%	0.022%
71	14.675	1964	1970	1981	rBV	97896	194972	7.90%	0.973%
72	14.828	1993	1996	2000	rBV6	8567	11396	0.46%	0.057%
73	15.098	2039	2042	2046	rBV5	3106	4327	0.18%	0.022%
74	15.145	2047	2050	2054	rVB4	2317	3719	0.15%	0.019%
75	15.281	2067	2073	2076	rBV3	4644	9190	0.37%	0.046%
76	15.463	2098	2104	2113	rBV	704611	1007661	40.82%	5.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018713.D
 Acq On : 08 Dec 2023 15:30
 Operator : MA/JU
 Sample : 05459-16
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	15.581	2119	2124	2132	rBV2	77304	125201	5.07%	0.625%
78	15.945	2184	2186	2188	rBV2	3932	4590	0.19%	0.023%
79	16.210	2229	2231	2234	rVB2	4340	4010	0.16%	0.020%
80	16.757	2322	2324	2326	rBV2	7171	8336	0.34%	0.042%
81	16.986	2361	2363	2364	rVV2	5449	3268	0.13%	0.016%
82	17.028	2368	2370	2372	rBV2	3874	3609	0.15%	0.018%
83	17.222	2397	2403	2408	rBV	1166381	1677143	67.95%	8.369%
84	17.263	2408	2410	2414	rVV	37113	43907	1.78%	0.219%
85	17.322	2414	2420	2430	rVB2	779767	1132353	45.87%	5.651%
86	17.628	2470	2472	2476	rVB4	4535	4723	0.19%	0.024%
87	17.722	2485	2488	2490	rBV4	6907	9829	0.40%	0.049%
88	17.992	2530	2534	2540	rVB5	9889	16296	0.66%	0.081%
89	18.110	2549	2554	2563	rBV4	68395	105014	4.25%	0.524%
90	18.181	2565	2566	2571	rVB2	8232	8118	0.33%	0.041%
91	18.575	2631	2633	2638	rVB6	8834	13683	0.55%	0.068%
92	18.669	2646	2649	2653	rBV3	15735	17915	0.73%	0.089%
93	18.886	2682	2686	2690	rBV3	23065	32815	1.33%	0.164%
94	18.928	2691	2693	2697	rVV4	9484	10652	0.43%	0.053%
95	19.233	2741	2745	2751	rVB	101654	126600	5.13%	0.632%
96	19.345	2761	2764	2767	rBV3	29270	36696	1.49%	0.183%
97	19.557	2795	2800	2814	rBV	1256535	1760467	71.32%	8.785%
98	21.310	3093	3098	3102	rBV	1809924	2329128	94.36%	11.623%
99	23.521	3469	3474	3481	rBV2	884723	1599020	64.78%	7.979%
100	23.680	3494	3501	3508	rVB	1248166	2468362	100.00%	12.318%




Sum of corrected areas: 20039447

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018713.D
Acq On : 08 Dec 2023 15:30
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

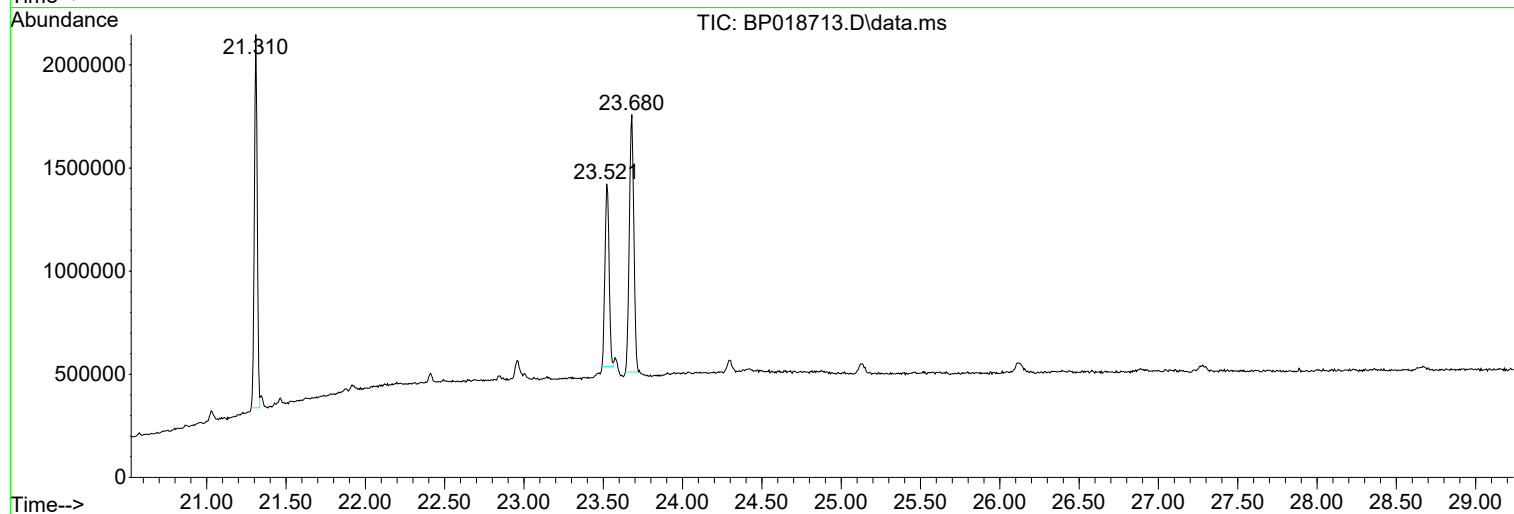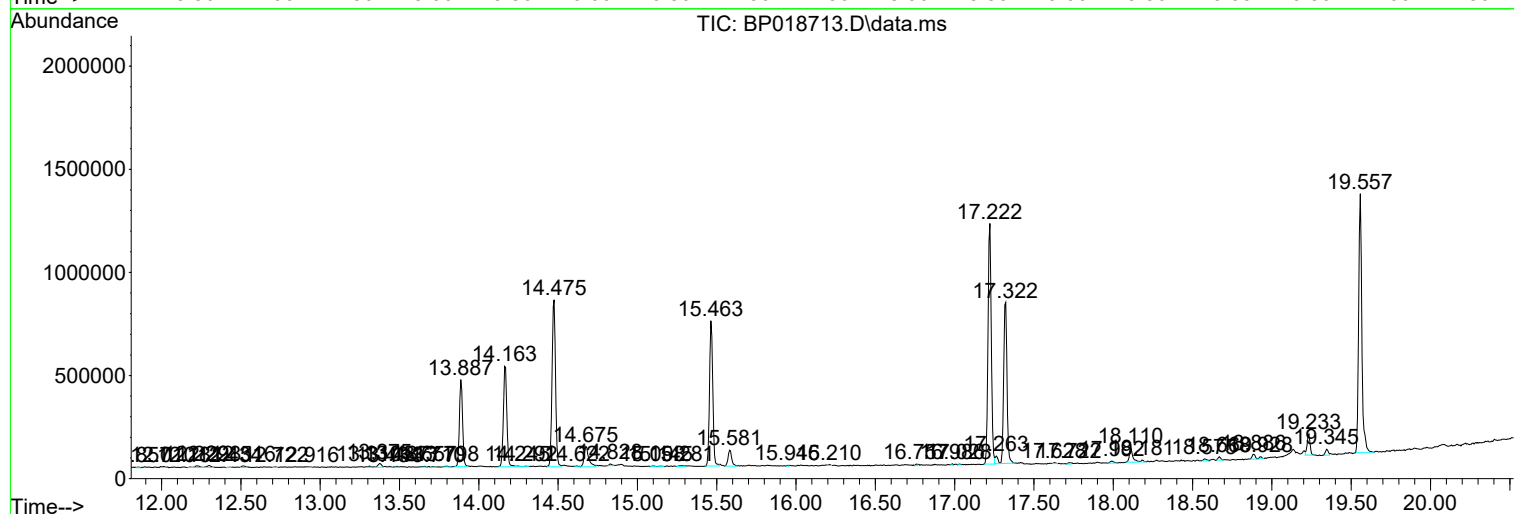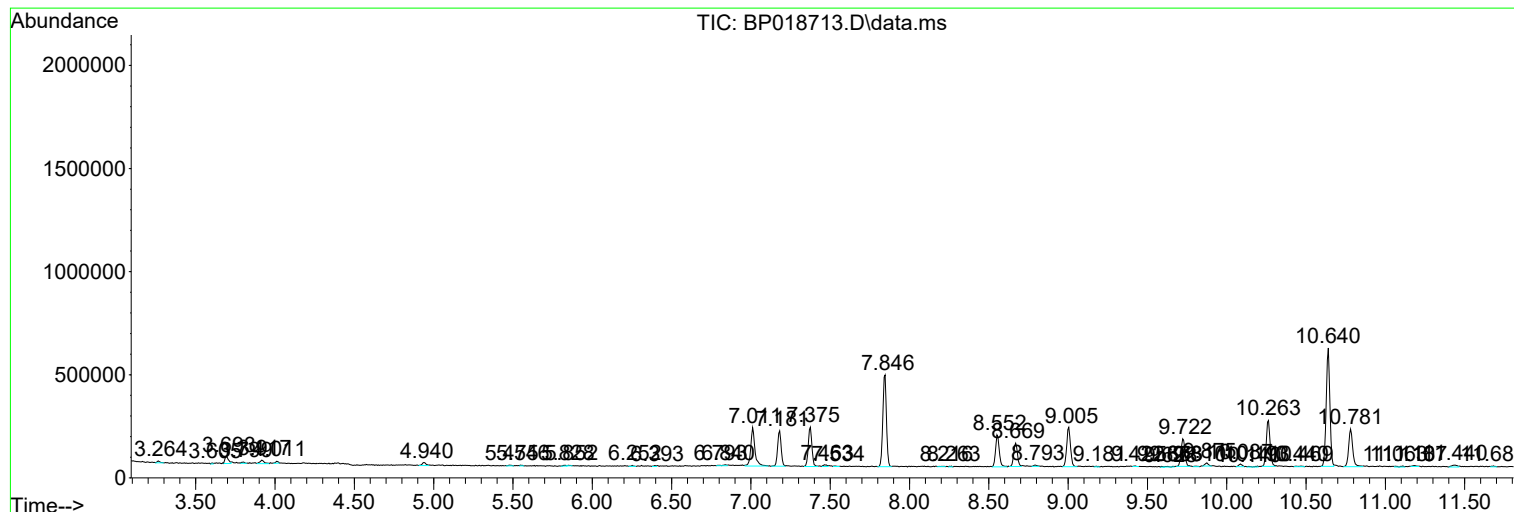

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018713.D
Acq On : 08 Dec 2023 15:30
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018713.D
Acq On : 08 Dec 2023 15:30
Operator : MA/JU
Sample : 05459-16
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------