

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018714.D
 Acq On : 08 Dec 2023 16:04
 Operator : MA/JU
 Sample : 05459-04
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018714.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	99	102	112	rBV	52153	80426	2.63%	0.400%
2	3.917	137	141	147	rVB2	20962	33057	1.08%	0.164%
3	4.017	153	158	162	rBV2	13790	21084	0.69%	0.105%
4	4.446	230	231	234	rVB2	6367	4354	0.14%	0.022%
5	4.852	297	300	303	rBV3	3956	4298	0.14%	0.021%
6	4.934	311	314	320	rVB	15064	20835	0.68%	0.104%
7	5.040	330	332	335	rVB4	3572	4198	0.14%	0.021%
8	5.187	355	357	359	rBV	4949	4422	0.14%	0.022%
9	5.481	403	407	411	rVB6	5143	7484	0.24%	0.037%
10	5.852	467	470	475	rVB6	7076	9734	0.32%	0.048%
11	6.652	604	606	609	rVB3	3831	4106	0.13%	0.020%
12	6.840	633	638	641	rVV6	3600	5759	0.19%	0.029%
13	7.010	659	667	682	rVB	164277	309445	10.11%	1.537%
14	7.181	689	696	703	rVB	129512	202009	6.60%	1.004%
15	7.369	722	728	738	rVB	151999	247619	8.09%	1.230%
16	7.469	740	745	747	rBV5	6966	10876	0.36%	0.054%
17	7.569	760	762	765	rVB3	4539	5029	0.16%	0.025%
18	7.657	773	777	779	rBV3	4022	4711	0.15%	0.023%
19	7.846	802	809	815	rVB	467663	733797	23.98%	3.645%
20	8.446	908	911	914	rVB2	2957	3796	0.12%	0.019%
21	8.552	924	929	936	rBV	152234	246617	8.06%	1.225%
22	8.669	944	949	956	rBV	117306	184238	6.02%	0.915%
23	8.793	966	970	975	rBV3	5739	8870	0.29%	0.044%
24	9.004	999	1006	1014	rBV	145338	241694	7.90%	1.201%
25	9.075	1014	1018	1020	rVB2	4556	4560	0.15%	0.023%
26	9.175	1032	1035	1040	rVB2	5474	8292	0.27%	0.041%
27	9.363	1065	1067	1069	rBV2	3584	4114	0.13%	0.020%
28	9.540	1094	1097	1099	rBV2	3997	4592	0.15%	0.023%
29	9.581	1102	1104	1109	rVB2	4102	5010	0.16%	0.025%
30	9.628	1109	1112	1115	rBV3	4489	5619	0.18%	0.028%
31	9.722	1122	1128	1137	rVV2	96929	174115	5.69%	0.865%
32	9.875	1147	1154	1160	rVV	18318	37289	1.22%	0.185%
33	10.081	1185	1189	1200	rVB4	12760	26320	0.86%	0.131%
34	10.263	1212	1220	1229	rBV	177321	300656	9.83%	1.494%
35	10.434	1246	1249	1251	rBV3	2900	4327	0.14%	0.021%
36	10.640	1273	1284	1291	rVV	571370	972179	31.77%	4.830%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018714.D
 Acq On : 08 Dec 2023 16:04
 Operator : MA/JU
 Sample : 05459-04
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	10.687	1291	1292	1298	rVV2	10305	13157	0.43%	0.065%
38	10.781	1301	1308	1316	rBV2	145038	261747	8.55%	1.300%
39	10.834	1316	1317	1324	rVV4	5552	9460	0.31%	0.047%
40	10.887	1324	1326	1330	rVB	4415	4591	0.15%	0.023%

41	11.181	1374	1376	1381	rVB5	6524	8216	0.27%	0.041%
42	11.428	1413	1418	1424	rBV2	7561	15578	0.51%	0.077%
43	11.675	1454	1460	1465	rBV8	6230	13294	0.43%	0.066%
44	12.004	1512	1516	1520	rBV5	5187	10707	0.35%	0.053%
45	12.069	1525	1527	1530	rVB4	3577	3913	0.13%	0.019%

46	12.134	1536	1538	1545	rVB	3701	4501	0.15%	0.022%
47	12.222	1545	1553	1558	rBV5	7368	14889	0.49%	0.074%
48	12.298	1562	1566	1572	rVB5	11182	19257	0.63%	0.096%
49	12.522	1598	1604	1609	rVB2	10542	18273	0.60%	0.091%
50	13.169	1711	1714	1717	rBV3	3307	4240	0.14%	0.021%

51	13.304	1734	1737	1742	rVB4	7505	10305	0.34%	0.051%
52	13.381	1742	1750	1755	rBV4	13009	24479	0.80%	0.122%
53	13.622	1788	1791	1793	rBV3	3579	3744	0.12%	0.019%
54	13.669	1797	1799	1803	rVB	3562	4465	0.15%	0.022%
55	13.792	1814	1820	1826	rBV8	7997	17456	0.57%	0.087%

56	13.845	1826	1829	1830	rVV3	6056	5966	0.19%	0.030%
57	13.887	1830	1836	1844	rVV	321169	451838	14.77%	2.245%
58	13.963	1844	1849	1853	rVV3	6361	13700	0.45%	0.068%
59	13.992	1853	1854	1857	rVV2	4160	4446	0.15%	0.022%
60	14.034	1857	1861	1862	rVV4	6396	6760	0.22%	0.034%

61	14.063	1865	1866	1871	rVB4	2954	3786	0.12%	0.019%
62	14.163	1877	1883	1896	rVB	361509	551206	18.01%	2.738%
63	14.381	1916	1920	1924	rBV4	6163	8968	0.29%	0.045%
64	14.475	1929	1936	1943	rBV	833547	1242854	40.62%	6.174%
65	14.675	1963	1970	1980	rBV	94317	181922	5.95%	0.904%

66	14.828	1993	1996	1997	rBV3	6303	6688	0.22%	0.033%
67	14.887	2000	2006	2007	rBV3	7172	13050	0.43%	0.065%
68	15.139	2045	2049	2054	rBV4	5268	9640	0.32%	0.048%
69	15.245	2062	2067	2068	rBV2	3825	6160	0.20%	0.031%
70	15.263	2068	2070	2072	rVV3	6613	7499	0.25%	0.037%

71	15.286	2072	2074	2076	rVV2	6663	6216	0.20%	0.031%
72	15.328	2079	2081	2084	rVV3	5508	5769	0.19%	0.029%
73	15.386	2086	2091	2094	rBV2	2617	5509	0.18%	0.027%
74	15.463	2098	2104	2111	rVV	534210	762144	24.91%	3.786%
75	15.510	2111	2112	2116	rVV3	12935	14401	0.47%	0.072%

76	15.581	2119	2124	2138	rVB3	74548	116424	3.80%	0.578%
----	--------	------	------	------	------	-------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018714.D
 Acq On : 08 Dec 2023 16:04
 Operator : MA/JU
 Sample : 05459-04
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	15.734	2147	2150	2153	rVB5	3788	4482	0.15%	0.022%
78	15.786	2155	2159	2161	rBV3	3283	5490	0.18%	0.027%
79	15.804	2161	2162	2166	rBV4	3768	5308	0.17%	0.026%
80	16.210	2224	2231	2236	rBV4	14996	32142	1.05%	0.160%
81	16.681	2309	2311	2314	rBV4	3139	4171	0.14%	0.021%
82	16.763	2321	2325	2329	rBV6	5738	9544	0.31%	0.047%
83	16.875	2341	2344	2346	rBV4	3508	4327	0.14%	0.021%
84	16.933	2352	2354	2355	rBV	3907	3759	0.12%	0.019%
85	16.986	2360	2363	2365	rVV4	3793	5320	0.17%	0.026%
86	17.222	2396	2403	2408	rBV	1161575	1733743	56.66%	8.613%
87	17.316	2414	2419	2431	rVB	589281	874708	28.59%	4.345%
88	17.622	2469	2471	2472	rBV2	4534	4071	0.13%	0.020%
89	17.722	2486	2488	2495	rVB7	8218	11506	0.38%	0.057%
90	17.892	2515	2517	2518	rBV2	6455	4649	0.15%	0.023%
91	17.986	2531	2533	2536	rBV3	8672	8701	0.28%	0.043%
92	18.110	2550	2554	2565	rVB3	79909	121361	3.97%	0.603%
93	18.669	2646	2649	2653	rVB3	17929	20699	0.68%	0.103%
94	18.886	2682	2686	2689	rBV	32829	45138	1.48%	0.224%
95	19.227	2741	2744	2749	rVB	73870	96456	3.15%	0.479%
96	19.345	2760	2764	2769	rBV2	61559	80073	2.62%	0.398%
97	19.557	2794	2800	2811	rBV	1151822	1685719	55.09%	8.374%
98	21.310	3092	3098	3103	rBV	2354623	2985497	97.57%	14.831%
99	23.521	3468	3474	3480	rBV2	767984	1490239	48.70%	7.403%
100	23.674	3494	3500	3513	rVB	1500197	3059777	100.00%	15.200%




Sum of corrected areas: 20129629

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018714.D
Acq On : 08 Dec 2023 16:04
Operator : MA/JU
Sample : 05459-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

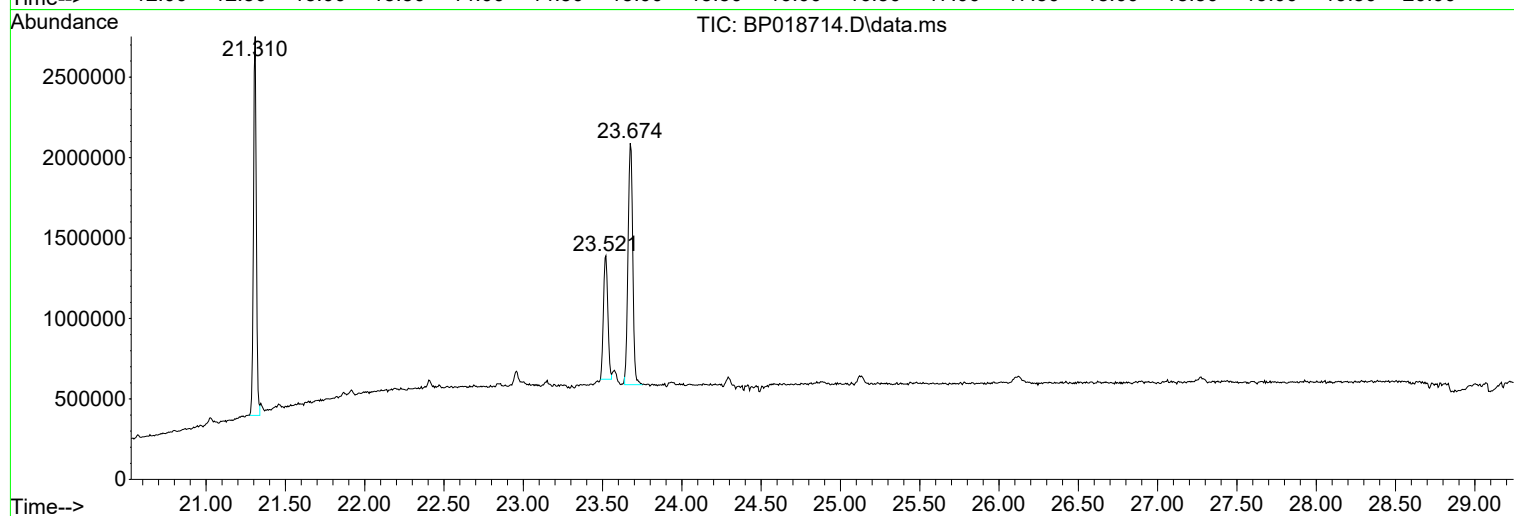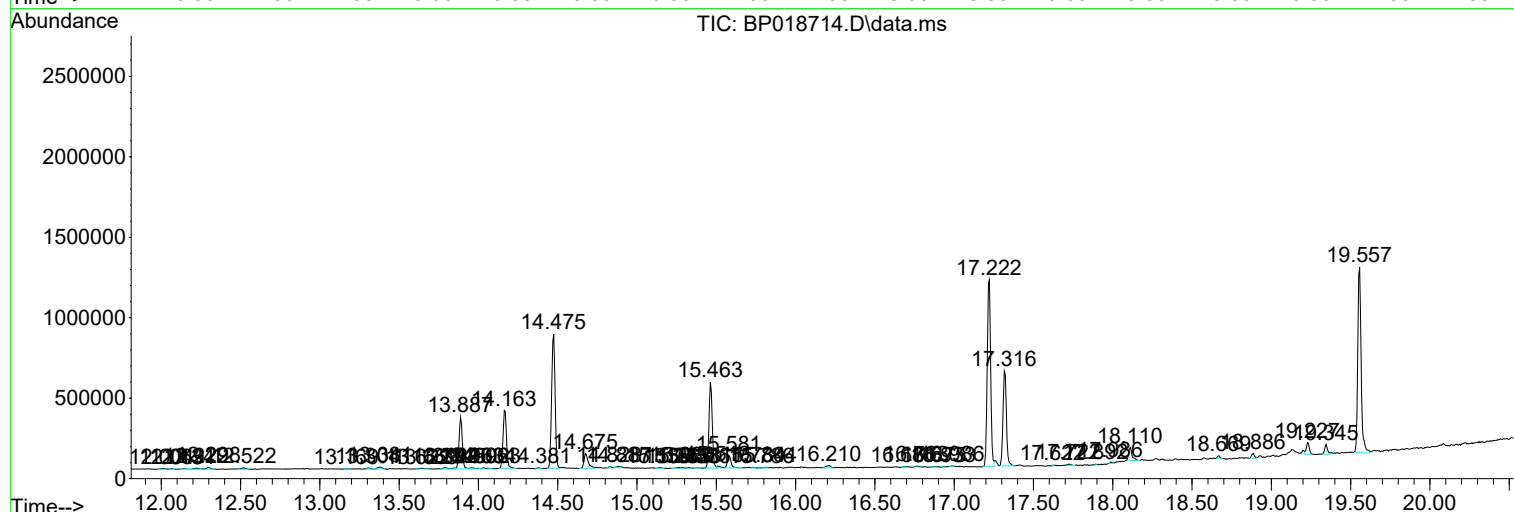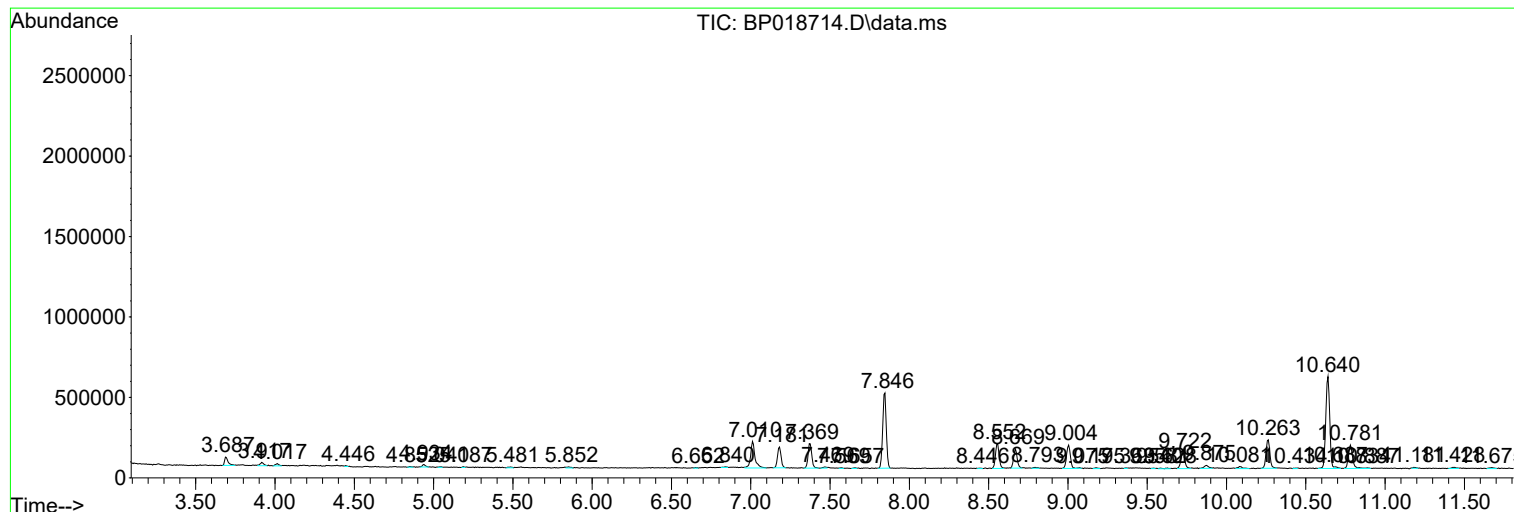

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018714.D
Acq On : 08 Dec 2023 16:04
Operator : MA/JU
Sample : 05459-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018714.D
Acq On : 08 Dec 2023 16:04
Operator : MA/JU
Sample : 05459-04
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------