

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018717.D
 Acq On : 08 Dec 2023 17:46
 Operator : MA/JU
 Sample : 05497-03
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	40	rVB	20949	34220	0.55%	0.079%
2	3.693	99	103	108	rBV	47477	67626	1.08%	0.157%
3	3.916	137	141	148	rVB3	34003	53069	0.85%	0.123%
4	4.011	154	157	161	rBV	23154	29663	0.47%	0.069%
5	4.940	311	315	319	rBV	33091	43444	0.69%	0.101%
6	5.481	404	407	412	rBV4	6404	9831	0.16%	0.023%
7	5.828	463	466	467	rBV2	7739	7245	0.12%	0.017%
8	7.010	659	667	681	rVB2	357873	665811	10.64%	1.546%
9	7.181	689	696	709	rVB	332160	523509	8.37%	1.215%
10	7.375	723	729	736	rBV	375343	583681	9.33%	1.355%
11	7.469	741	745	752	rVB5	16362	30019	0.48%	0.070%
12	7.846	802	809	818	rBV	1185307	1839910	29.40%	4.272%
13	8.128	855	857	860	rBV	7578	8762	0.14%	0.020%
14	8.322	886	890	893	rBV2	5871	11904	0.19%	0.028%
15	8.410	901	905	906	rBV	9293	13690	0.22%	0.032%
16	8.422	906	907	910	rVB	15726	7914	0.13%	0.018%
17	8.475	913	916	919	rBV3	4335	8462	0.14%	0.020%
18	8.557	922	930	939	rBV	209953	344283	5.50%	0.799%
19	8.669	943	949	957	rBV	247528	390235	6.24%	0.906%
20	8.793	964	970	976	rBV3	8915	16384	0.26%	0.038%
21	9.004	1000	1006	1013	rBV	276097	443504	7.09%	1.030%
22	9.116	1021	1025	1028	rVB3	6377	8275	0.13%	0.019%
23	9.175	1028	1035	1037	rBV4	4575	8609	0.14%	0.020%
24	9.428	1074	1078	1082	rBV5	4126	6941	0.11%	0.016%
25	9.728	1118	1129	1136	rBV	196926	335431	5.36%	0.779%
26	9.881	1149	1155	1160	rBV2	38798	77473	1.24%	0.180%
27	10.087	1185	1190	1195	rBV2	31952	61009	0.97%	0.142%
28	10.263	1213	1220	1229	rBV	402662	669289	10.70%	1.554%
29	10.640	1277	1284	1291	rBV	1494463	2408325	38.49%	5.591%
30	10.781	1302	1308	1318	rBV	296111	494978	7.91%	1.149%
31	11.181	1372	1376	1383	rBV4	18039	32527	0.52%	0.076%
32	11.428	1414	1418	1425	rBV	22056	39185	0.63%	0.091%
33	11.675	1457	1460	1468	rVB6	8257	17005	0.27%	0.039%
34	12.004	1514	1516	1520	rVB3	9017	13066	0.21%	0.030%
35	12.298	1562	1566	1572	rVB2	17460	32168	0.51%	0.075%
36	12.910	1668	1670	1676	rVB4	7149	9433	0.15%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
 Data File : BP018717.D
 Acq On : 08 Dec 2023 17:46
 Operator : MA/JU
 Sample : 05497-03
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	13.304	1735	1737	1743	rVB2	8683	10857	0.17%	0.025%
38	13.381	1743	1750	1755	rBV2	69750	114421	1.83%	0.266%
39	13.798	1818	1821	1826	rVB6	11873	15097	0.24%	0.035%
40	13.887	1831	1836	1843	rVV	736111	1005997	16.08%	2.336%
41	14.169	1877	1884	1896	rBV	839485	1281032	20.47%	2.974%
42	14.381	1917	1920	1924	rVB2	8057	10493	0.17%	0.024%
43	14.475	1929	1936	1943	rBV	2157125	3195106	51.06%	7.418%
44	14.675	1965	1970	1984	rBV2	195877	331767	5.30%	0.770%
45	14.828	1993	1996	2001	rBV3	16841	25947	0.41%	0.060%
46	14.892	2005	2007	2015	rVB6	28486	45594	0.73%	0.106%
47	15.263	2068	2070	2072	rBV2	6935	7405	0.12%	0.017%
48	15.463	2098	2104	2111	rBV	1216074	1745634	27.90%	4.053%
49	15.581	2120	2124	2131	rVB	145744	203014	3.24%	0.471%
50	16.769	2322	2326	2328	rBV5	10808	15137	0.24%	0.035%
51	16.875	2341	2344	2347	rBV3	8692	14738	0.24%	0.034%
52	16.980	2360	2362	2364	rBV2	8806	9579	0.15%	0.022%
53	17.222	2397	2403	2408	rBV	3080731	4271624	68.27%	9.917%
54	17.263	2408	2410	2414	rVV	130149	147176	2.35%	0.342%
55	17.322	2414	2420	2430	rVB	1331700	1931020	30.86%	4.483%
56	17.727	2485	2489	2495	rBV6	19818	32884	0.53%	0.076%
57	17.992	2530	2534	2541	rVB2	25331	40315	0.64%	0.094%
58	18.110	2548	2554	2563	rBV3	161484	271113	4.33%	0.629%
59	18.275	2579	2582	2586	rBV5	18700	23074	0.37%	0.054%
60	18.574	2630	2633	2638	rBV5	21547	33258	0.53%	0.077%
61	18.669	2645	2649	2653	rVB2	49706	57753	0.92%	0.134%
62	18.886	2682	2686	2690	rVB	56753	66943	1.07%	0.155%
63	19.233	2741	2745	2752	rVB	251033	323653	5.17%	0.751%
64	19.345	2761	2764	2769	rBV3	67657	89059	1.42%	0.207%
65	19.557	2794	2800	2814	rBV	2179575	3177292	50.78%	7.377%
66	21.310	3092	3098	3103	rBV	4648745	5996242	95.83%	13.921%
67	22.957	3375	3378	3384	rVB	206310	302378	4.83%	0.702%
68	23.527	3469	3475	3480	rBV2	1458196	2672199	42.70%	6.204%
69	23.680	3494	3501	3518	rVB	2982981	6257357	100.00%	14.528%




Sum of corrected areas: 43072038

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018717.D
Acq On : 08 Dec 2023 17:46
Operator : MA/JU
Sample : 05497-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

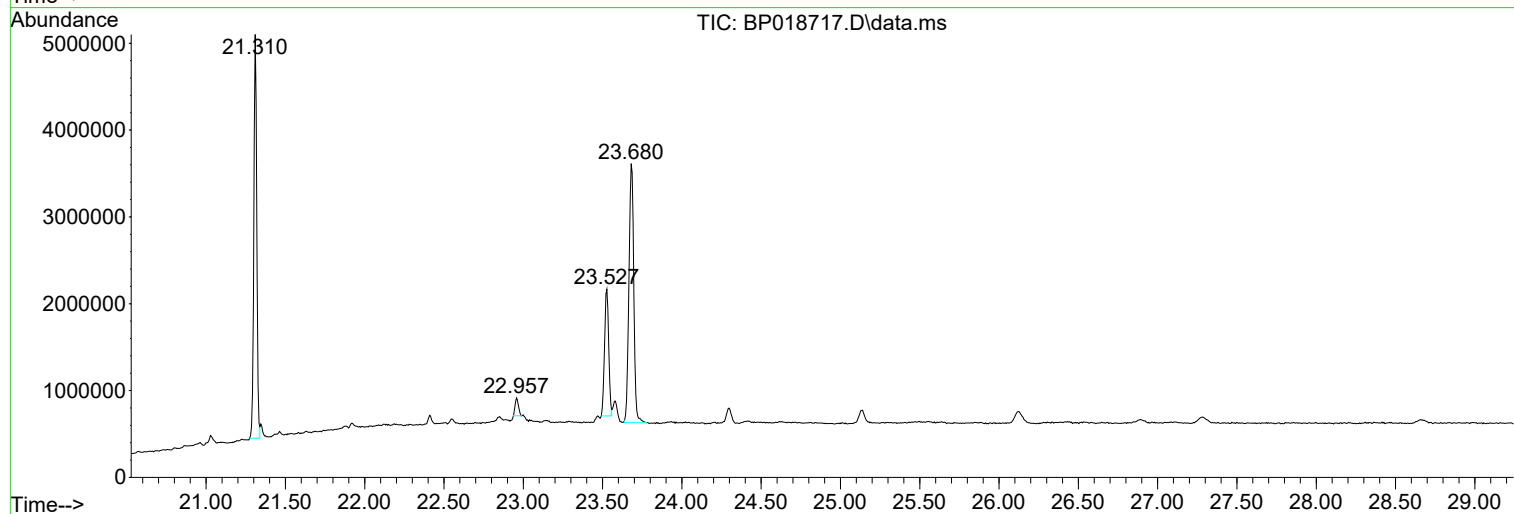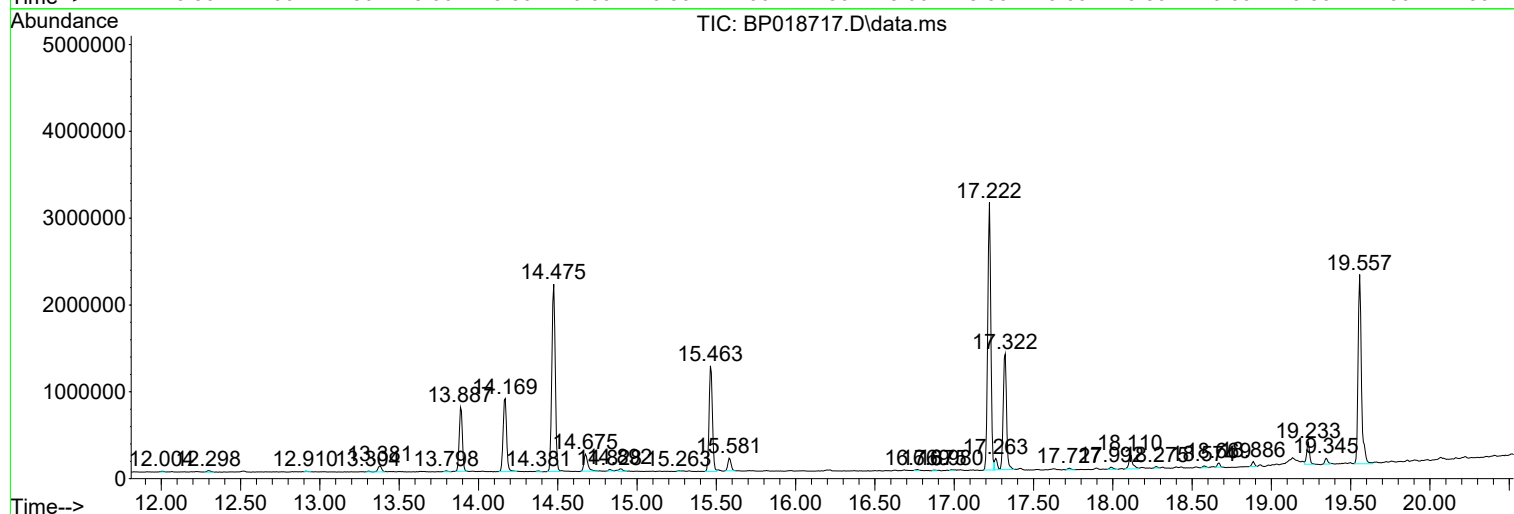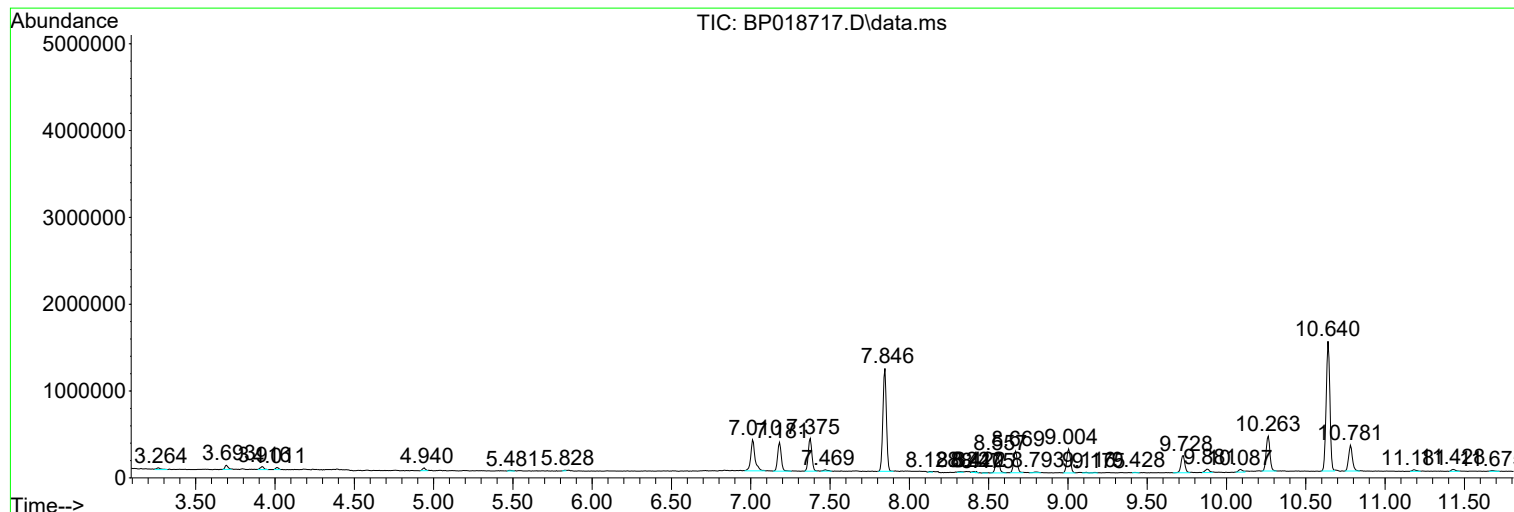

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018717.D
Acq On : 08 Dec 2023 17:46
Operator : MA/JU
Sample : 05497-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120723\
Data File : BP018717.D
Acq On : 08 Dec 2023 17:46
Operator : MA/JU
Sample : 05497-03
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc