
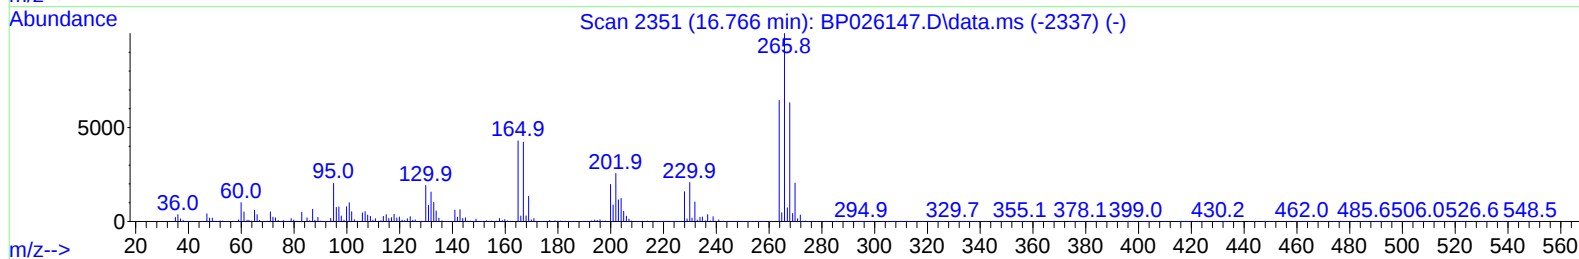
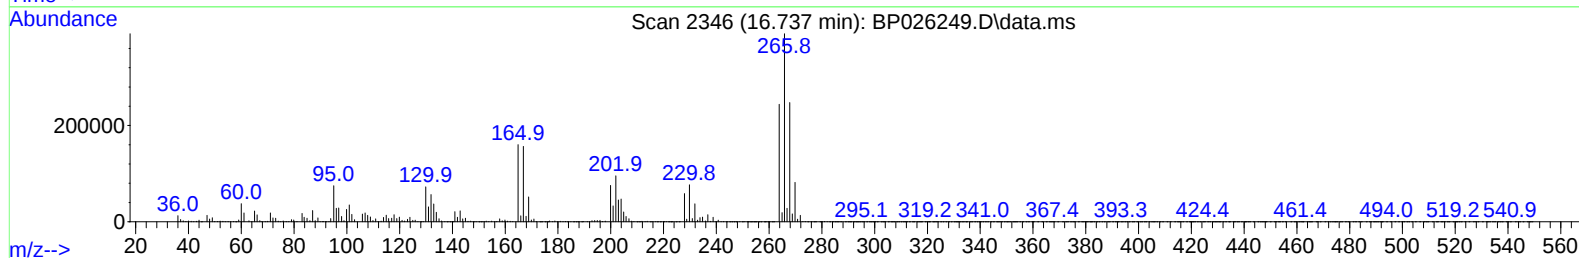


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120825\
Data File : BP026249.D
Acq On : 08 Dec 2025 13:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 13:36:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

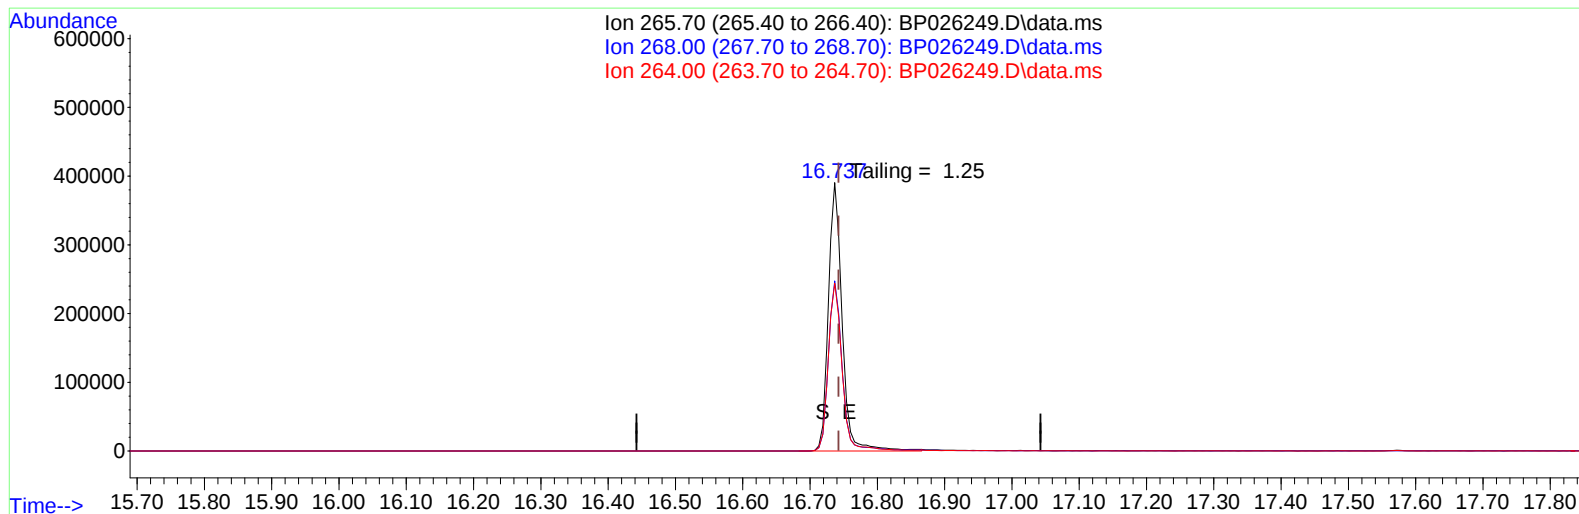

TIC: BP026249.D\data.ms

(70) Pentachlorophenol (C)




16.737min (-0.006) 52008.38 ng

response 550867

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.39
264.00	62.70	62.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120825\
Data File : BP026249.D
Acq On : 08 Dec 2025 13:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 08 13:36:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

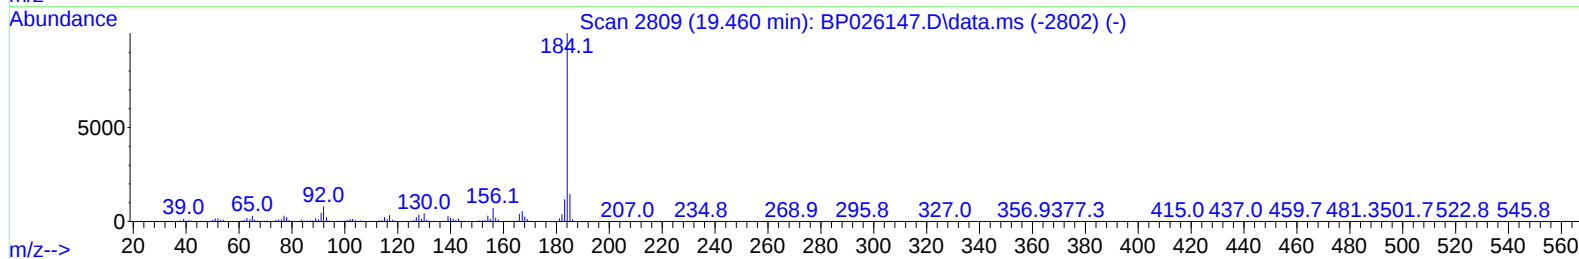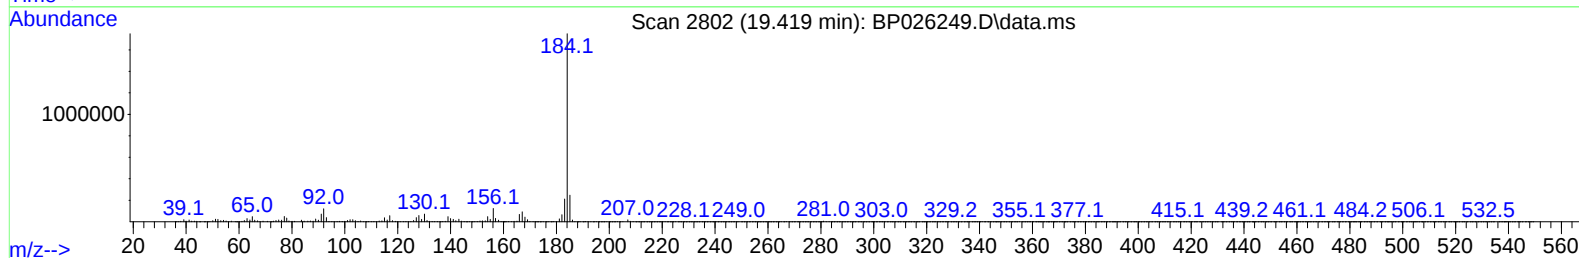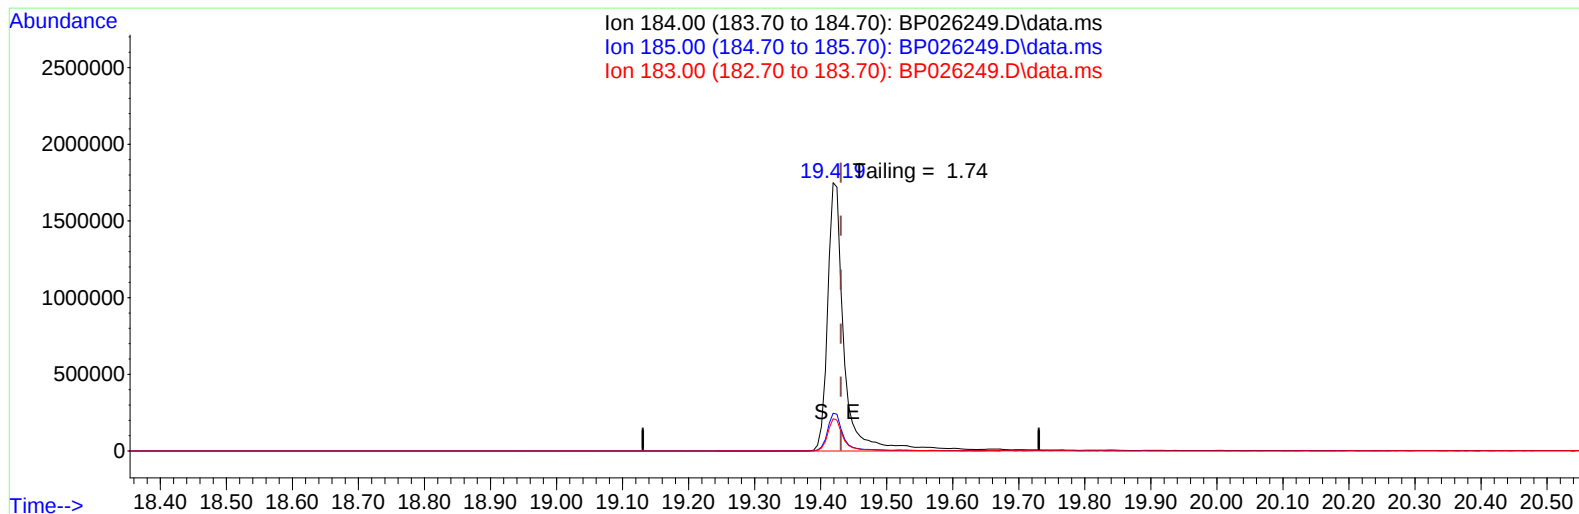

TIC: BP026249.D\data.ms

(77) Benzidine

19.419min (-0.012) 23636.55 ng

response 2964704

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.10
183.00	11.30	12.07
0.00	0.00	0.00