


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP120919\
 Data File : BP001270.D
 Acq On : 09 Dec 2019 15:19
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 05 12:34:47 2019

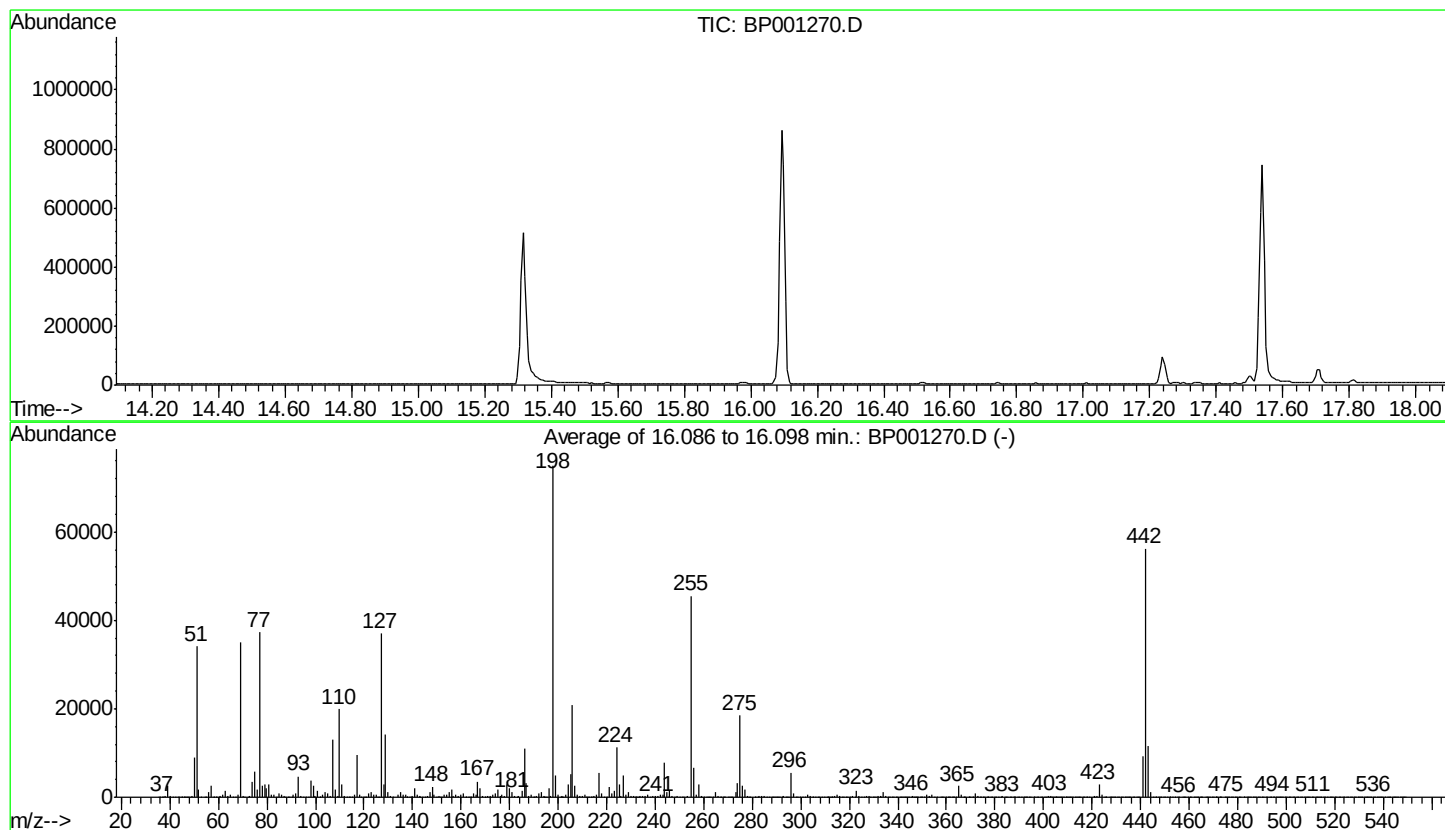

AutoFind: Scans 2380, 2381, 2382; Background Corrected with Scan 2372

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	34045	PASS
68	69	0.00	2	1.7	606	PASS
69	198	0.00	100	46.9	35148	PASS
70	69	0.00	2	0.5	170	PASS
127	198	10	80	49.3	36950	PASS
197	198	0.00	2	0.2	176	PASS
198	198	100	100	100.0	74976	PASS
199	198	5	9	6.6	4959	PASS
275	198	10	60	24.7	18492	PASS
365	198	1	100	3.3	2482	PASS
441	198	0.01	100	12.3	9250	PASS
442	198	50	100	74.9	56155	PASS
443	442	15	24	20.5	11504	PASS