
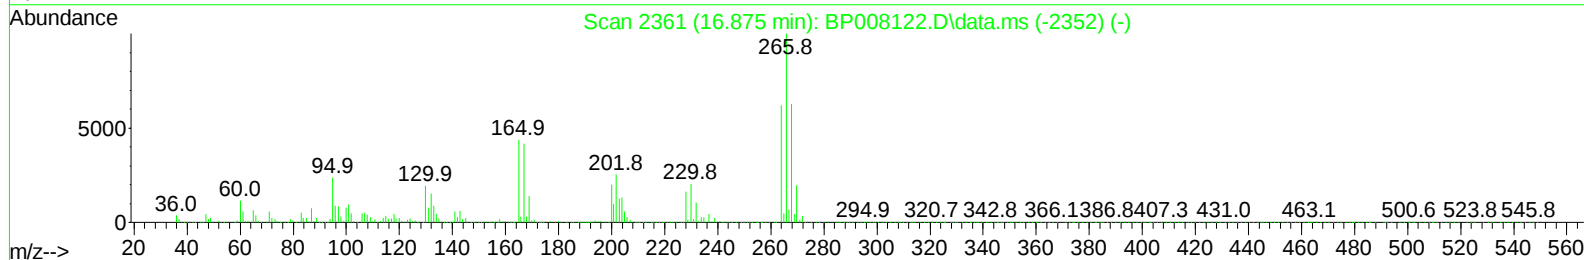
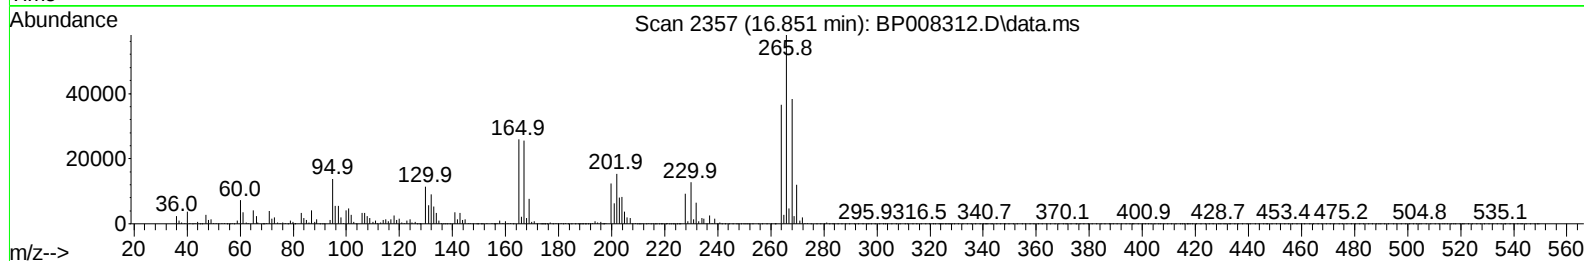


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120921\
Data File : BP008312.D
Acq On : 09 Dec 2021 15:26
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 05:44:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 01:43:36 2021
Response via : Initial Calibration

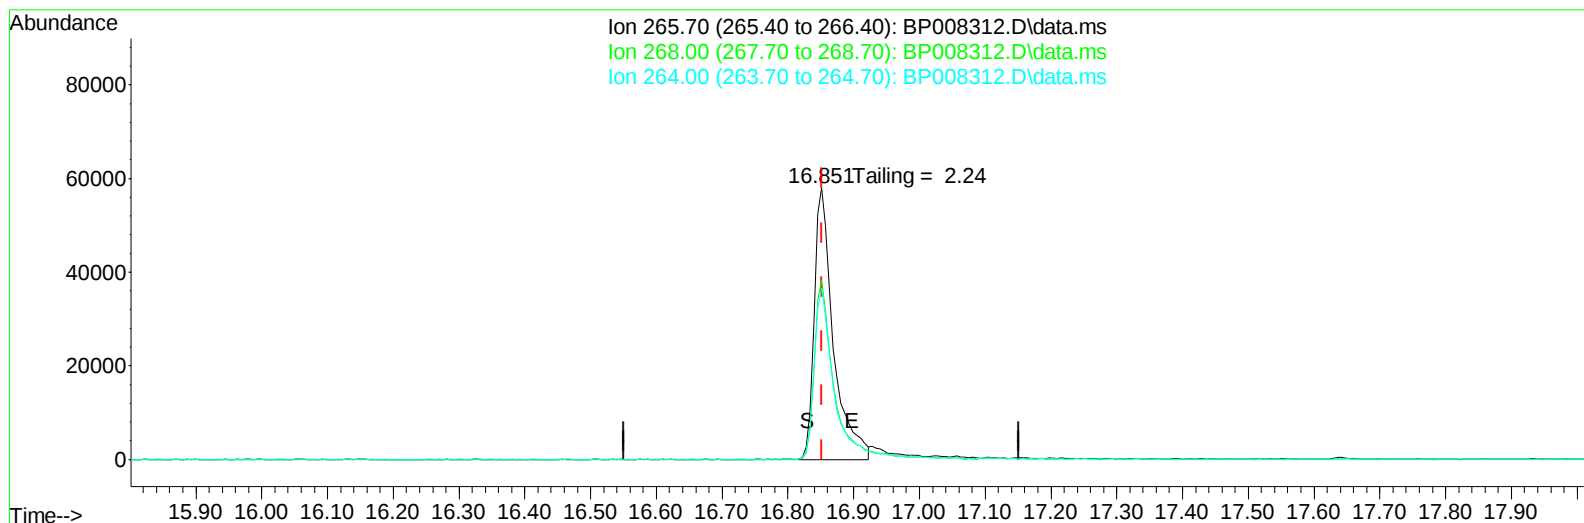

TIC: BP008312.D\data.ms

(70) Pentachlorophenol (C)




16.851min (+ 0.000) 1171304.89 ng

response 124183

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.25
264.00	61.90	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120921\
Data File : BP008312.D
Acq On : 09 Dec 2021 15:26
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 10 05:44:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 01:43:36 2021
Response via : Initial Calibration

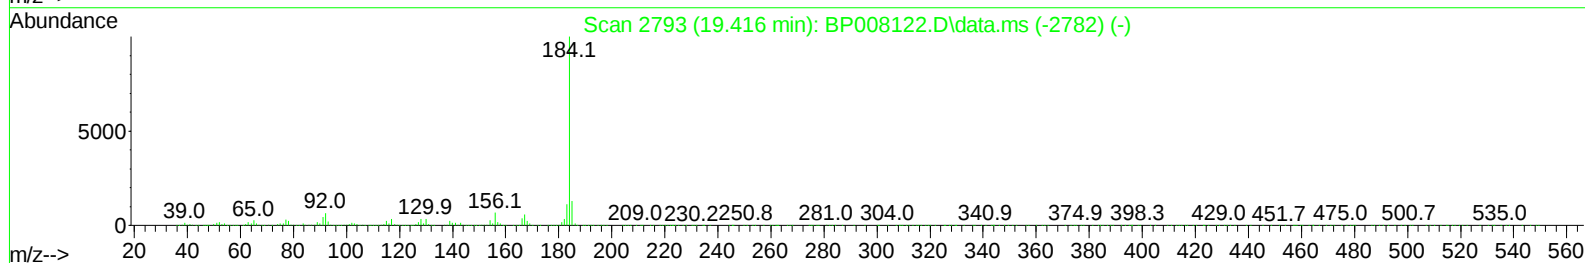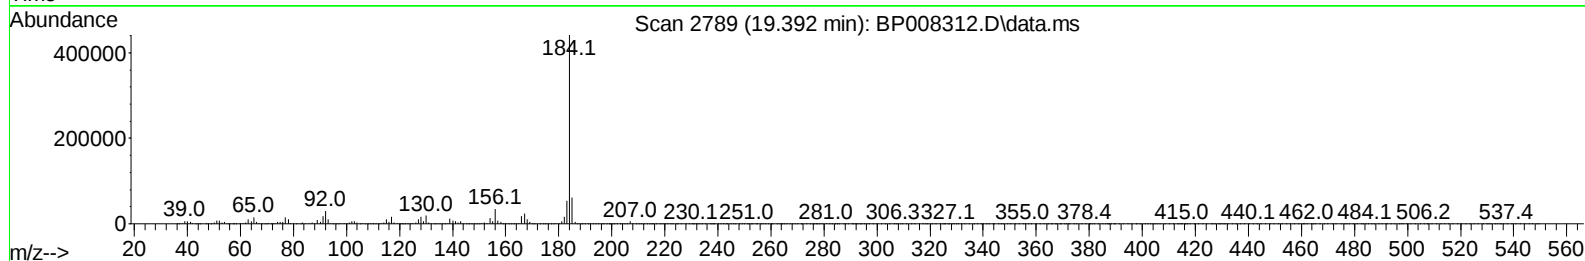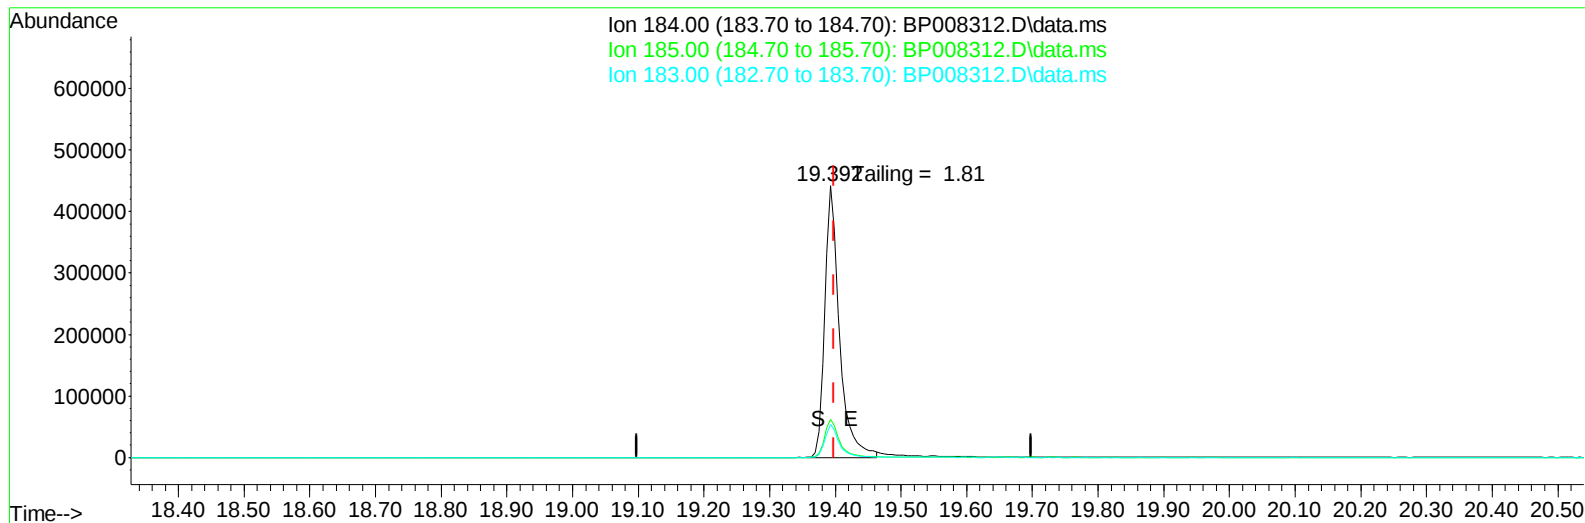

TIC: BP008312.D\data.ms

(77) Benzidine**19.392min (-0.006) 889538.81 ng****response 707716**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.05
183.00	11.40	12.08
0.00	0.00	0.00