

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120921\
 Data File : BP008305.D
 Acq On : 09 Dec 2021 10:40
 Operator : CG/JU
 Sample : PB141259BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB141259BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	398	405	426	rBV	1252227	1953305	50.94%	11.468%
2	6.963	668	676	696	rBV	1059236	1888209	49.24%	11.086%
3	7.769	807	813	825	rBV	222957	356295	9.29%	2.092%
4	8.934	1004	1011	1031	rBV	700491	1233360	32.17%	7.241%
5	10.569	1282	1289	1302	rBV	238446	451301	11.77%	2.650%
6	13.039	1702	1709	1728	rBV	1510995	2410184	62.86%	14.151%
7	14.427	1938	1945	1957	rBV	333941	545061	14.22%	3.200%
8	15.927	2193	2200	2220	rBV	1032823	1752589	45.71%	10.290%
9	17.192	2407	2415	2431	rBV	378057	644703	16.81%	3.785%
10	19.762	2846	2852	2864	rBV	3208234	3834353	100.00%	22.512%
11	21.080	3074	3076	3083	rVB	34862	46534	1.21%	0.273%
12	21.298	3108	3113	3122	rBV	612520	837540	21.84%	4.917%
13	21.415	3129	3133	3144	rBV	100240	182981	4.77%	1.074%
14	23.686	3513	3519	3530	rVB2	410716	895721	23.36%	5.259%

Sum of corrected areas: 17032136

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120921\
Data File : BP008305.D
Acq On : 09 Dec 2021 10:40
Operator : CG/JU
Sample : PB141259BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141259BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.415	4.37 ng	182981	Chrysene-d12	21.298

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	91
2			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	47
3			2-Phenyl-6-(trifluoromethyl)-1H...	277	C15H10F3NO	1000387-59-3	47
4			Dimethoxymethyl-hydroxy-tripheny...	354	C21H23O3P	1000132-00-1	47
5			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	43

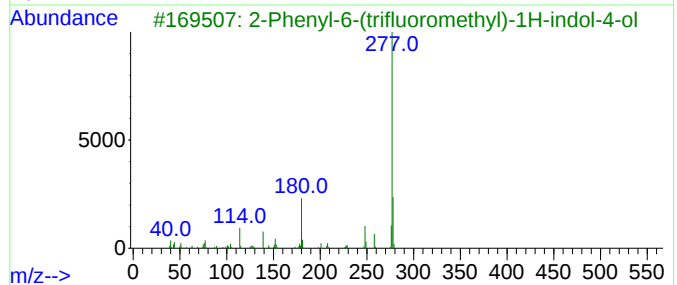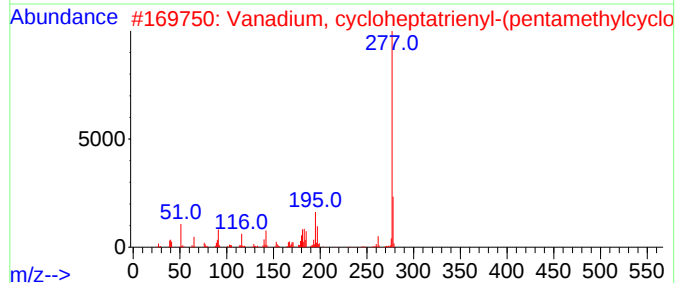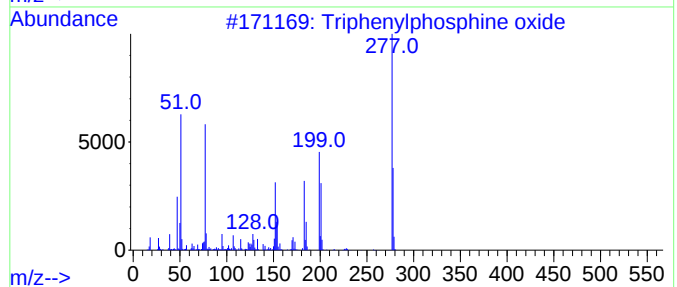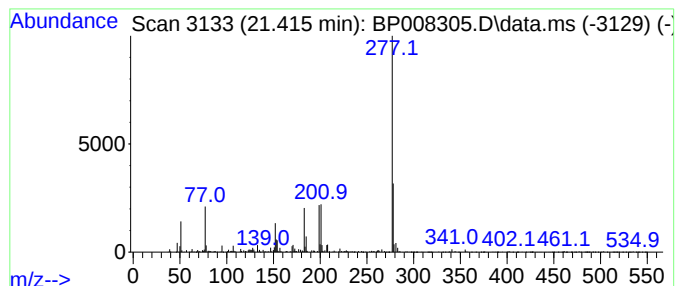

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120921\
Data File : BP008305.D
Acq On : 09 Dec 2021 10:40
Operator : CG/JU
Sample : PB141259BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141259BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	21.415	4.4	ng	182981	5	21.298	837540	20.0