
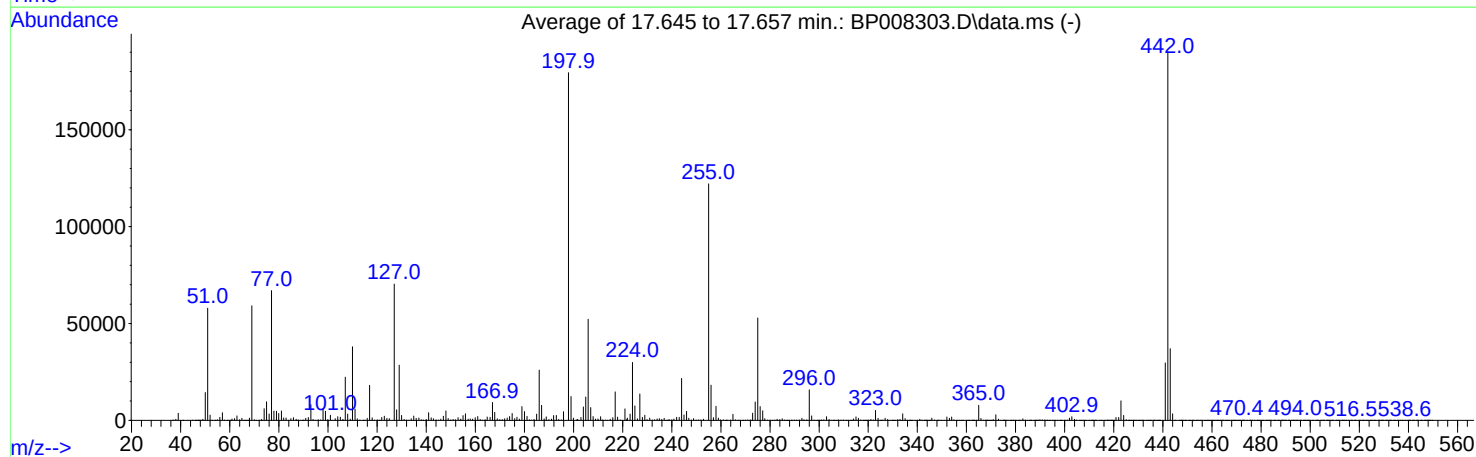


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP120921\  
 Data File : BP008303.D  
 Acq On : 09 Dec 2021 09:32  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP112521.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sat Dec 11 03:53:01 2021

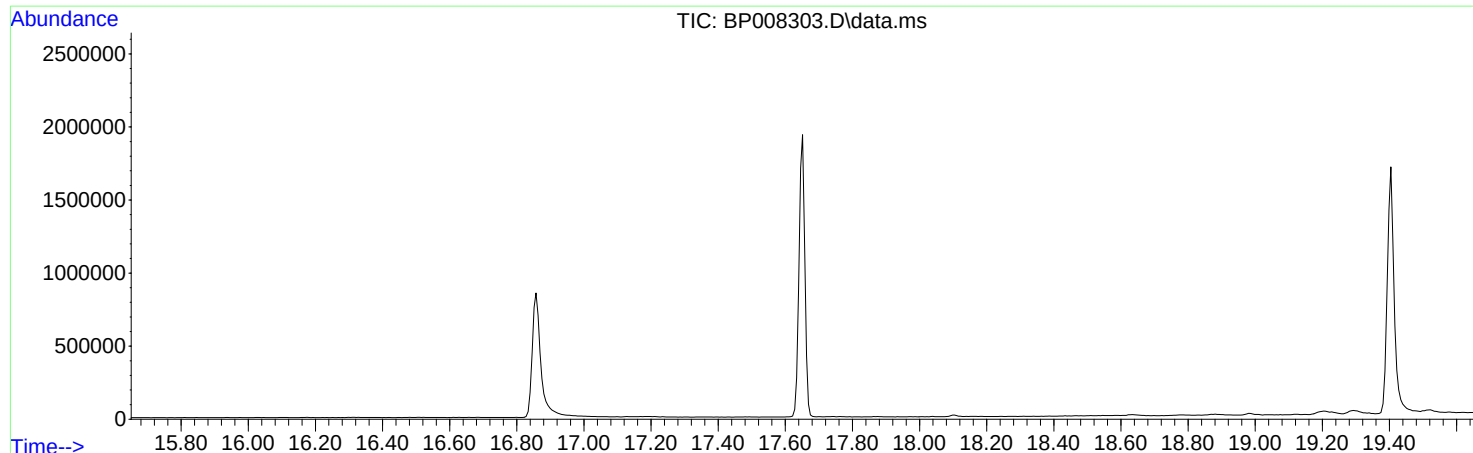




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2479

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 32.3         | 57929      | PASS                |
| 68             | 69              | 0.00            | 2               | 2.0          | 1154       | PASS                |
| 69             | 198             | 0.00            | 100             | 33.0         | 59161      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 366        | PASS                |
| 127            | 198             | 10              | 80              | 39.2         | 70383      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 179463     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 12330      | PASS                |
| 275            | 198             | 10              | 60              | 29.5         | 52852      | PASS                |
| 365            | 198             | 1               | 100             | 4.3          | 7752       | PASS                |
| 441            | 198             | 0.01            | 100             | 16.5         | 29656      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 189867     | PASS                |
| 443            | 442             | 15              | 24              | 19.5         | 37024      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP120921\  
Data File : BP008303.D  
Acq On : 09 Dec 2021 09:32  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Dec 10 05:42:13 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP112521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 09 01:43:36 2021  
Response via : Initial Calibration

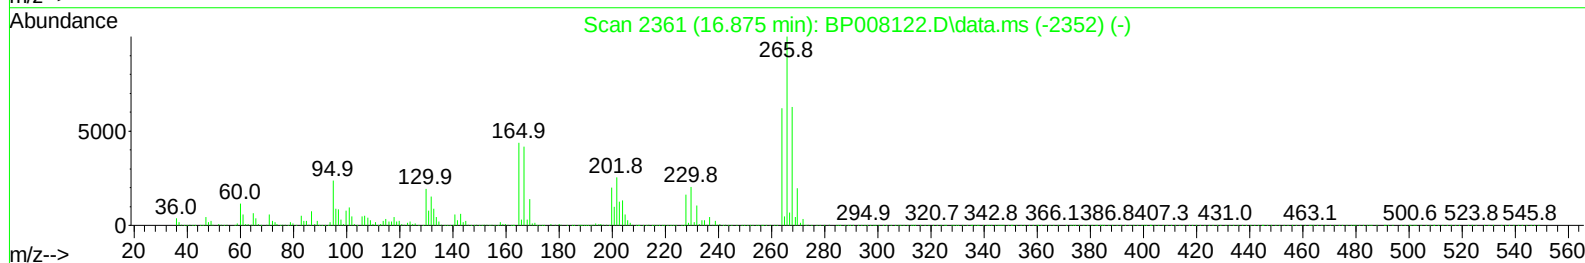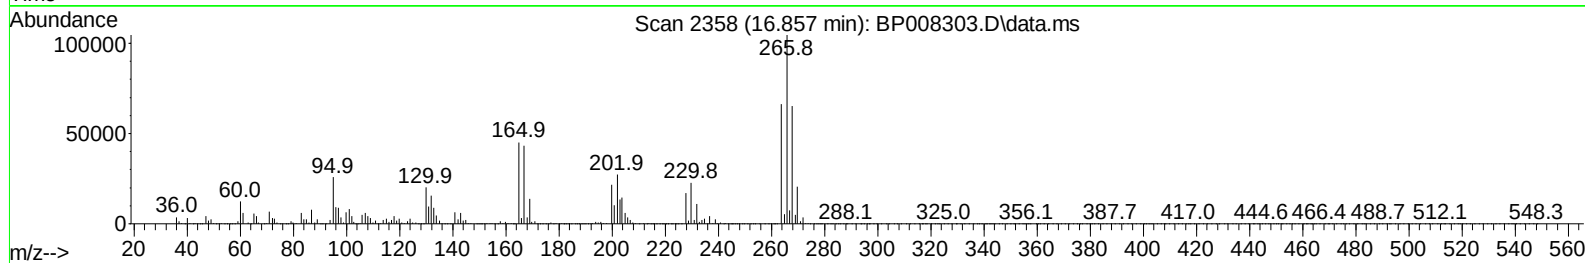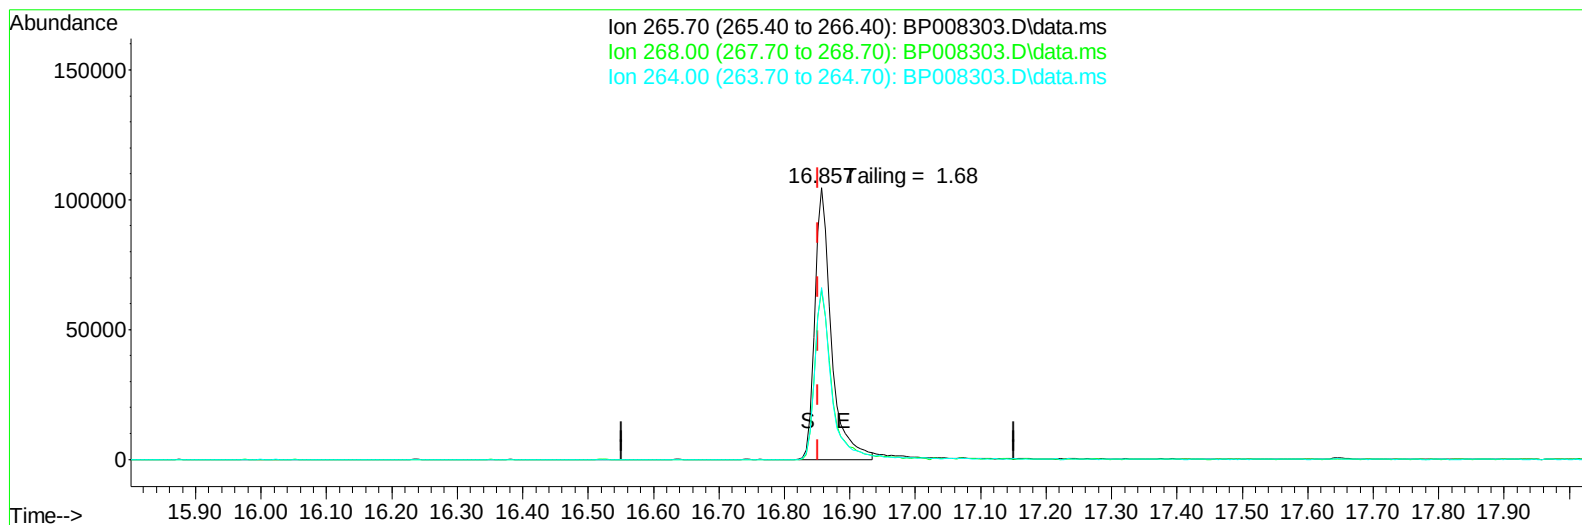

TIC: BP008303.D\data.ms

**(70) Pentachlorophenol (C)**

**16.857min (+ 0.006) 2439935.21 ng**




**response 189702**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.60  | 62.41  |
| 264.00 | 61.90  | 63.32  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP120921\  
Data File : BP008303.D  
Acq On : 09 Dec 2021 09:32  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Dec 10 05:42:13 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP112521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 09 01:43:36 2021  
Response via : Initial Calibration

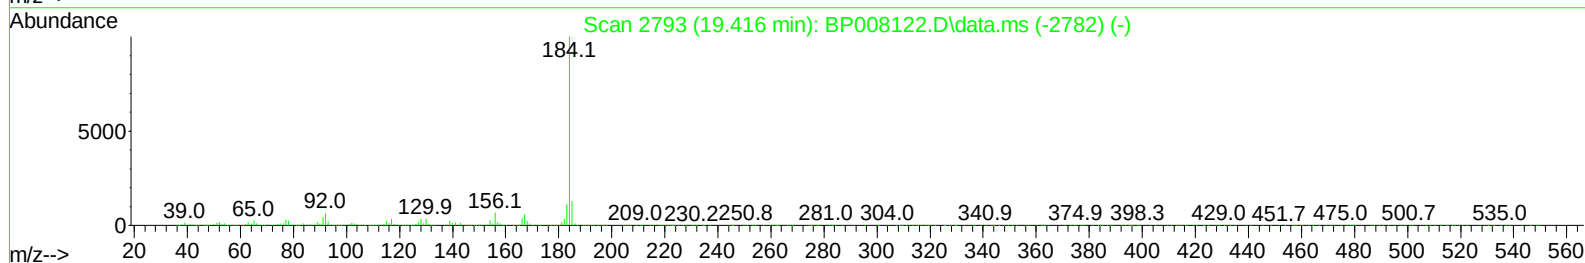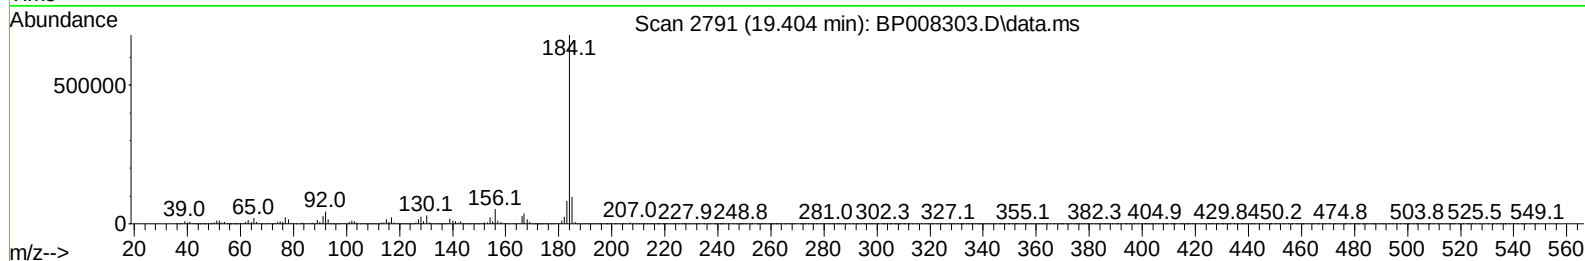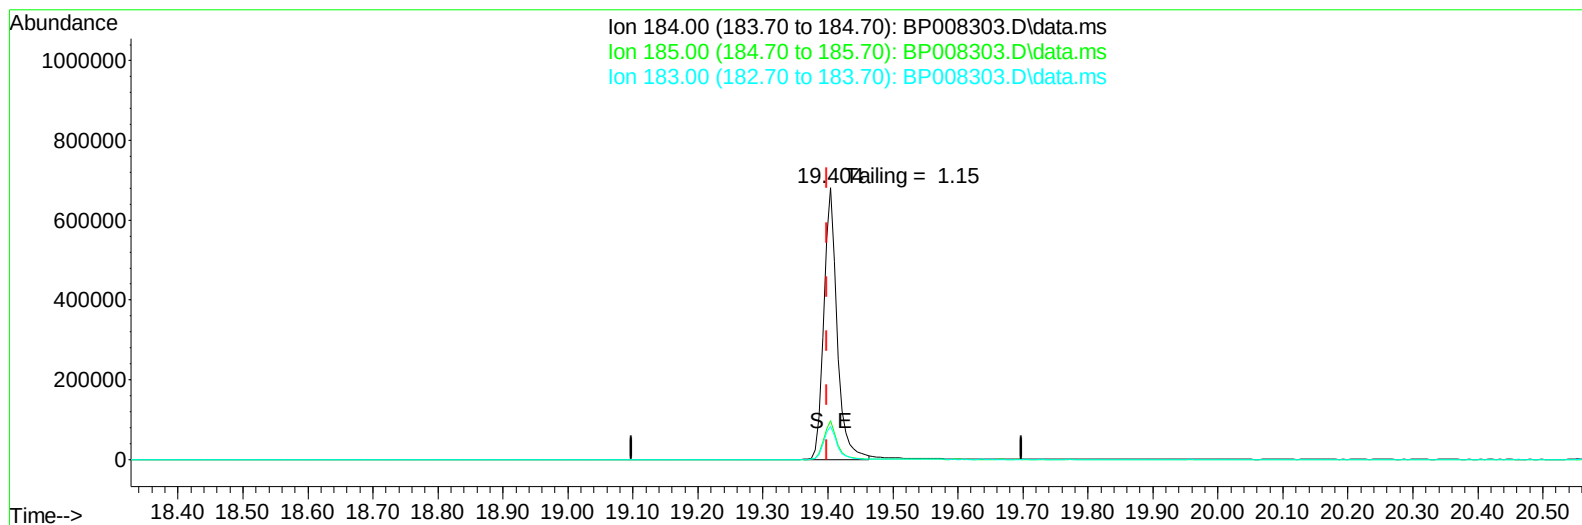

TIC: BP008303.D\data.ms

(77) Benzidine

19.404min (+ 0.006) 604627.35 ng

response 986963

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 12.90  | 14.17  |
| 183.00 | 11.40  | 12.10  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 12/9/2021     | BNA_P            | BP008303.D         |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 615362           | 20.604             |
| DDD           | 18418            | 20.181             |
| DDE           | 2811             | 19.681             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 21229         | 636591           | 3.33               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP