
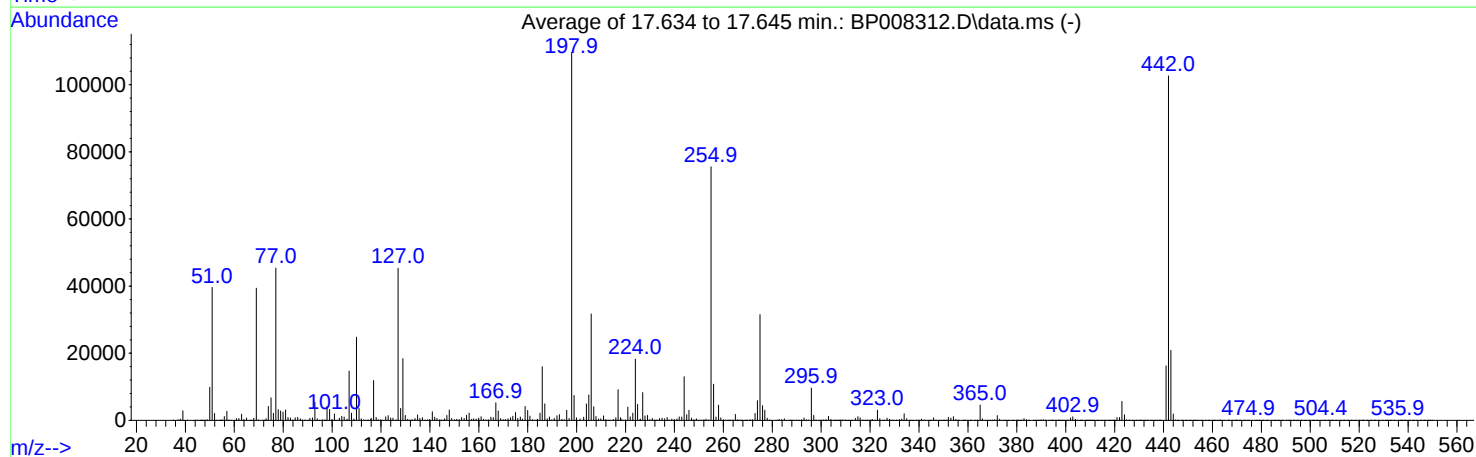


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120921\
 Data File : BP008312.D
 Acq On : 09 Dec 2021 15:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 03:53:01 2021

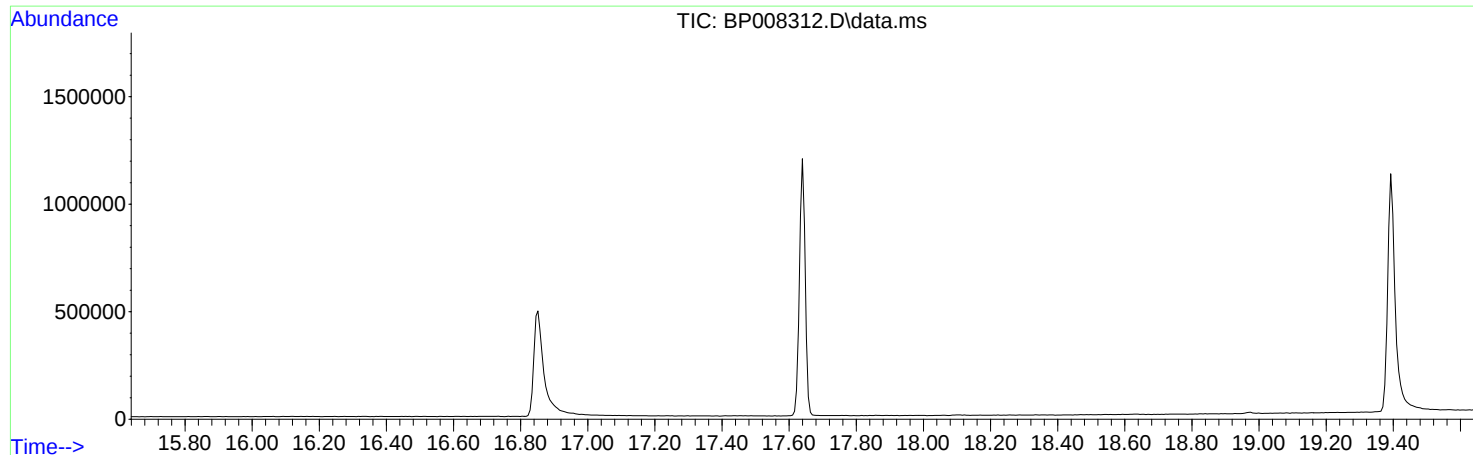




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	39613	PASS
68	69	0.00	2	1.6	636	PASS
69	198	0.00	100	35.9	39378	PASS
70	69	0.00	2	0.4	165	PASS
127	198	10	80	41.3	45317	PASS
197	198	0.00	2	0.5	576	PASS
198	198	100	100	100.0	109600	PASS
199	198	5	9	6.8	7436	PASS
275	198	10	60	28.8	31536	PASS
365	198	1	100	4.2	4556	PASS
441	198	0.01	100	14.8	16242	PASS
442	442	100	100	100.0	102627	PASS
443	442	15	24	20.4	20888	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120921\
Data File : BP008312.D
Acq On : 09 Dec 2021 15:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 10 05:44:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 01:43:36 2021
Response via : Initial Calibration

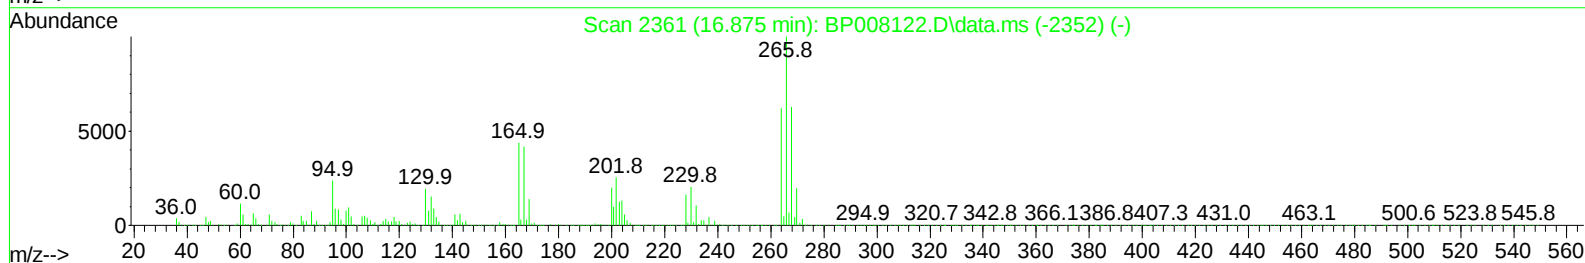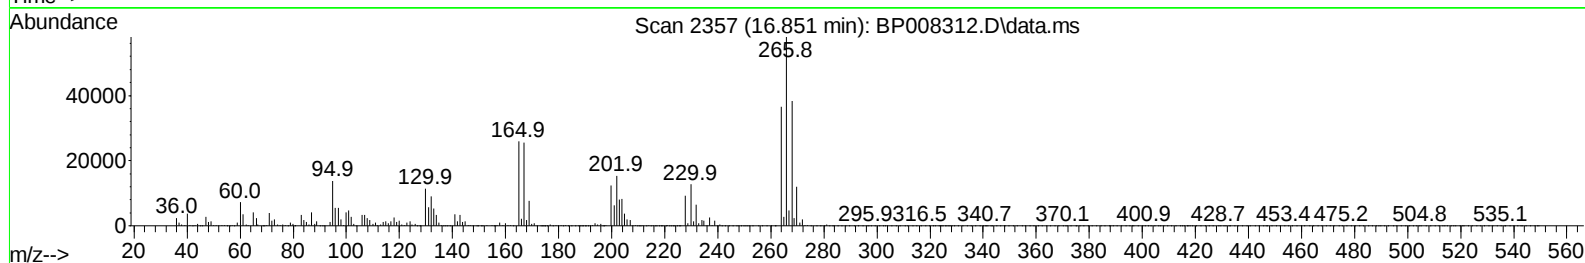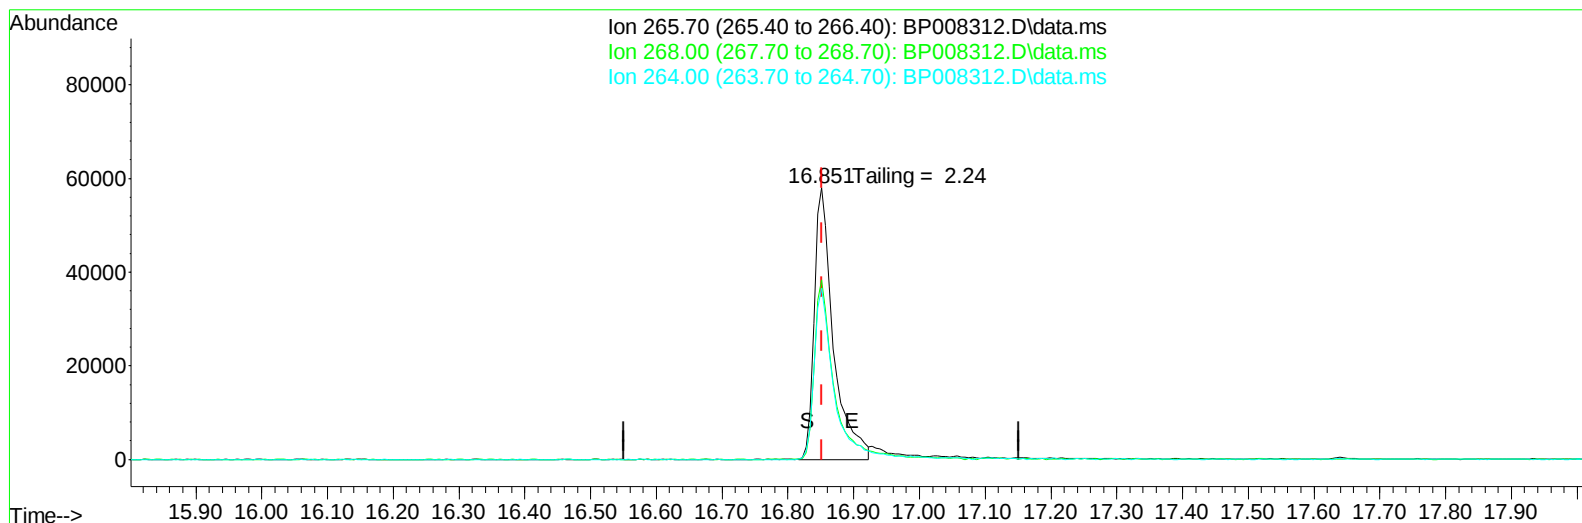

TIC: BP008312.D\data.ms

(70) Pentachlorophenol (C)

16.851min (+ 0.000) 1171304.89 ng




response 124183

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.25
264.00	61.90	63.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120921\
 Data File : BP008312.D
 Acq On : 09 Dec 2021 15:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 10 05:44:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 01:43:36 2021
 Response via : Initial Calibration

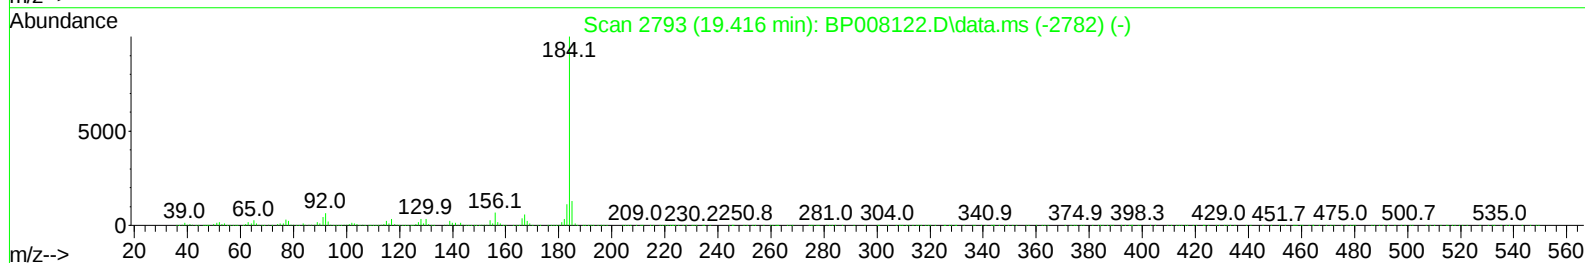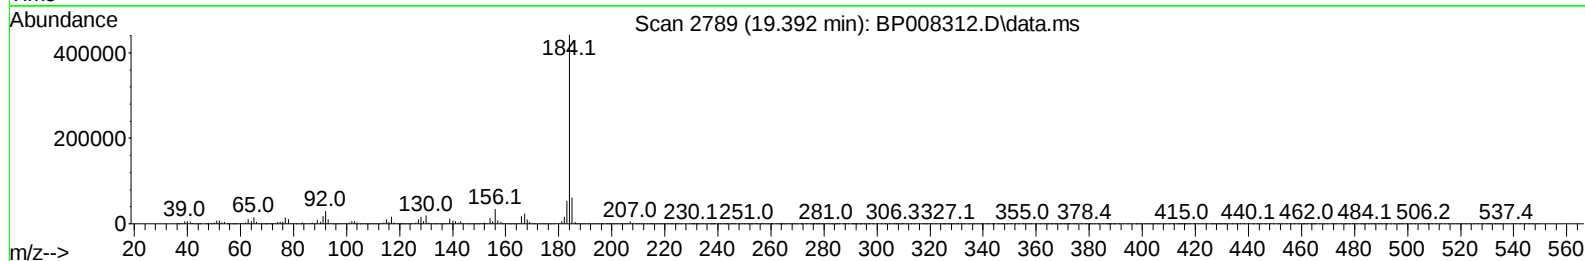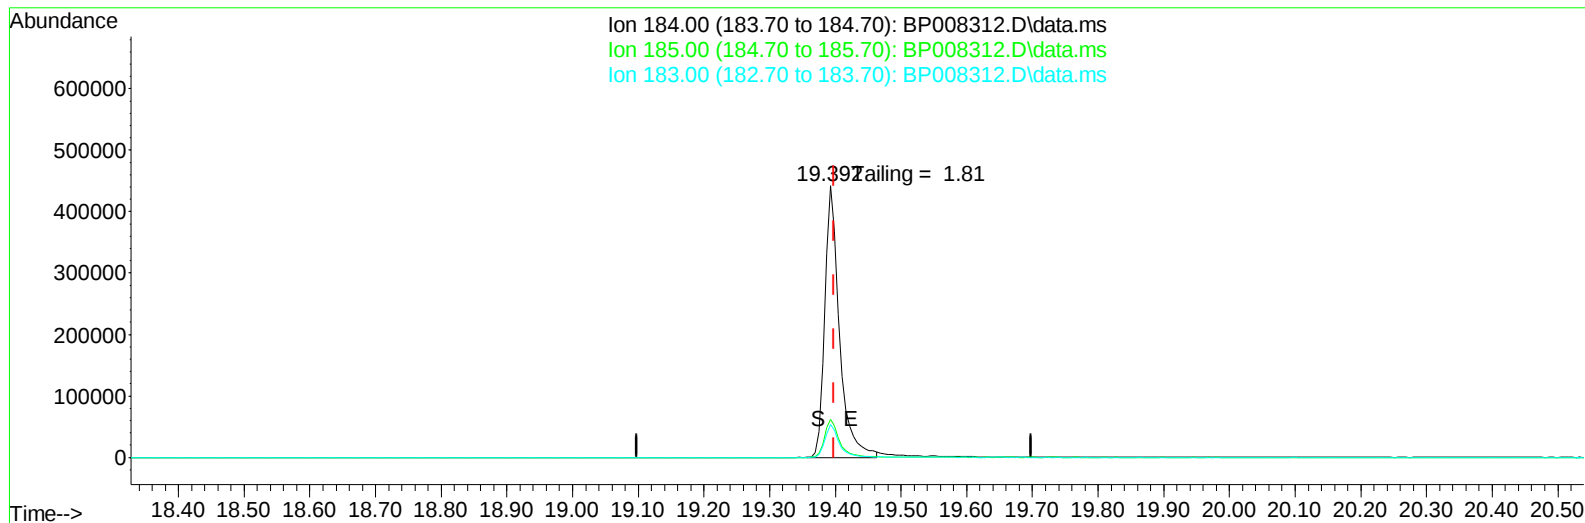

TIC: BP008312.D\data.ms

(77) Benzidine**19.392min (-0.006) 889538.81 ng****response 707716**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.05
183.00	11.40	12.08
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
12/9/2021	BNA_P	BP008312.D
Compound Name	Response	Retention Time
DDT	388151	20.592
DDD	7896	20.169
DDE	1250	19.675
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9146	397297	2.30

Instrument :
BNA_P
ClientSampleId :
DFTPP