
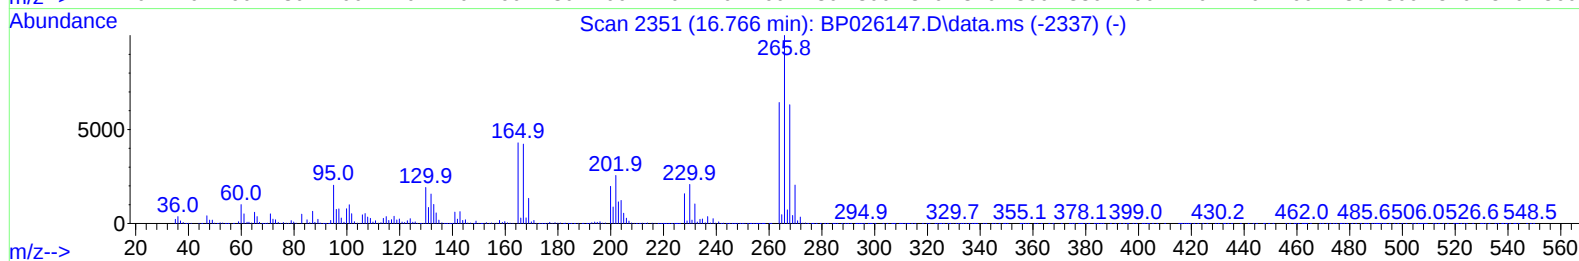
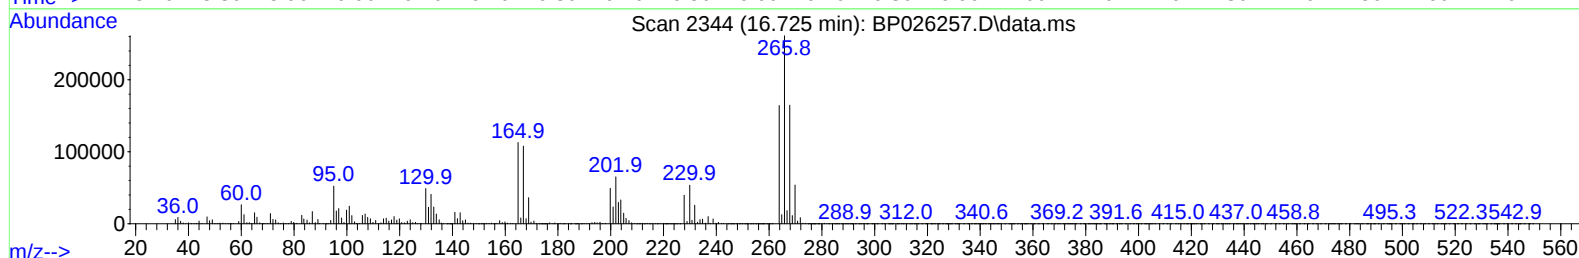


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120925\
Data File : BP026257.D
Acq On : 09 Dec 2025 11:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 11:53:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

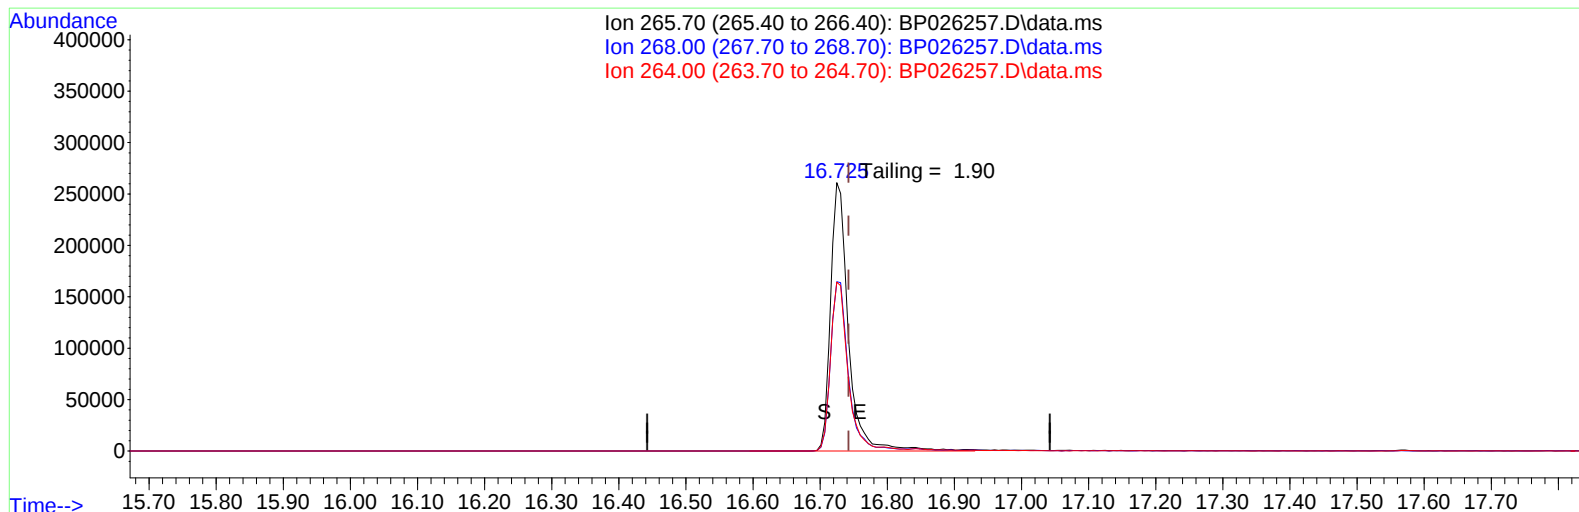

TIC: BP026257.D\data.ms

(70) Pentachlorophenol (C)




16.725min (-0.018) 2411089.14 ng

response 474123

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.10
264.00	62.70	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120925\
Data File : BP026257.D
Acq On : 09 Dec 2025 11:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 11:53:11 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

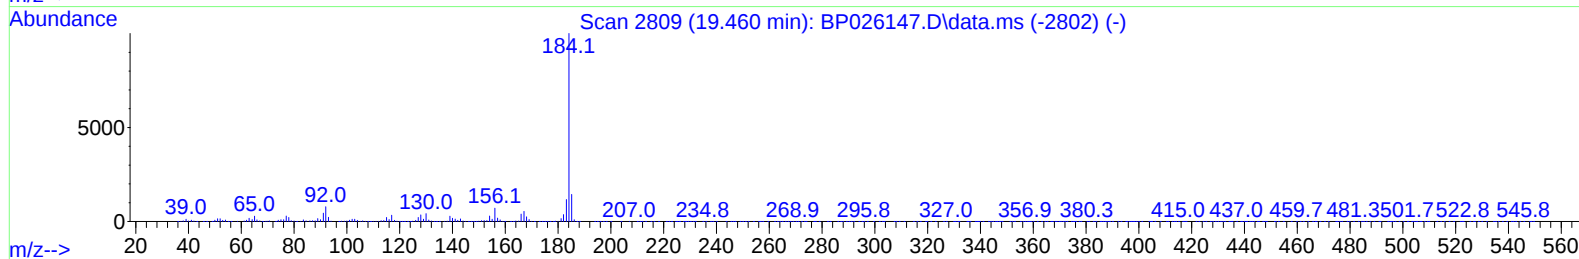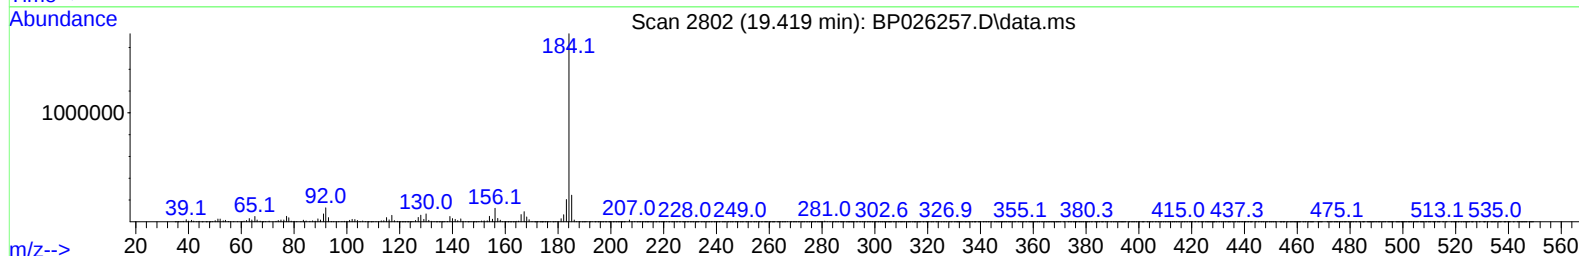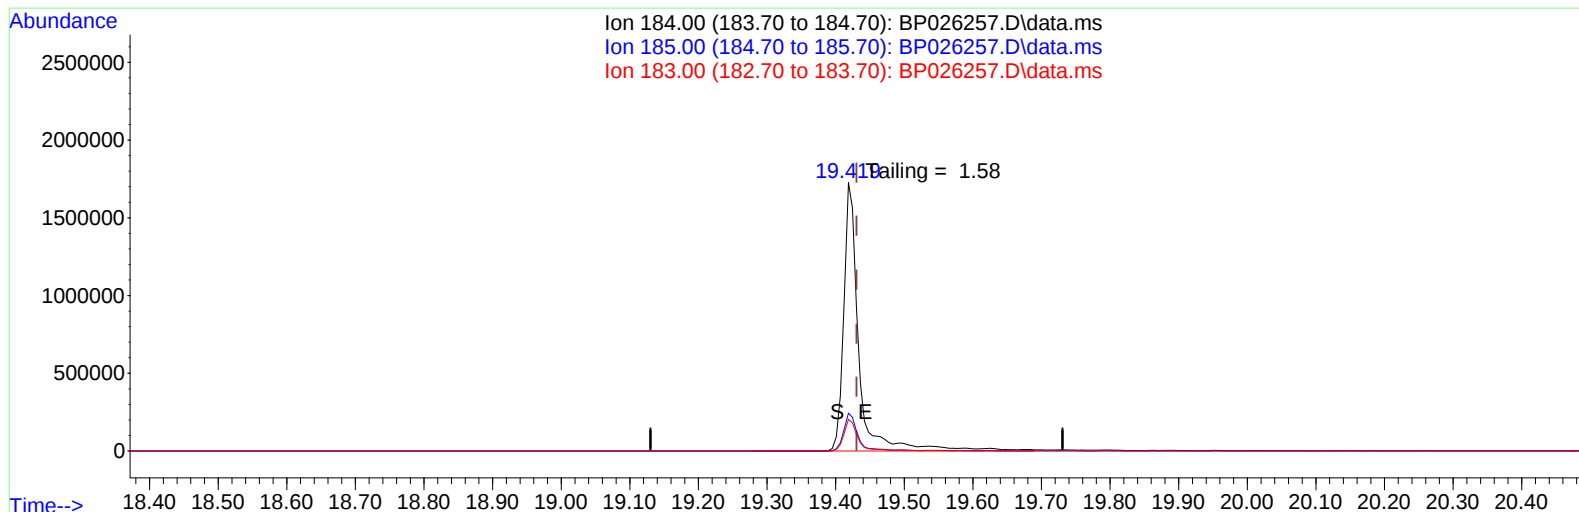

TIC: BP026257.D\data.ms

(77) Benzidine**19.419min (-0.012) 322564.15 ng****response 2420441**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.17
183.00	11.30	11.84
0.00	0.00	0.00