
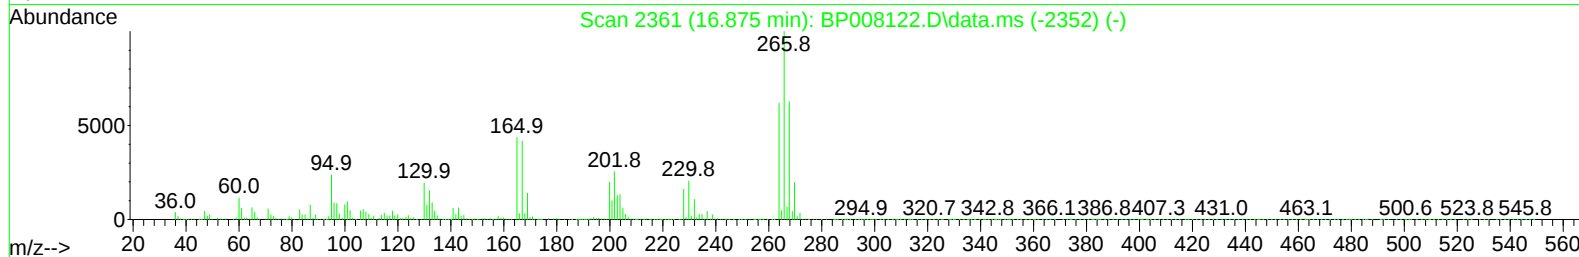
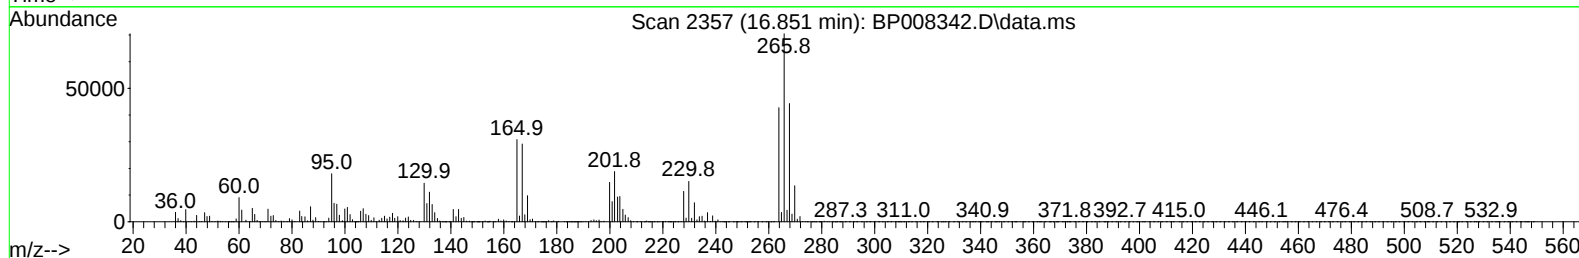


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
 Data File : BP008342.D
 Acq On : 10 Dec 2021 15:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 03:48:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 01:43:36 2021
 Response via : Initial Calibration

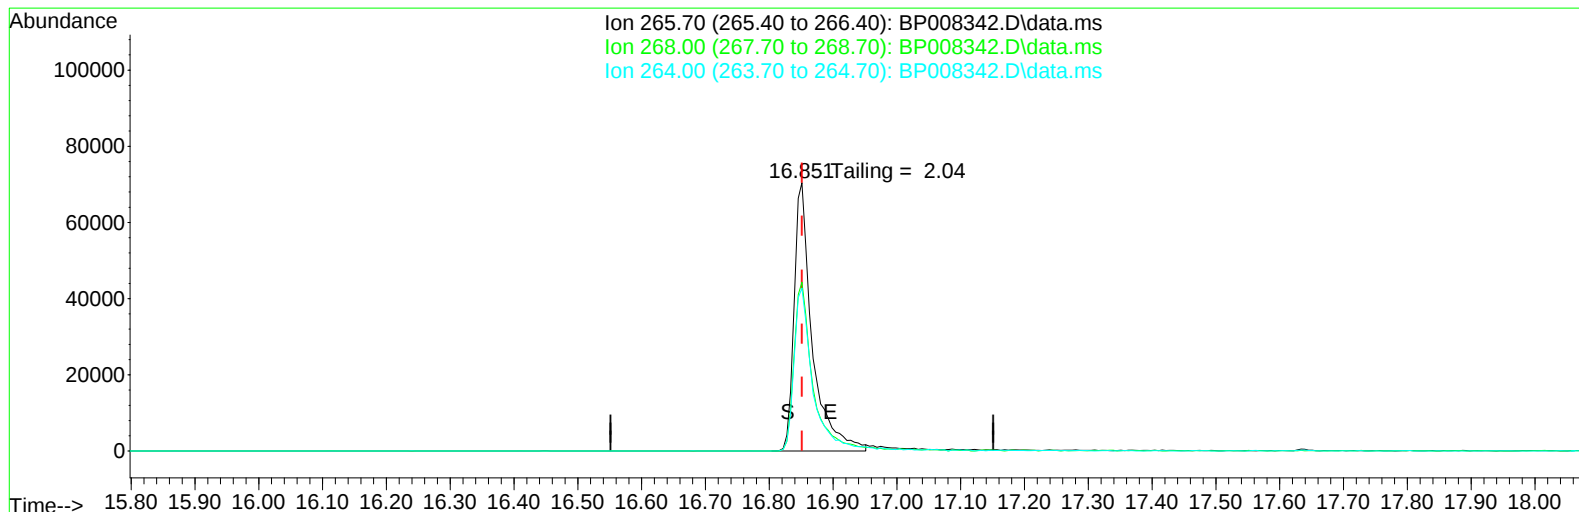

TIC: BP008342.D\data.ms

(70) Pentachlorophenol (C)




16.851min (+ 0.000) 314865.56 ng

response 144657

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.89
264.00	61.90	60.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
 Data File : BP008342.D
 Acq On : 10 Dec 2021 15:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 03:48:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 01:43:36 2021
 Response via : Initial Calibration

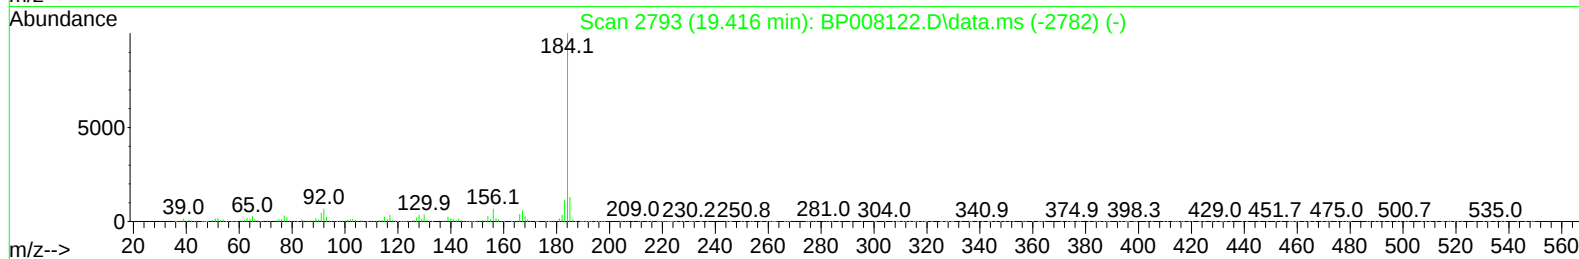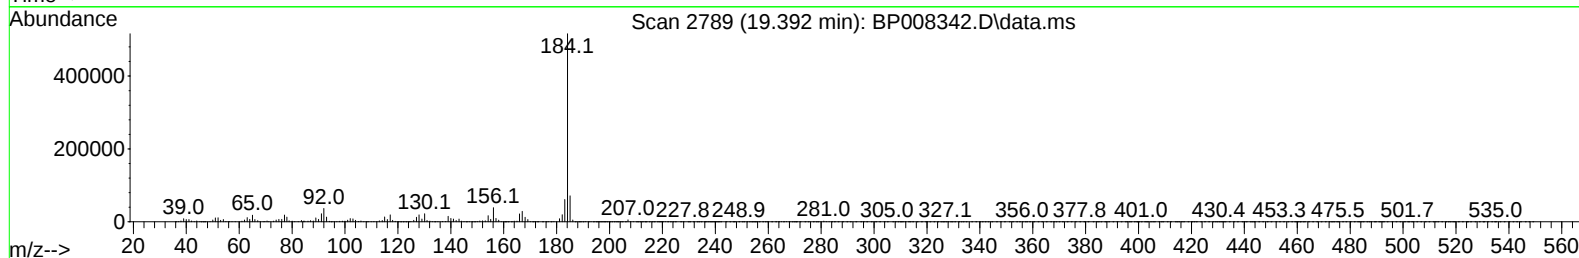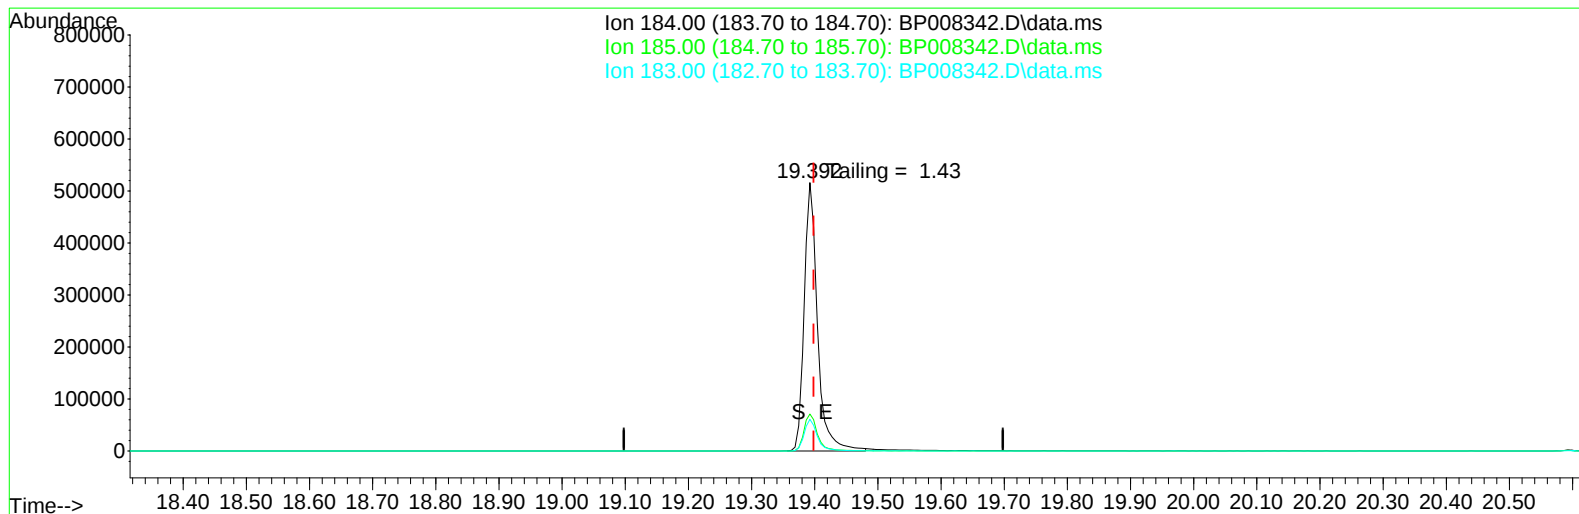

TIC: BP008342.D\data.ms

(77) Benzidine**19.392min (-0.006) 1449056.37 ng****response 775204**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.81
183.00	11.40	11.84
0.00	0.00	0.00