

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
 Data File : BP008360.D
 Acq On : 11 Dec 2021 02:11
 Operator : CG/JU
 Sample : M4980-01 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OK-03-120821

Quant Time: Dec 11 04:03:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 03:53:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.758	152	70997	20.000	ng	0.00
21) Naphthalene-d8	10.557	136	245704	20.000	ng	0.00
39) Acenaphthene-d10	14.410	164	154974	20.000	ng	0.00
64) Phenanthrene-d10	17.175	188	339118	20.000	ng	0.00
76) Chrysene-d12	21.286	240	393156	20.000	ng	0.00
86) Perylene-d12	23.663	264	436774	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.364	112	20675	4.689	ng	0.00
7) Phenol-d6	6.969	99	21841	3.669	ng	0.02
23) Nitrobenzene-d5	8.928	82	16020	2.965	ng	0.00
42) 2,4,6-Tribromophenol	15.922	330	8203	4.141	ng	0.00
45) 2-Fluorobiphenyl	13.034	172	33968	3.184	ng	0.00
79) Terphenyl-d14	19.751	244	66656	3.543	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
Data File : BP008360.D
Acq On : 11 Dec 2021 02:11
Operator : CG/JU
Sample : M4980-01 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-03-120821

Quant Time: Dec 11 04:03:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 03:53:01 2021
Response via : Initial Calibration



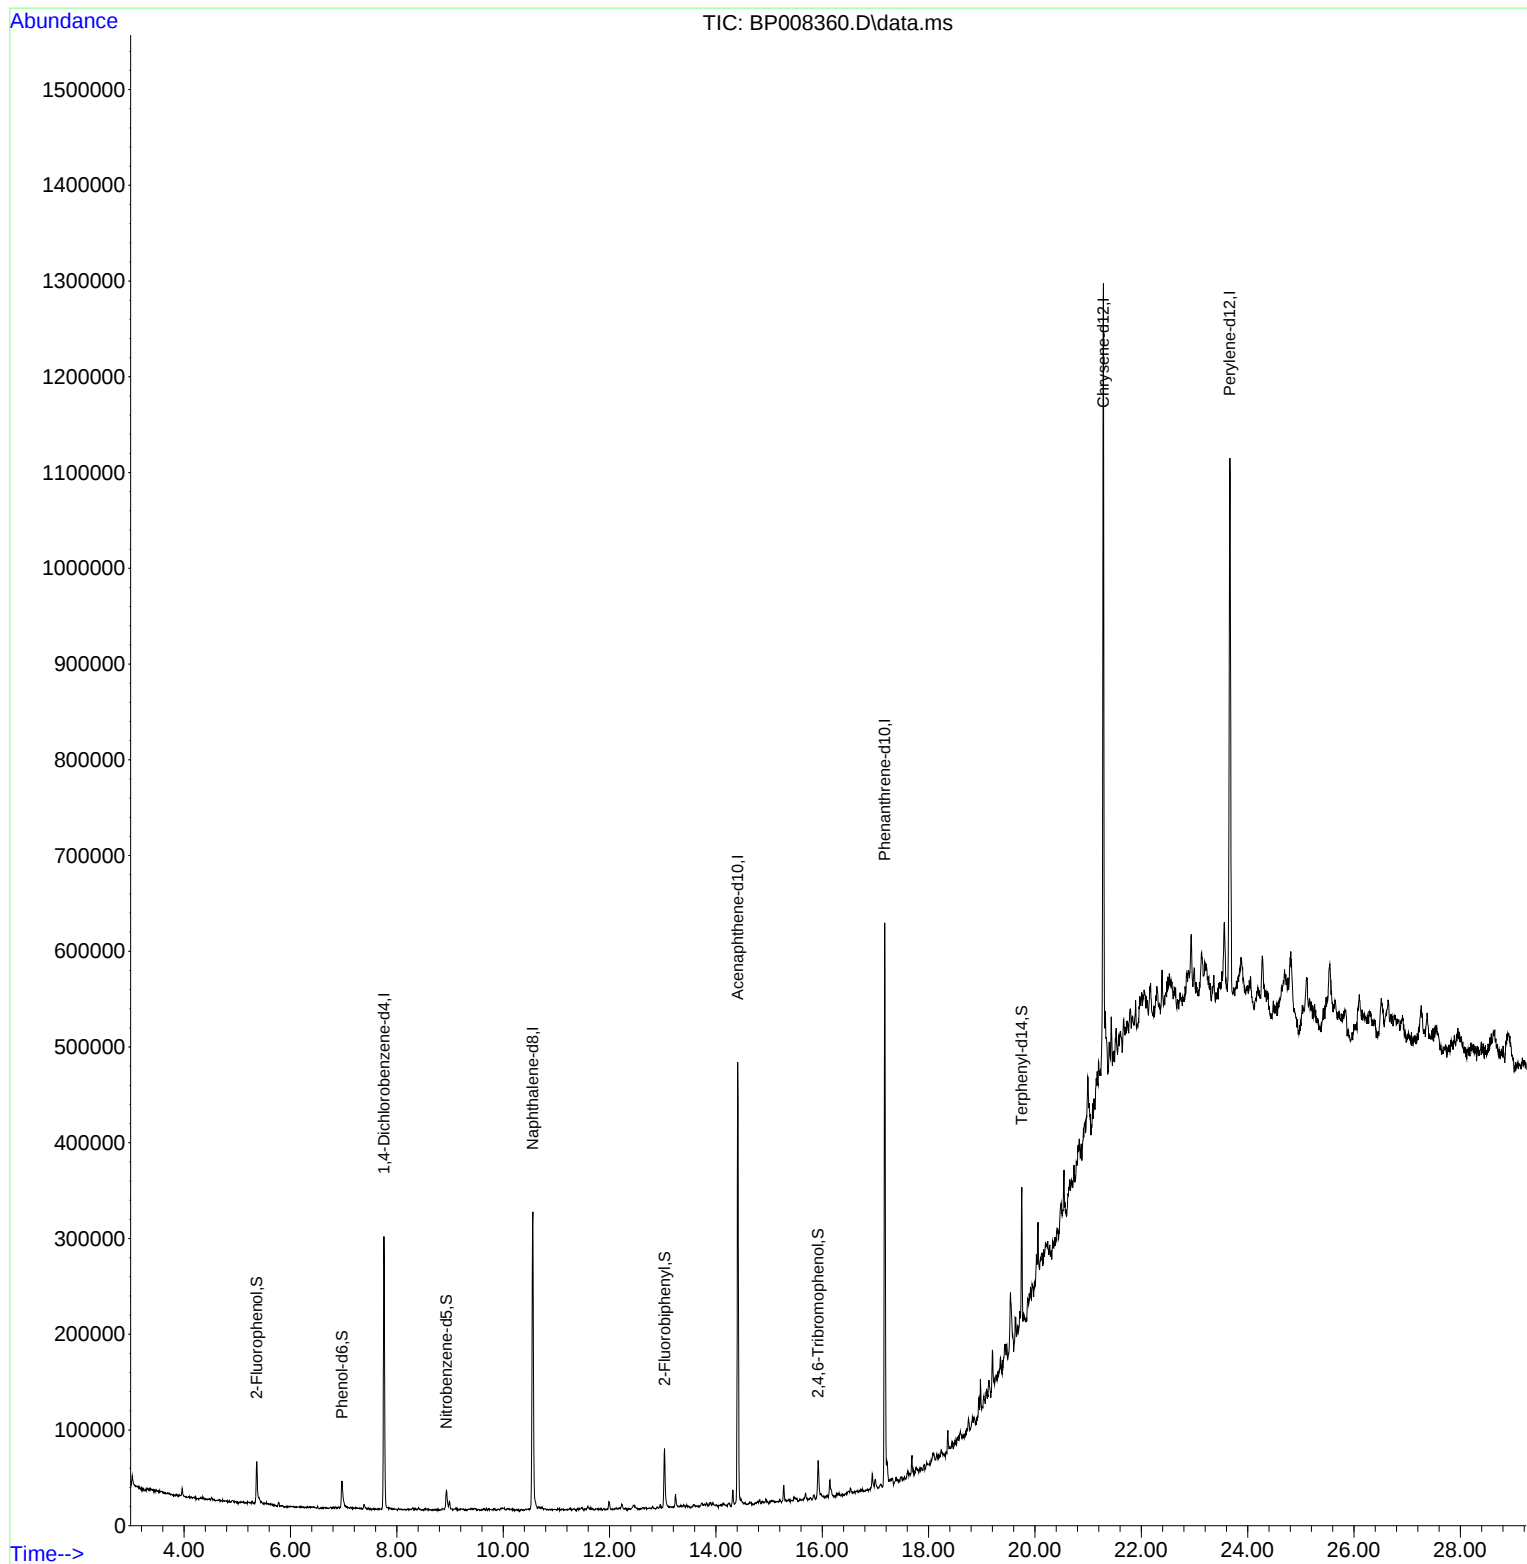


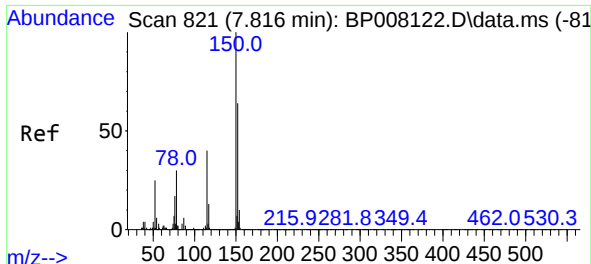

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.758 min Scan# 81
Delta R.T. -0.005 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11




Instrument :
BNA_P
ClientSampleId :
OK-03-120821

Tgt Ion:152 Resp: 70997
Ion Ratio Lower Upper
152 100
150 151.5 125.7 188.5
115 65.4 50.7 76.1

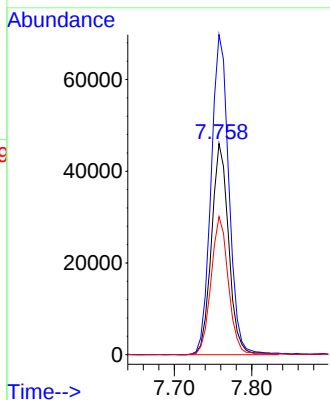

#5
2-Fluorophenol
Concen: 4.689 ng
RT: 5.364 min Scan# 404
Delta R.T. 0.006 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11

Tgt Ion:112 Resp: 20675
Ion Ratio Lower Upper
112 100
64 64.7 53.4 80.2
63 34.0 27.8 41.8


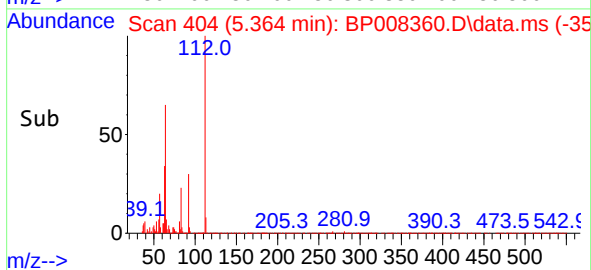
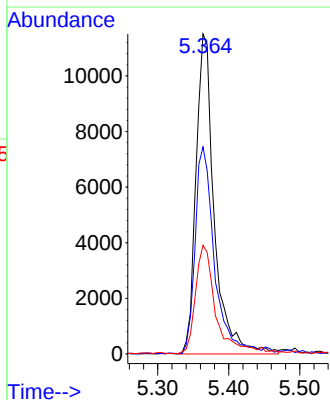
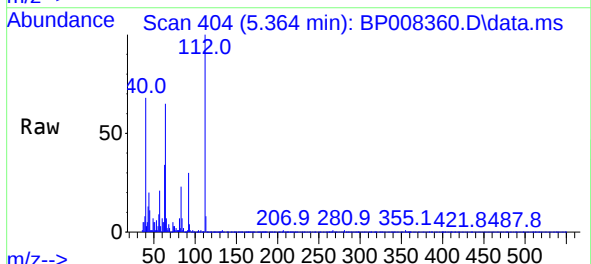




#7
Phenol-d6
Concen: 3.669 ng
RT: 6.969 min Scan# 61
Delta R.T. 0.018 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11




Instrument :
BNA_P
ClientSampleId :
OK-03-120821


Tgt Ion: 99 Resp: 21841
Ion Ratio Lower Upper
99 100
42 20.0 14.6 22.0
71 42.7 31.1 46.7

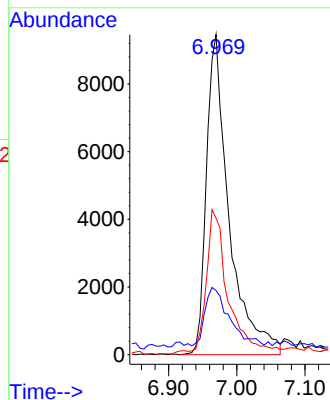

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.557 min Scan# 1287
Delta R.T. 0.000 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11

Tgt Ion: 136 Resp: 245704
Ion Ratio Lower Upper
136 100
137 10.6 9.0 13.6
54 10.3 8.2 12.4
68 6.3 5.8 8.8

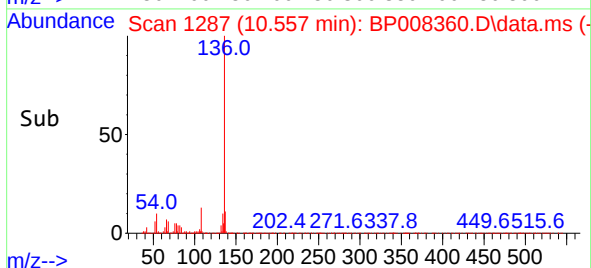
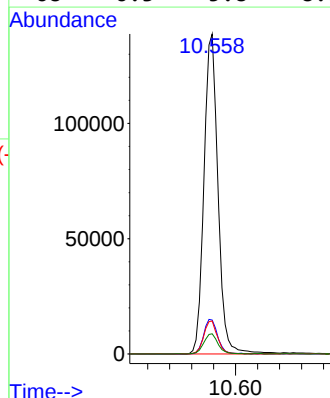
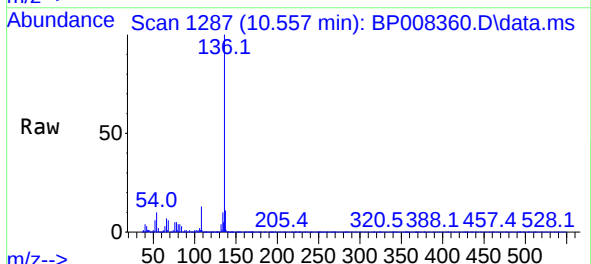


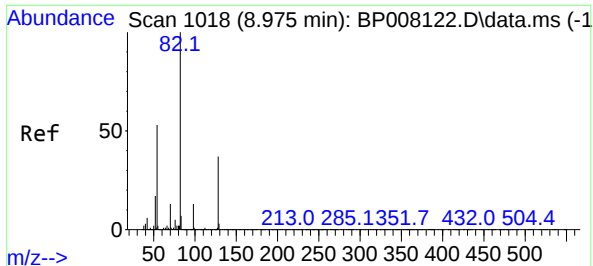

#23
Nitrobenzene-d5
Concen: 2.965 ng
RT: 8.928 min Scan# 1018
Delta R.T. 0.000 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11




Instrument :
BNA_P
ClientSampleId :
OK-03-120821


Tgt Ion: 82 Resp: 16020
Ion Ratio Lower Upper
82 100
128 38.6 29.6 44.4
54 48.8 42.7 64.1

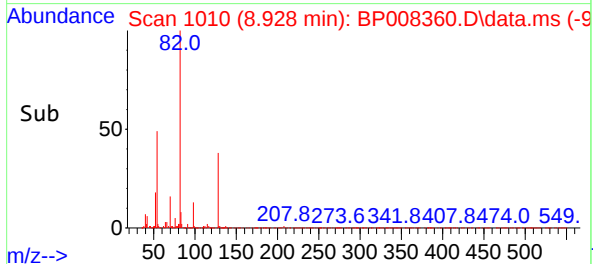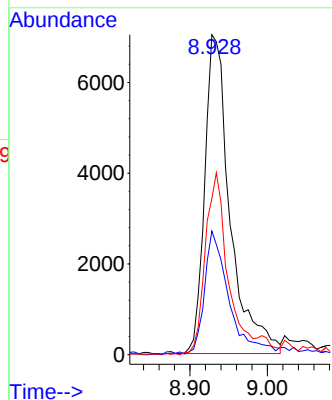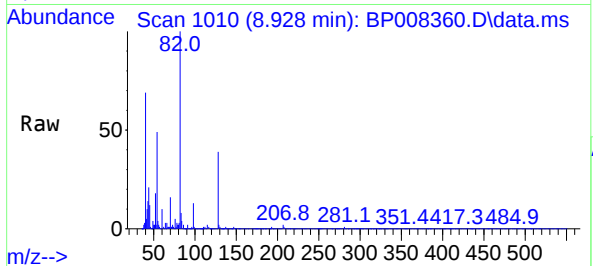

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.410 min Scan# 1942
Delta R.T. -0.006 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11

Tgt Ion: 164 Resp: 154974
Ion Ratio Lower Upper
164 100
162 100.4 81.9 122.9
160 44.1 35.4 53.0


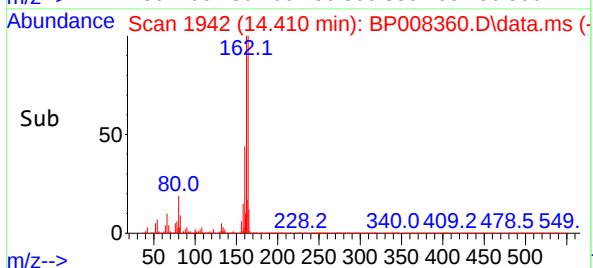
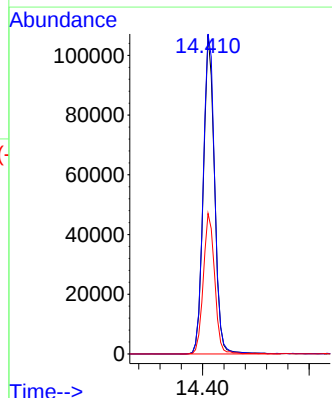
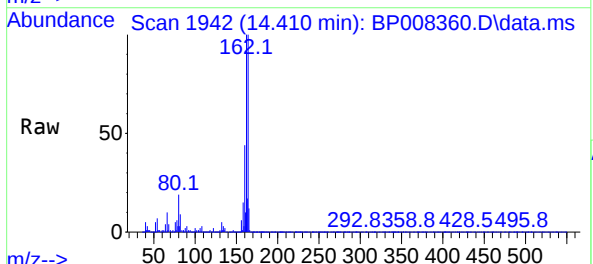


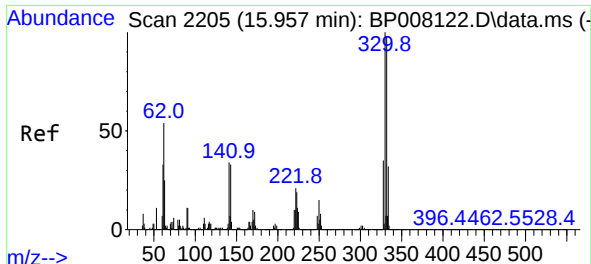

#42
2,4,6-Tribromophenol
Concen: 4.141 ng
RT: 15.922 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11




Instrument :
BNA_P
ClientSampleId :
OK-03-120821


Tgt Ion:	330	Resp:	8203
Ion	Ratio	Lower	Upper
330	100		
332	99.7	77.0	115.4
141	33.5	28.4	42.6

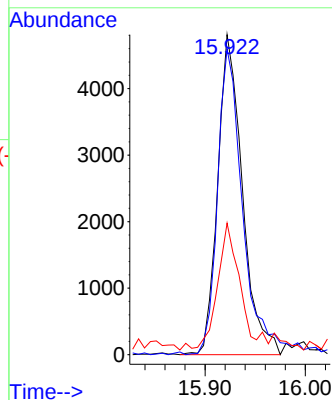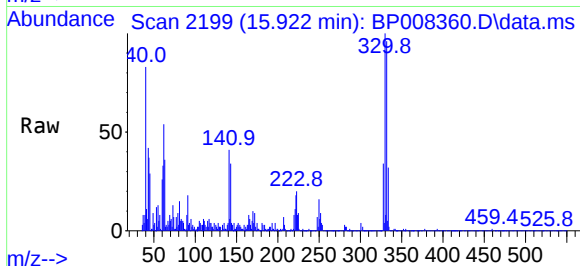

#45
2-Fluorobiphenyl
Concen: 3.184 ng
RT: 13.034 min Scan# 1708
Delta R.T. 0.000 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11

Tgt Ion:	172	Resp:	33968
Ion	Ratio	Lower	Upper
172	100		
171	36.1	28.0	42.0
170	25.9	18.9	28.3


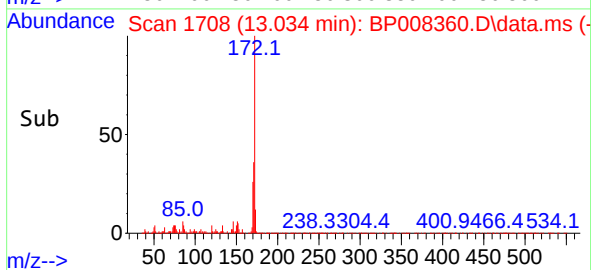
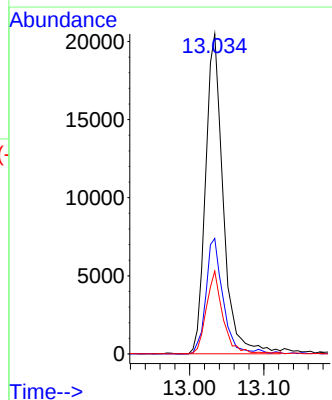
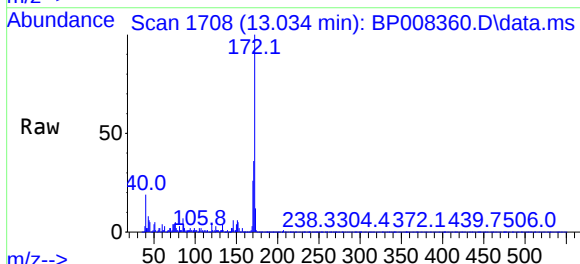




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.175 min Scan# 2419
Delta R.T. -0.006 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11




Instrument :
BNA_P
ClientSampleId :
OK-03-120821


Tgt Ion:188 Resp: 339118
Ion Ratio Lower Upper
188 100
94 8.1 7.2 10.8
80 9.5 8.2 12.4

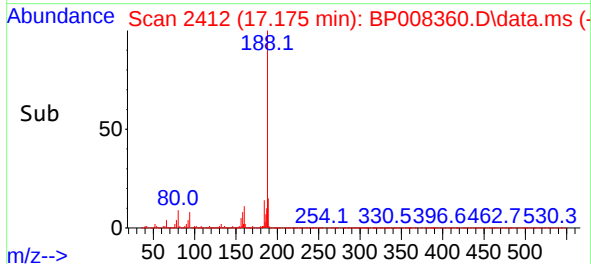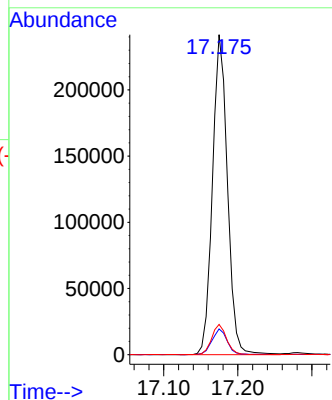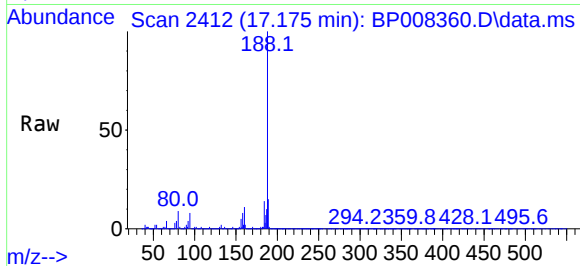

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.286 min Scan# 3111
Delta R.T. 0.000 min
Lab File: BP008360.D
Acq: 11 Dec 2021 02:11

Tgt Ion:240 Resp: 393156
Ion Ratio Lower Upper
240 100
120 7.5 7.3 10.9
236 26.3 21.4 32.2


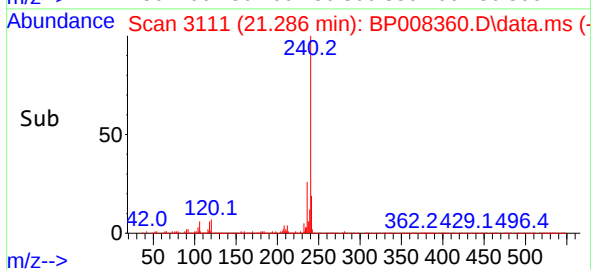
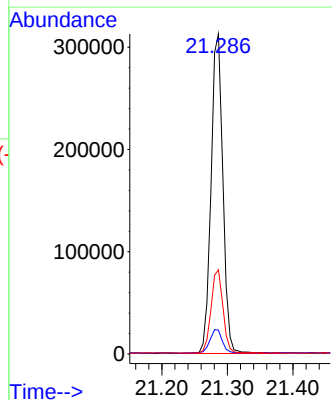
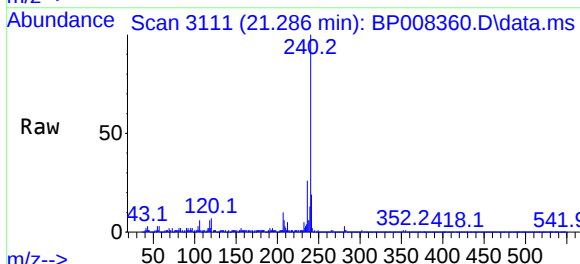




#79
 Terphenyl-d14
 Concen: 3.543 ng
 RT: 19.751 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP008360.D
 Acq: 11 Dec 2021 02:11

Instrument :
 BNA_P
 ClientSampleId :
 OK-03-120821

Tgt Ion:	244	Resp:	66656
Ion Ratio	Lower	Upper	
244	100		
212	8.2	6.0	9.0
122	8.6	6.6	9.8

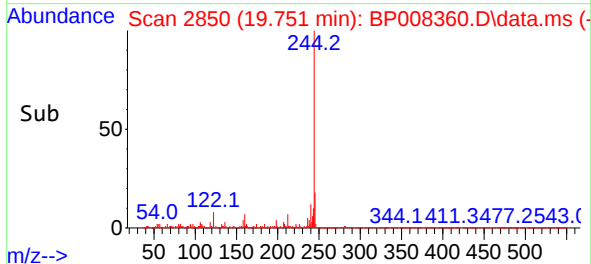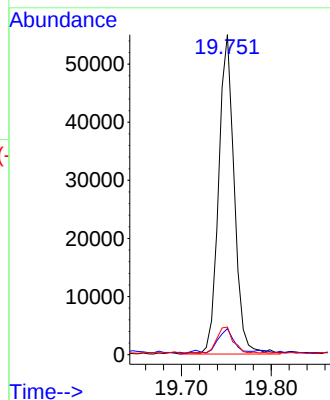

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.663 min Scan# 3515
 Delta R.T. -0.012 min
 Lab File: BP008360.D
 Acq: 11 Dec 2021 02:11

Tgt Ion:	264	Resp:	436774
Ion Ratio	Lower	Upper	
264	100		
260	24.1	19.4	29.2
265	22.5	17.6	26.4

