

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
Data File : BP008336.D
Acq On : 10 Dec 2021 12:11
Operator : CG/JU
Sample : PB141268BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141268BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.358	397	403	423	rBV	1203240	1840570	42.70%	9.330%
2	6.952	667	674	703	rBV	1067215	1839386	42.67%	9.324%
3	7.763	804	812	822	rBV	198379	325761	7.56%	1.651%
4	8.928	1000	1010	1034	rBV	641421	1172118	27.19%	5.941%
5	10.563	1280	1288	1301	rBV	203881	416824	9.67%	2.113%
6	13.034	1701	1708	1732	rBV	1579703	2457199	57.01%	12.455%
7	14.416	1936	1943	1958	rBV	343416	580363	13.46%	2.942%
8	15.916	2192	2198	2227	rBV	1236157	2039262	47.31%	10.337%
9	17.181	2407	2413	2429	rBV	438353	741852	17.21%	3.760%
10	19.757	2845	2851	2862	rBV	3564884	4310436	100.00%	21.850%
11	21.292	3107	3112	3121	rBV	648234	907218	21.05%	4.599%
12	21.404	3126	3131	3144	rBV	1458979	2156630	50.03%	10.932%
13	23.674	3511	3517	3532	rVB2	408925	940224	21.81%	4.766%




Sum of corrected areas: 19727843

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
Data File : BP008336.D
Acq On : 10 Dec 2021 12:11
Operator : CG/JU
Sample : PB141268BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141268BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

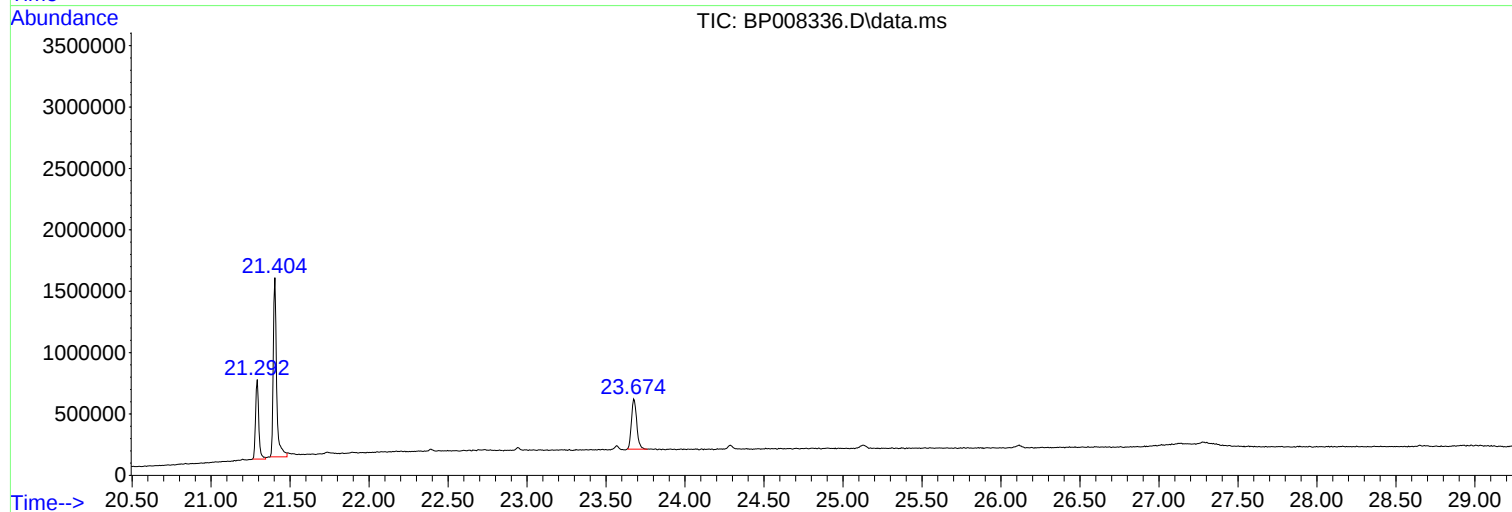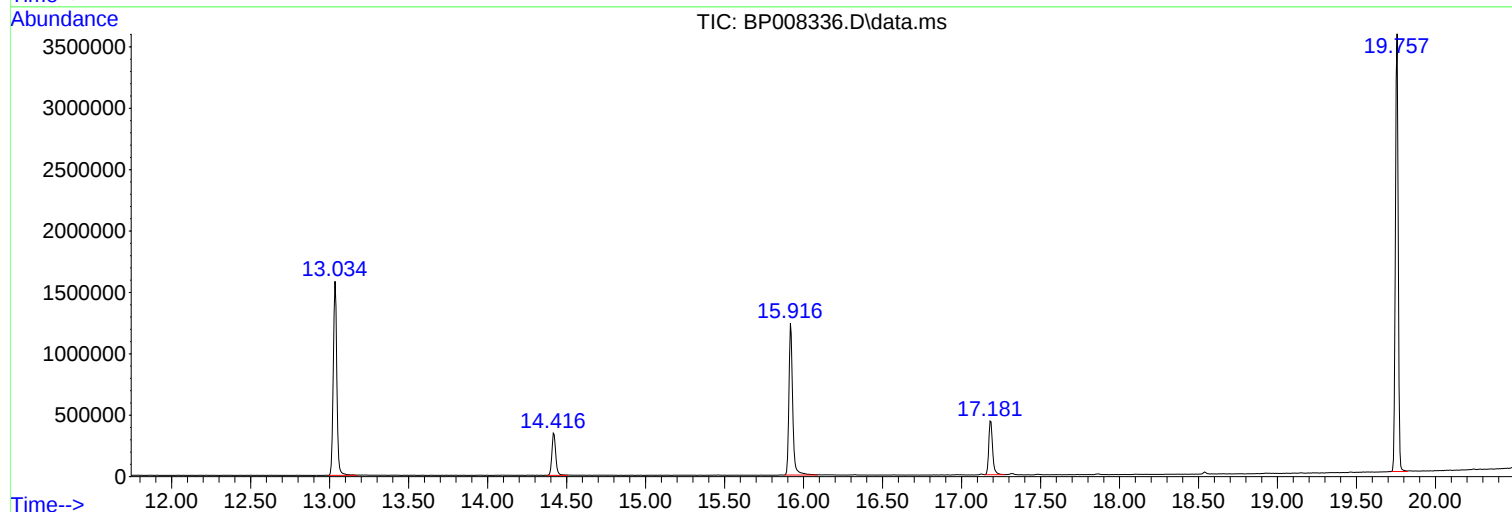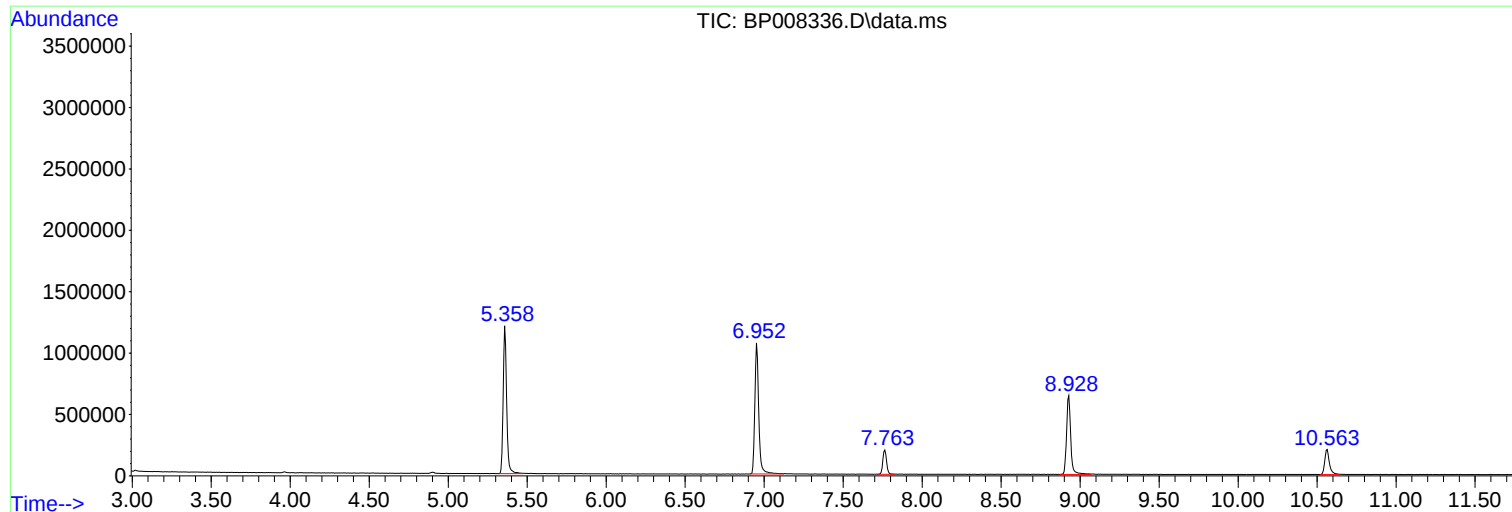

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
Data File : BP008336.D
Acq On : 10 Dec 2021 12:11
Operator : CG/JU
Sample : PB141268BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141268BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.404	47.54 ng	2156630	Chrysene-d12	21.292

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			Thiophene-3-carbonitrile, 4-(4-m...	277	C13H11NO2S2	1000268-75-0	9
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	9

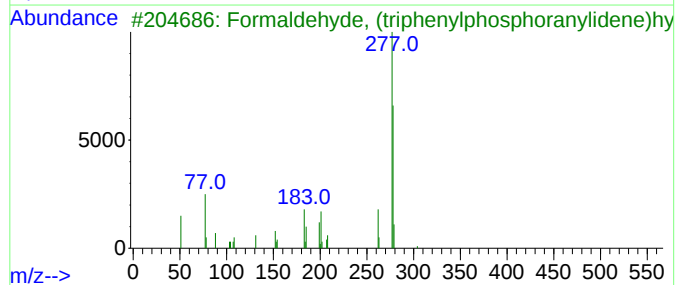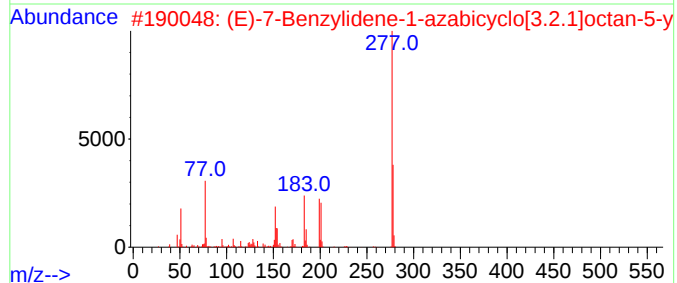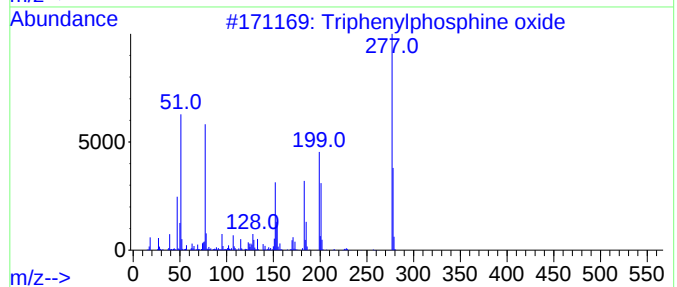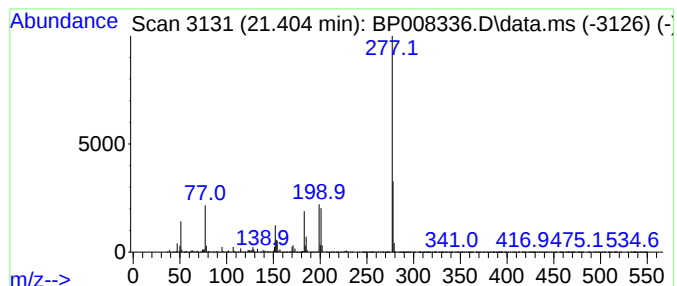

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
Data File : BP008336.D
Acq On : 10 Dec 2021 12:11
Operator : CG/JU
Sample : PB141268BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB141268BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	21.404	47.5	ng	2156630	5	21.292	907218	20.0