
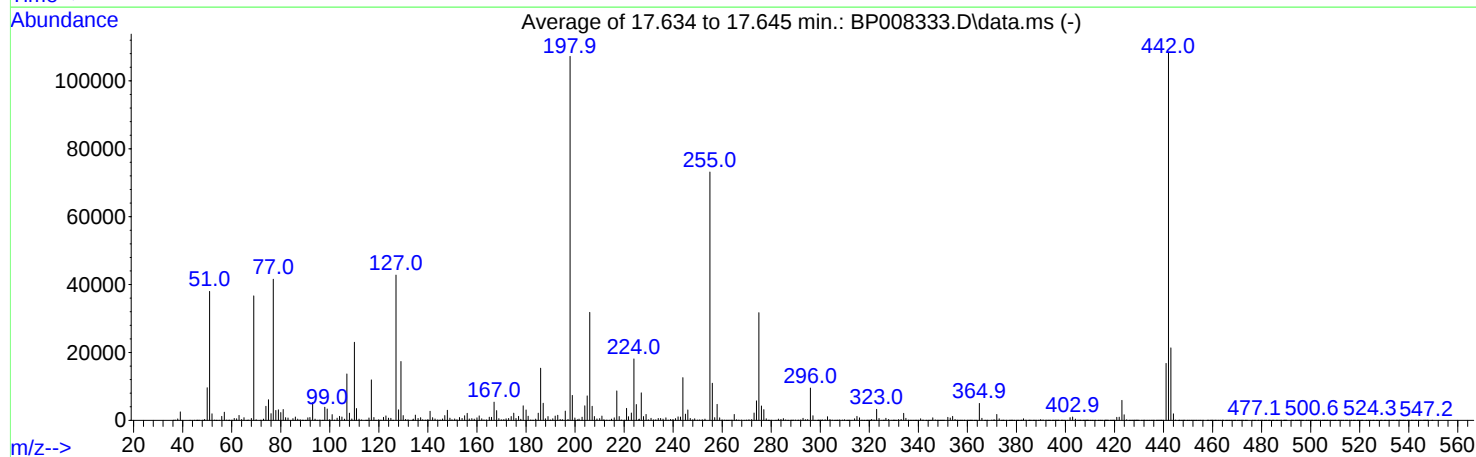


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
 Data File : BP008333.D
 Acq On : 10 Dec 2021 10:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 03:53:01 2021

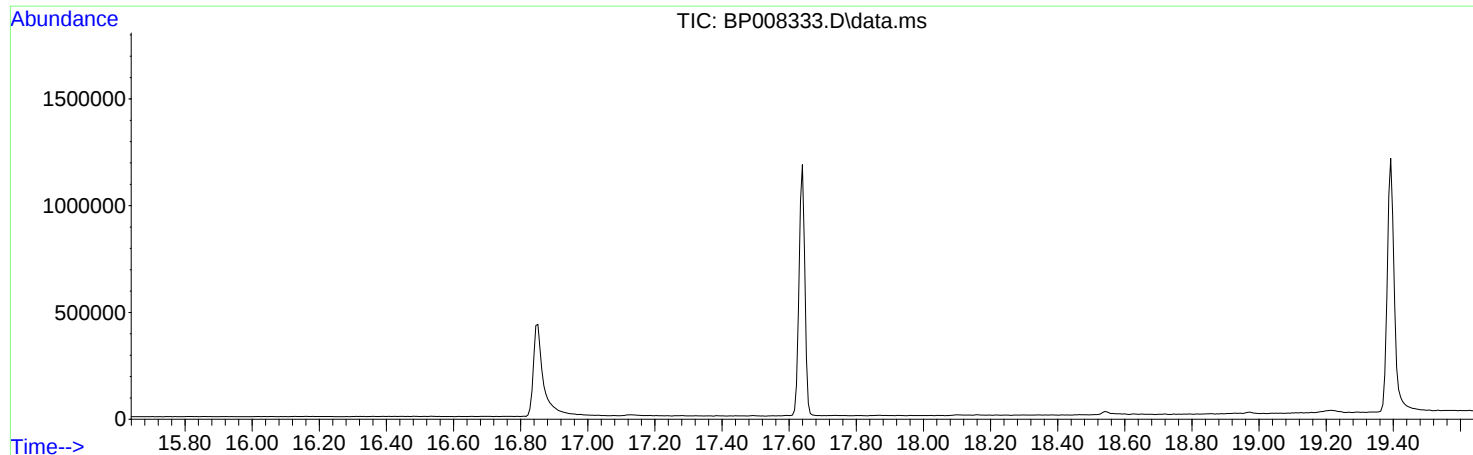




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	37998	PASS
68	69	0.00	2	1.5	545	PASS
69	198	0.00	100	34.2	36679	PASS
70	69	0.00	2	0.5	180	PASS
127	198	10	80	39.9	42804	PASS
197	198	0.00	2	0.3	279	PASS
198	198	100	100	100.0	107218	PASS
199	198	5	9	6.9	7370	PASS
275	198	10	60	29.6	31709	PASS
365	198	1	100	4.7	5017	PASS
441	198	0.01	100	15.7	16786	PASS
442	442	100	100	100.0	108352	PASS
443	442	15	24	19.7	21350	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
Data File : BP008333.D
Acq On : 10 Dec 2021 10:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 11 03:50:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 01:43:36 2021
Response via : Initial Calibration

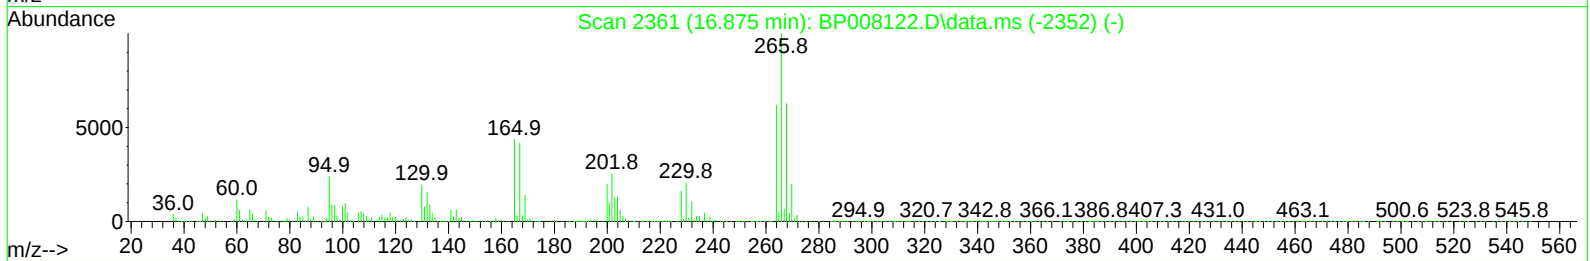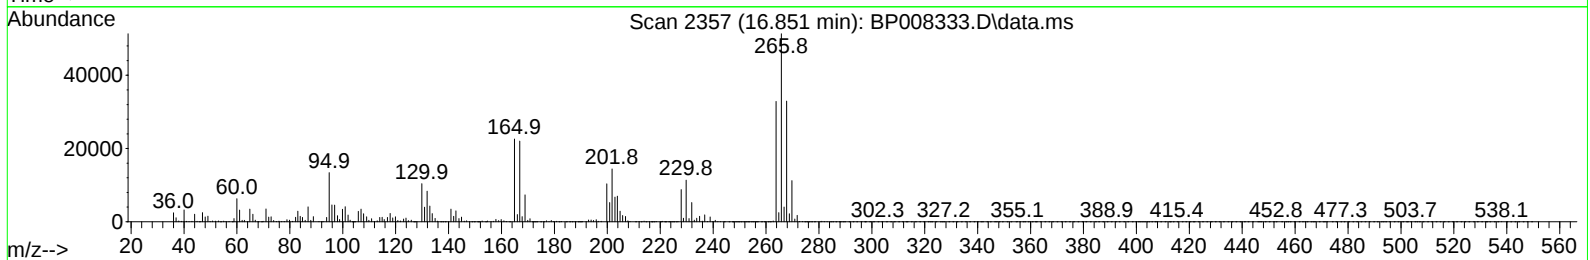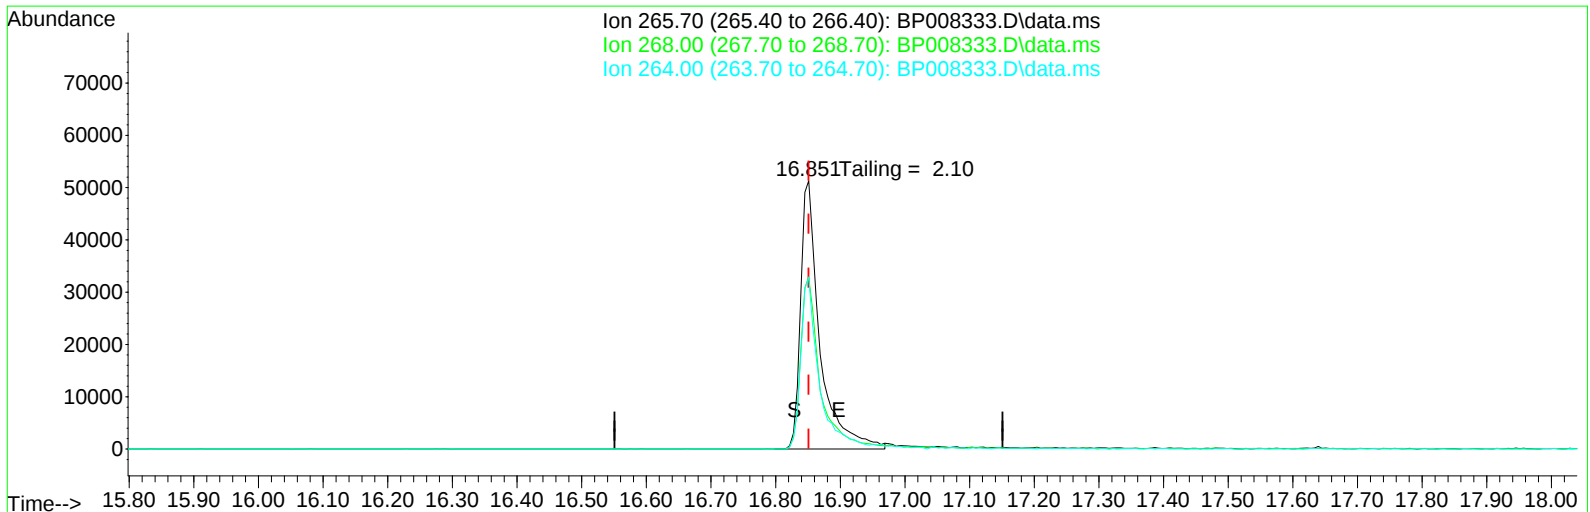

TIC: BP008333.D\data.ms

(70) Pentachlorophenol (C)

16.851min (+ 0.000) 1708764.09 ng




response 108699

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.16
264.00	61.90	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
 Data File : BP008333.D
 Acq On : 10 Dec 2021 10:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 11 03:50:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 01:43:36 2021
 Response via : Initial Calibration

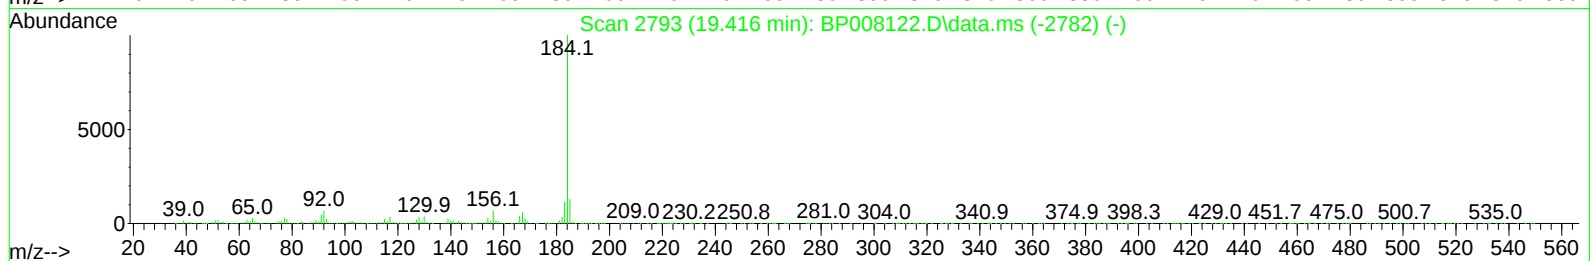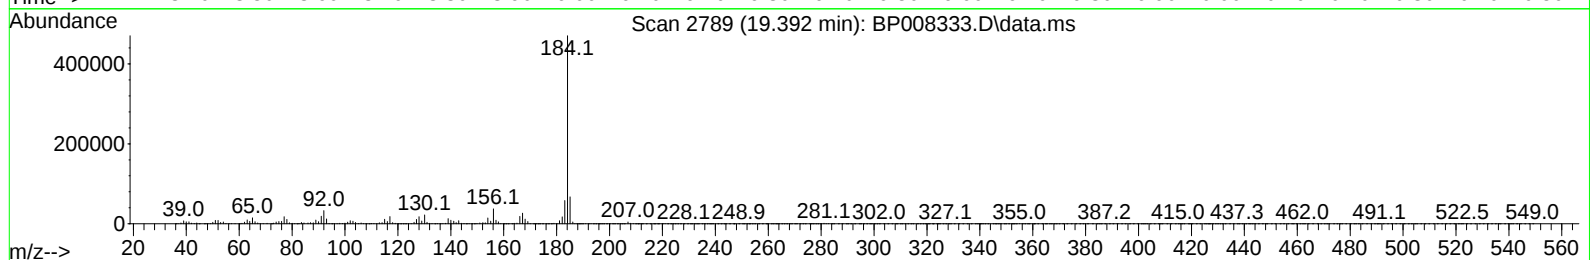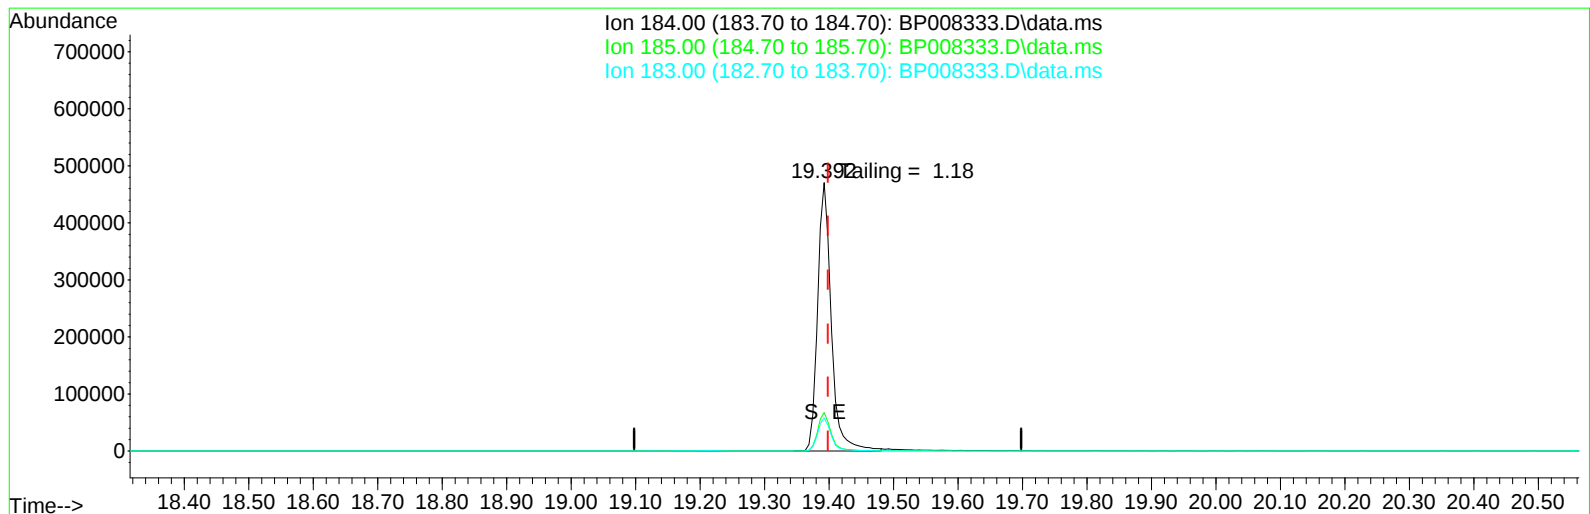

TIC: BP008333.D\data.ms

(77) Benzidine

19.392min (-0.006) 1167981.12 ng

response 704944

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.33
183.00	11.40	12.31
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
12/10/2021	BNA_P	<u>BP008333.D</u>
Compound Name	Response	Retention Time
DDT	393383	20.59
DDD	1730	20.17
DDE	974	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2704	396087	0.68

Instrument :
BNA_P
ClientSampleId :
DFTPP