
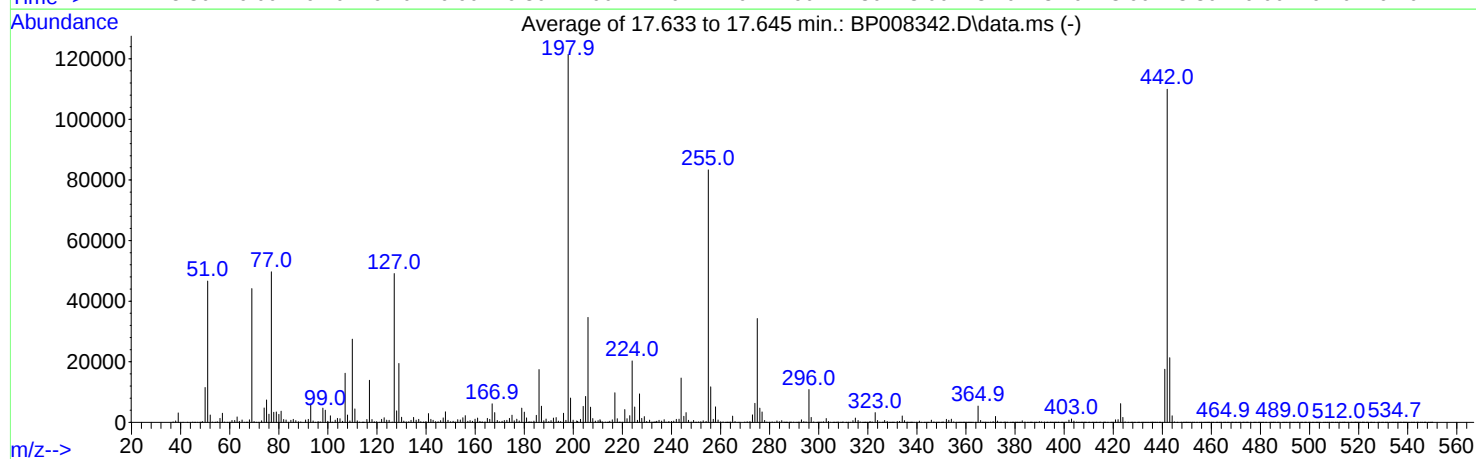


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
 Data File : BP008342.D
 Acq On : 10 Dec 2021 15:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 03:53:01 2021

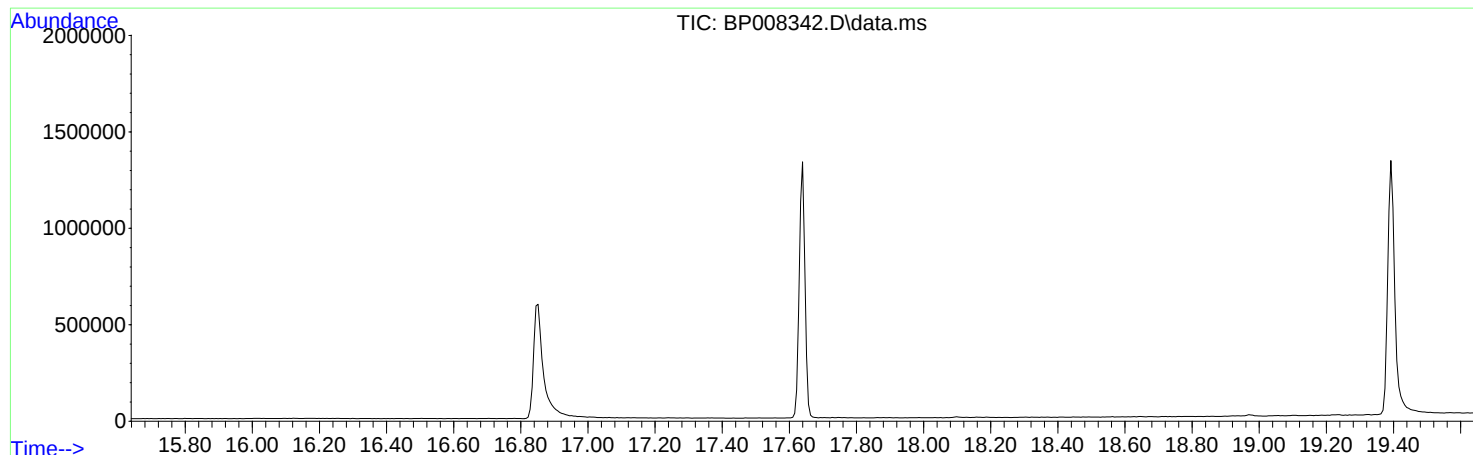




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	46650	PASS
68	69	0.00	2	1.9	843	PASS
69	198	0.00	100	36.4	44162	PASS
70	69	0.00	2	0.6	268	PASS
127	198	10	80	40.4	49091	PASS
197	198	0.00	2	0.6	700	PASS
198	198	100	100	100.0	121405	PASS
199	198	5	9	6.6	8026	PASS
275	198	10	60	28.2	34269	PASS
365	198	1	100	4.5	5406	PASS
441	198	0.01	100	14.4	17519	PASS
442	442	100	100	100.0	109916	PASS
443	442	15	24	19.4	21328	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
 Data File : BP008342.D
 Acq On : 10 Dec 2021 15:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 11 03:48:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 01:43:36 2021
 Response via : Initial Calibration

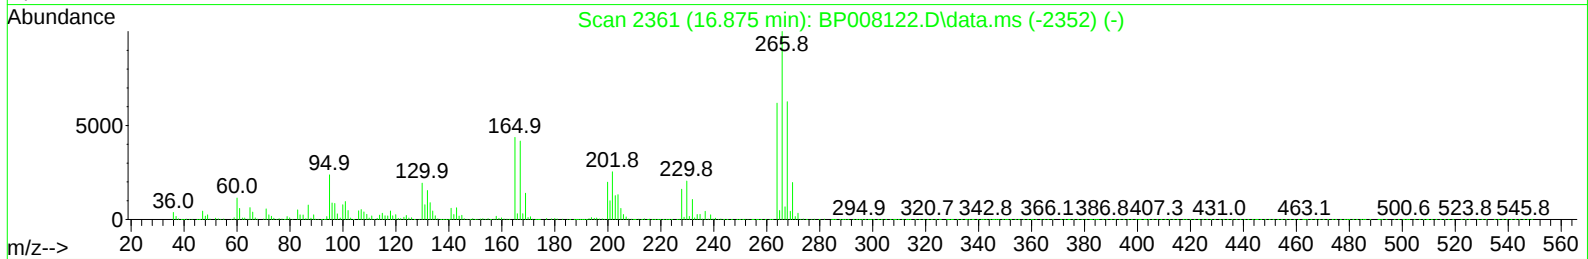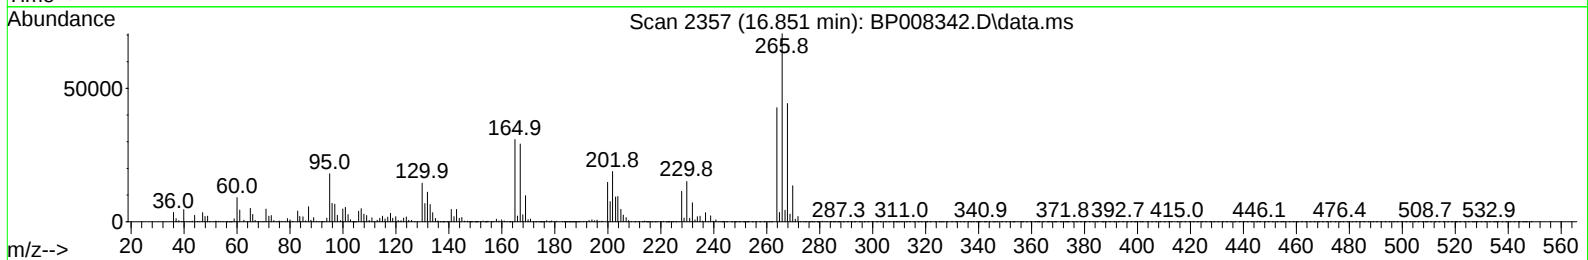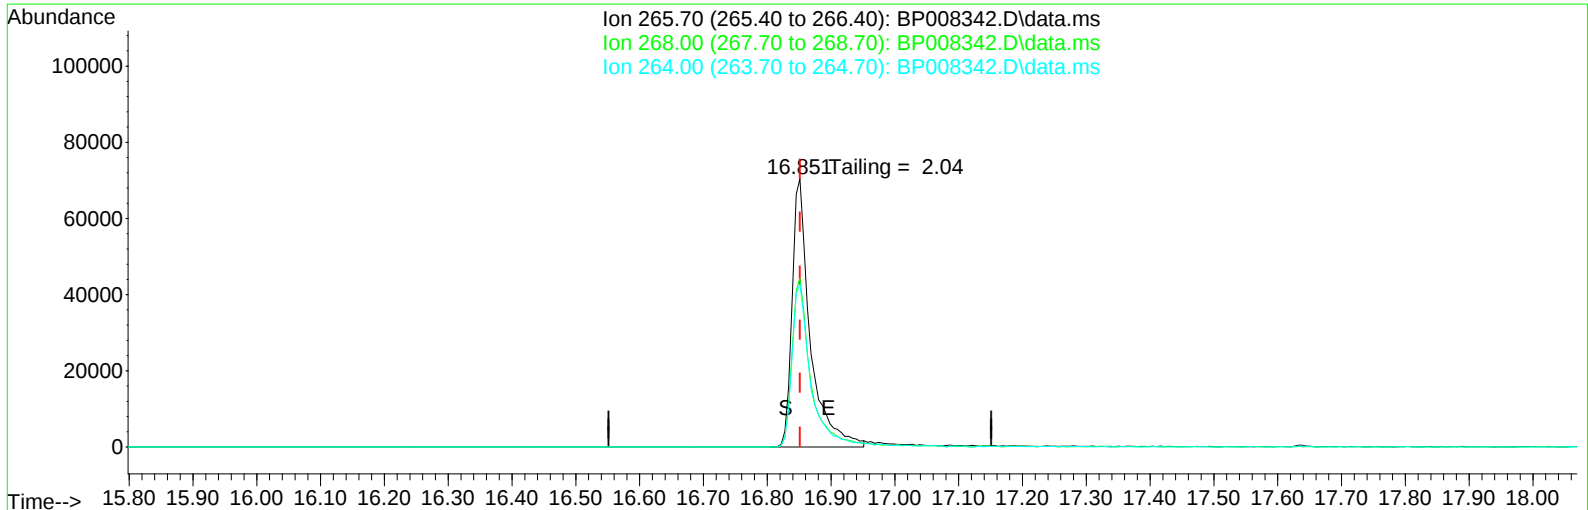

TIC: BP008342.D\data.ms

(70) Pentachlorophenol (C)

16.851min (+ 0.000) 314865.56 ng




response 144657

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.89
264.00	61.90	60.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121021\
 Data File : BP008342.D
 Acq On : 10 Dec 2021 15:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 11 03:48:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 01:43:36 2021
 Response via : Initial Calibration

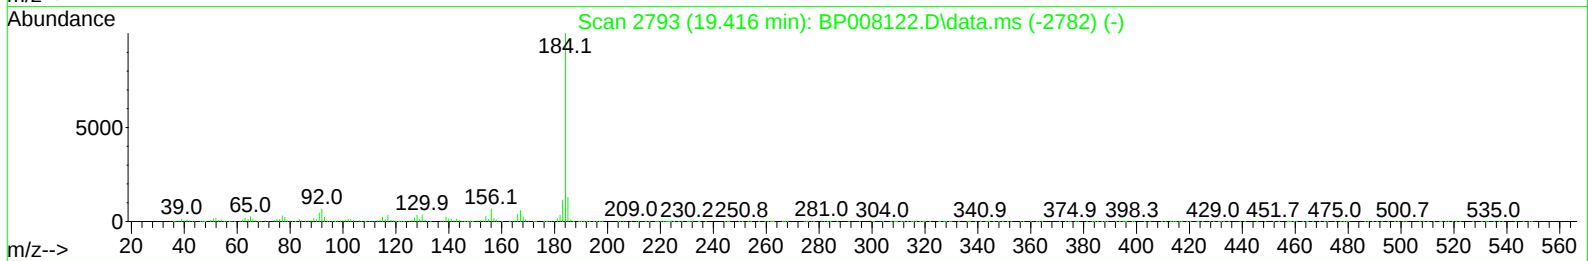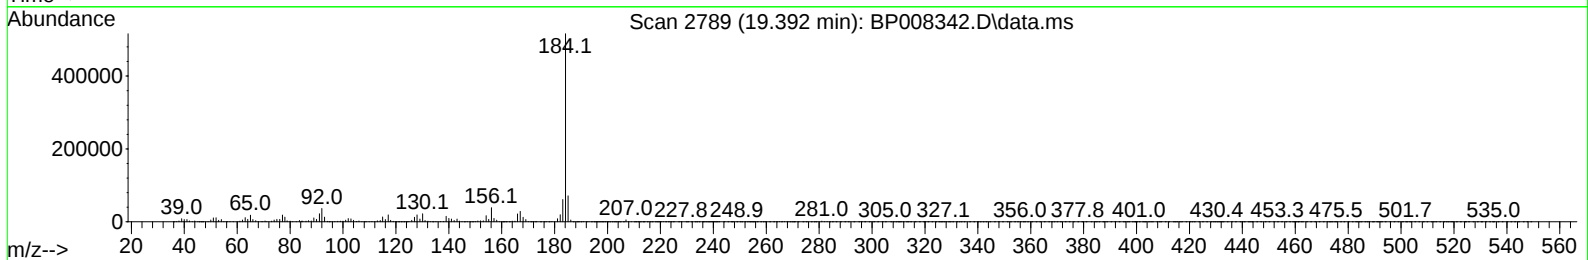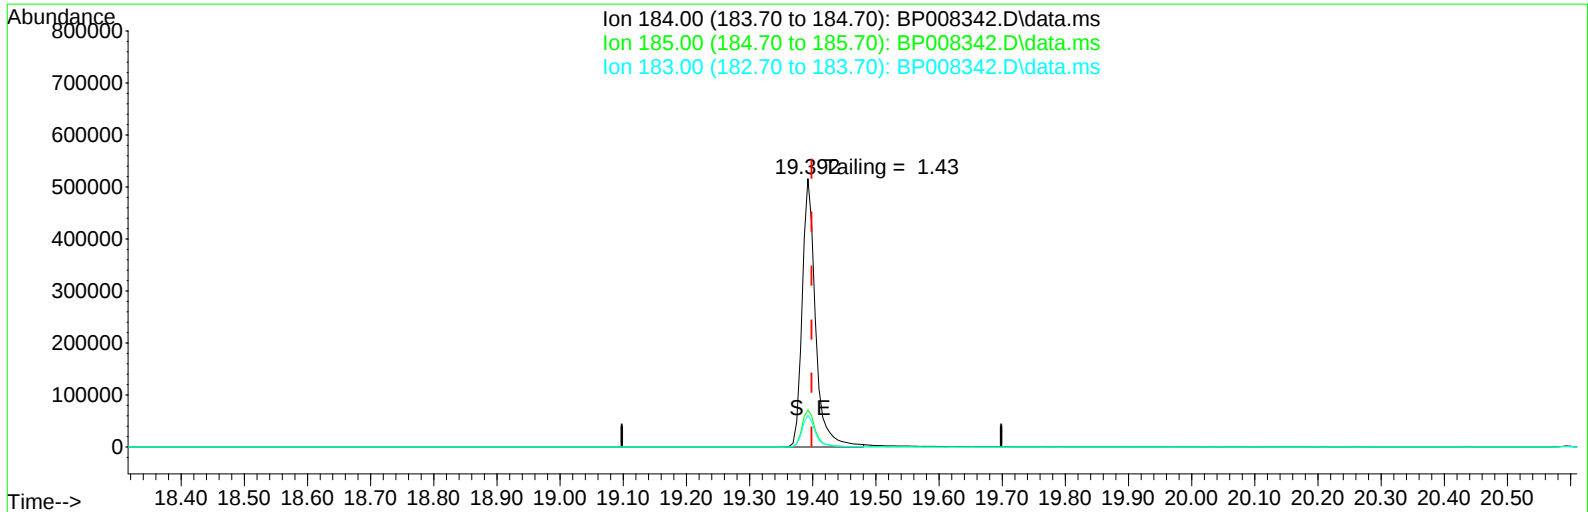

TIC: BP008342.D\data.ms

(77) Benzidine

19.392min (-0.006) 1449056.37 ng

response 775204

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.81
183.00	11.40	11.84
0.00	0.00	0.00

Instrument :
BNA_P
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/10/2021	BNA_P	BP008342.D
Compound Name	Response	Retention Time
DDT	425872	20.59
DDD	2355	20.16
DDE	932	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3287	429159	0.77

Instrument :
BNA_P
ClientSampleId :
DFTPP