
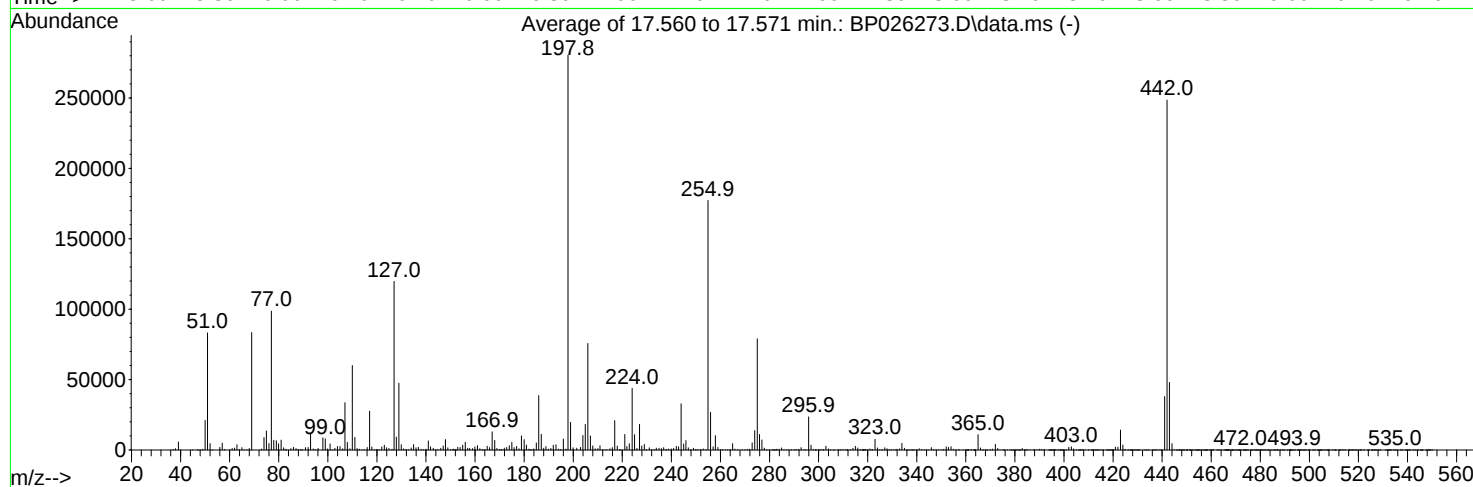


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121025\
Data File : BP026273.D
Acq On : 10 Dec 2025 13:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 05 14:52:44 2025

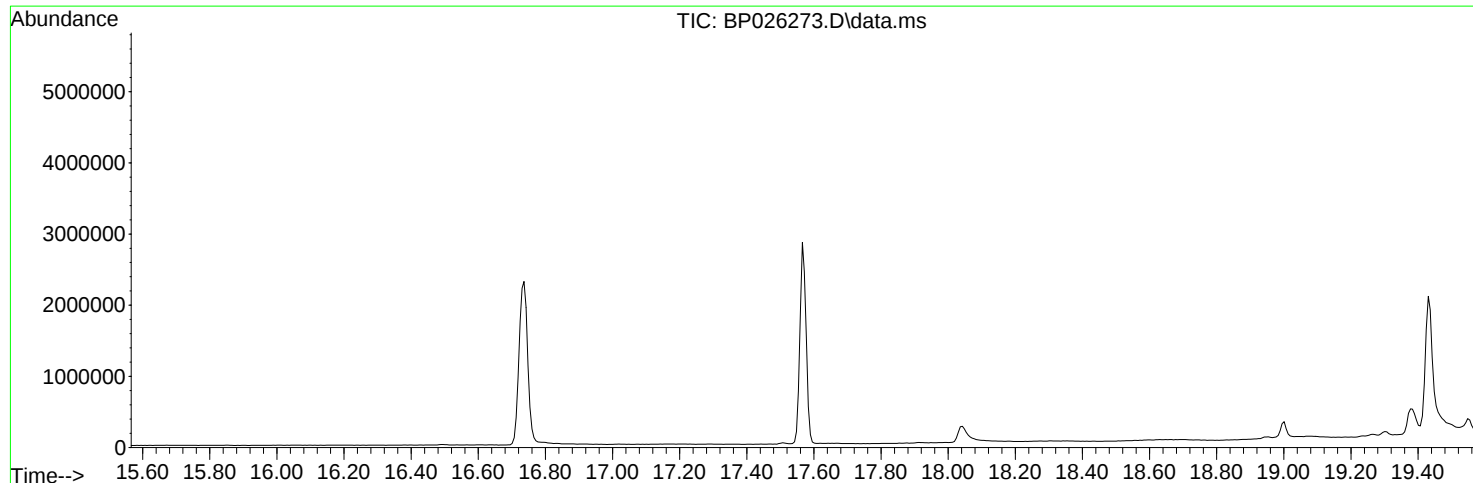




AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2478

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.4	1147	PASS
69	69	100	100	100.0	83449	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.2	582	PASS
198	198	100	100	100.0	280526	PASS
199	198	5	9	7.0	19665	PASS
365	198	1	100	3.9	10892	PASS
441	443	0.01	150	79.2	37903	PASS
442	442	100	100	100.0	248619	PASS
443	442	15	24	19.3	47875	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121025\
Data File : BP026273.D
Acq On : 10 Dec 2025 13:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 10 13:26:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

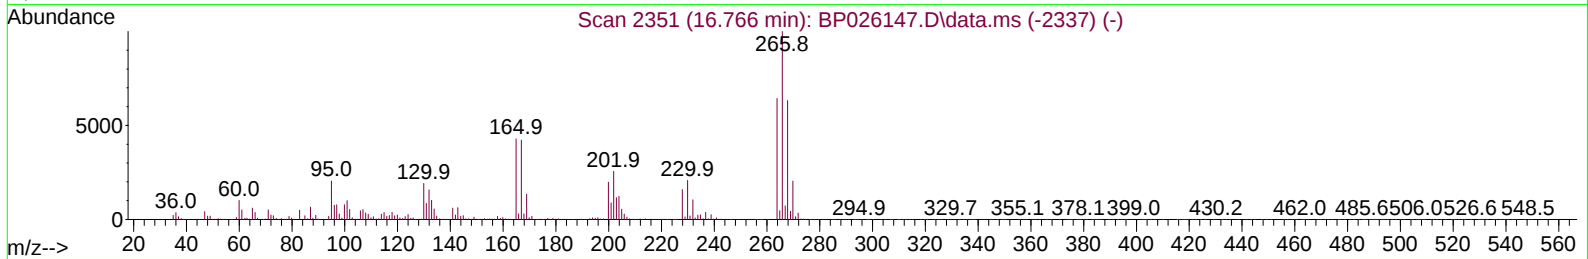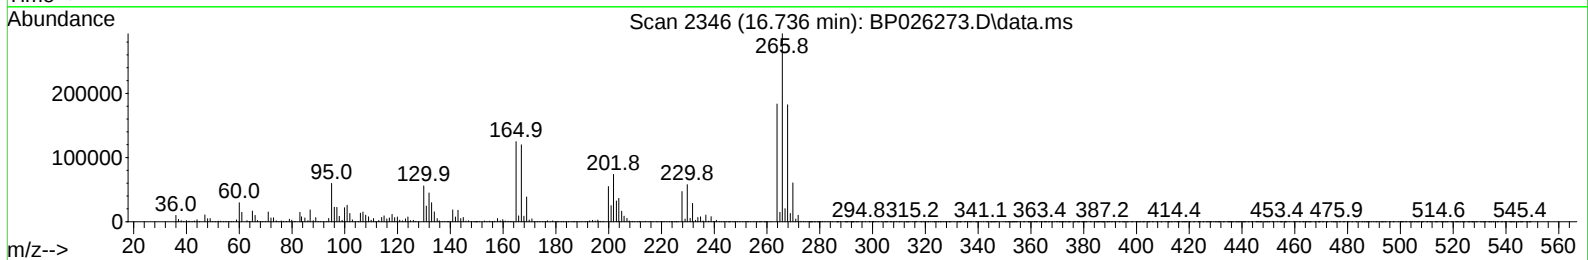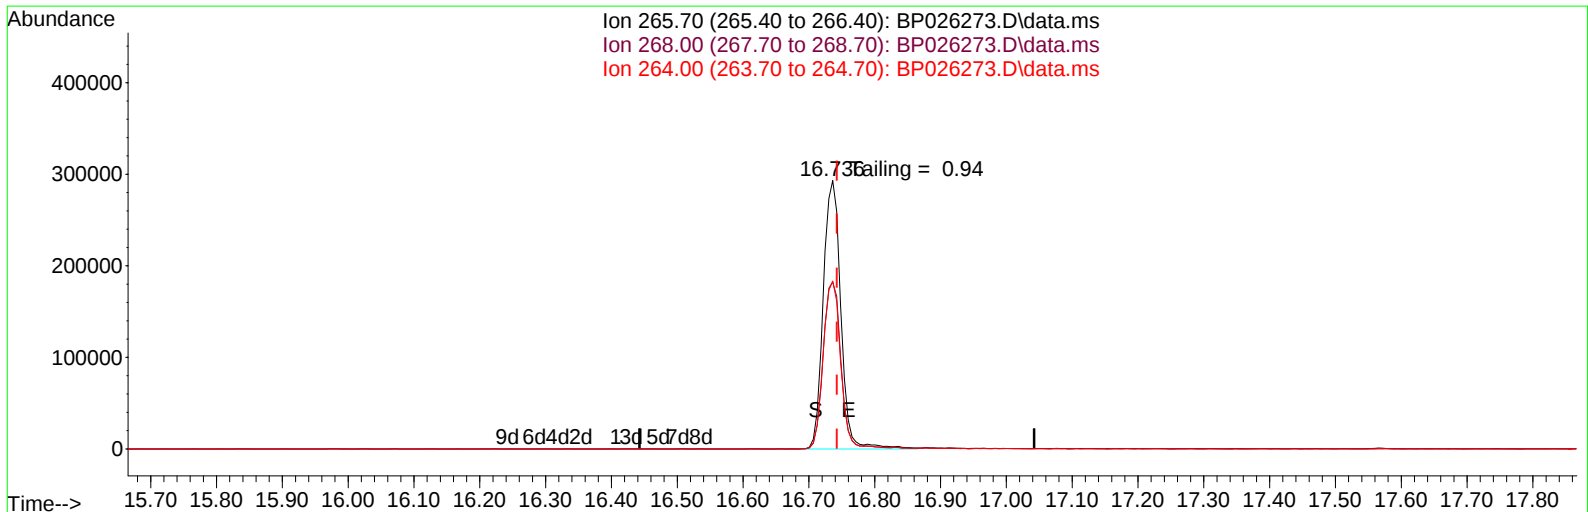

TIC: BP026273.D\data.ms

(70) Pentachlorophenol (C)

16.736min (-0.006) 170279.97 ng m




response 543359

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.21
264.00	62.70	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121025\
Data File : BP026273.D
Acq On : 10 Dec 2025 13:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 10 13:26:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 05 14:52:44 2025
Response via : Initial Calibration

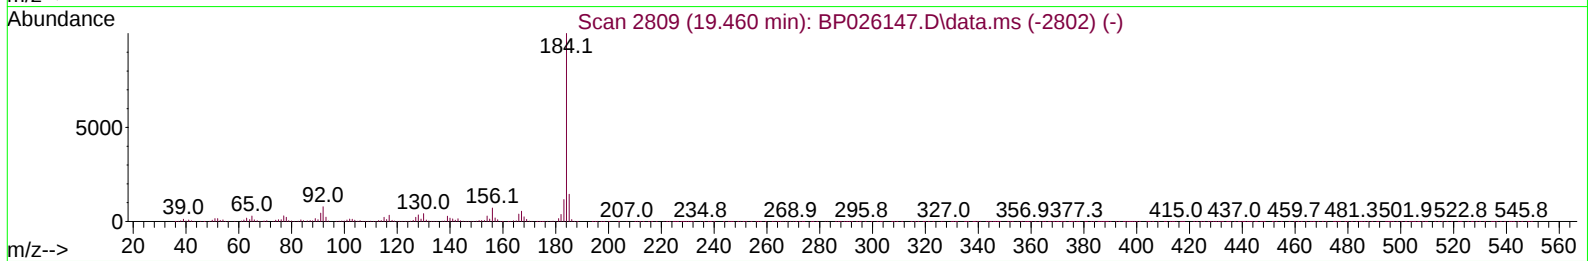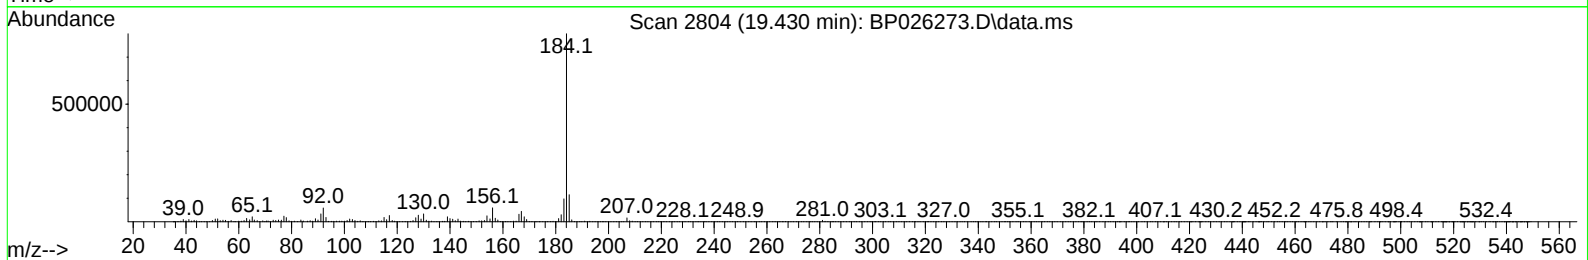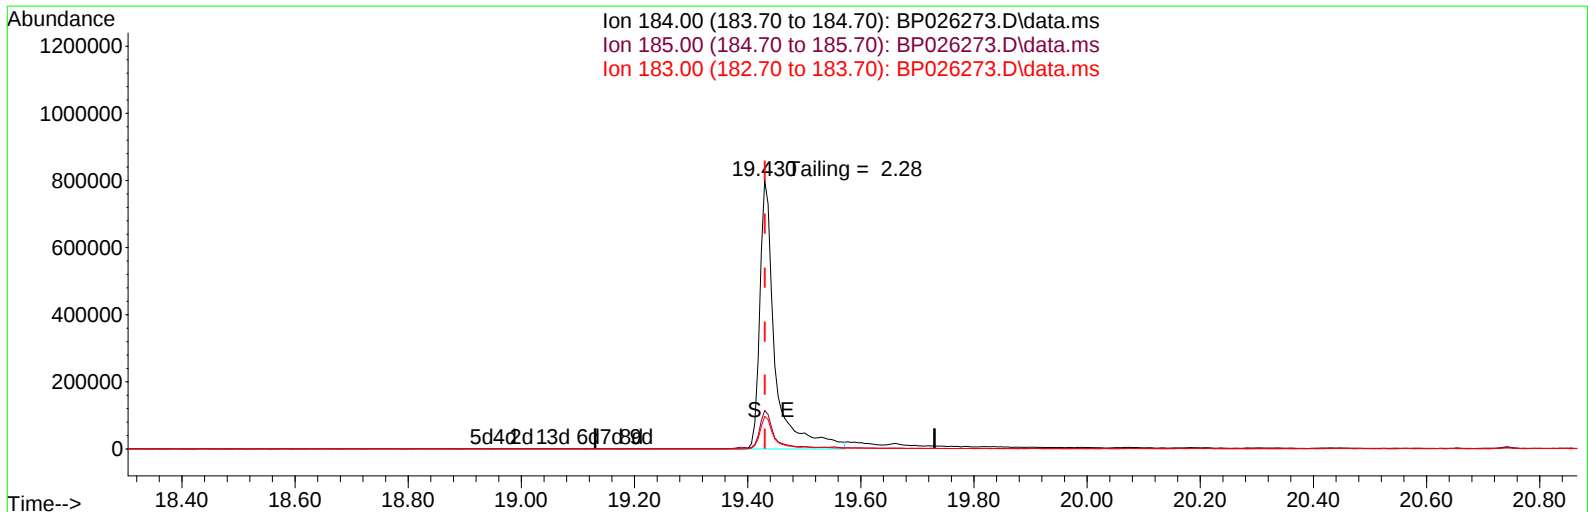

TIC: BP026273.D\data.ms

(77) Benzidine

19.430min (-0.000) 97542.59 ng m

response 1684370

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.36
183.00	11.30	12.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/10/2025	BNA_P	<u>BP026273.D</u>
Compound Name	Response	Retention Time
DDT	1323712	20.742
DDD	26243	20.271
DDE	4251	19.742
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
30494	1354206	2.25

Instrument :
BNA_P
ClientSampleId :
DFTPP