
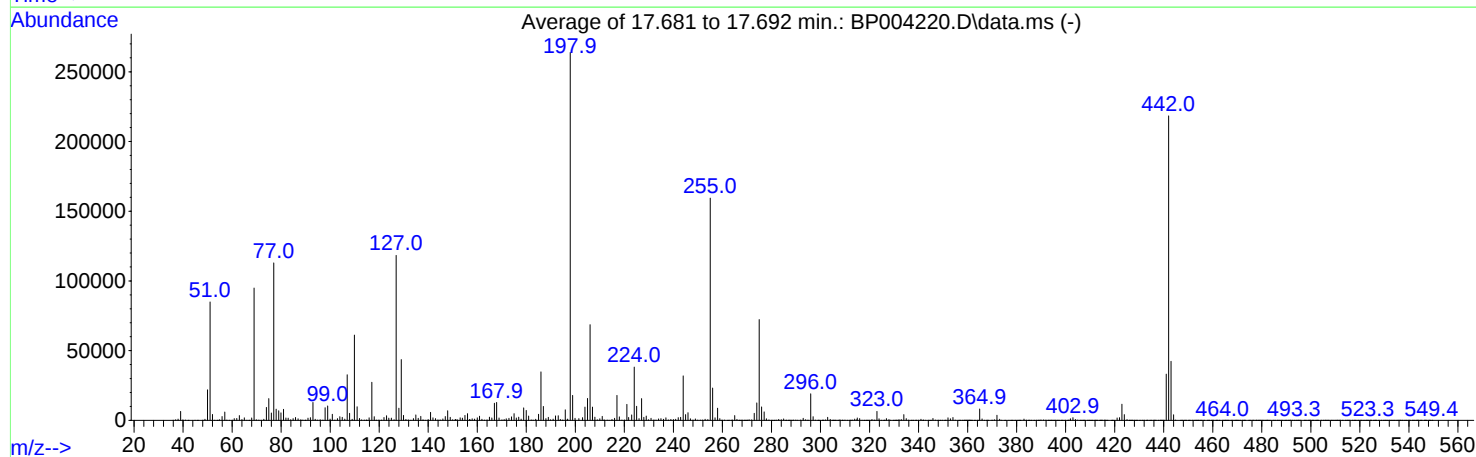


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121120\
 Data File : BP004220.D
 Acq On : 11 Dec 2020 09:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP121120.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 15 10:27:21 2020

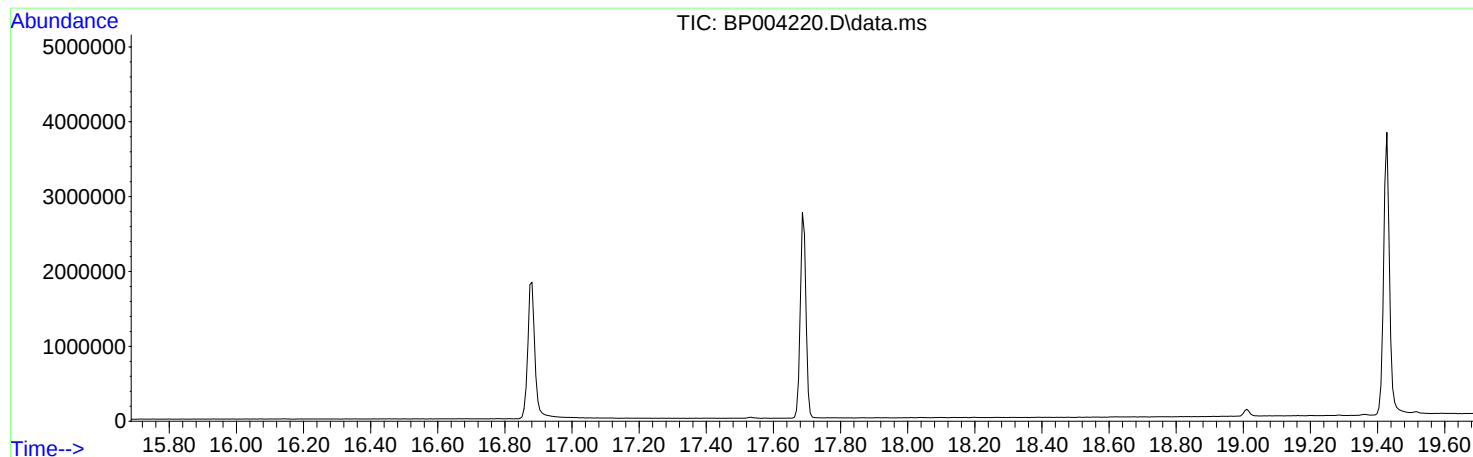

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	84939	PASS
68	69	0.00	2	1.8	1692	PASS
69	198	0.00	100	36.0	94874	PASS
70	69	0.00	2	0.5	481	PASS
127	198	10	80	44.8	118321	PASS
197	198	0.00	2	0.4	949	PASS
198	198	100	100	100.0	263841	PASS
199	198	5	9	6.8	17961	PASS
275	198	10	60	27.4	72268	PASS
365	198	1	100	3.1	8179	PASS
441	198	0.01	100	12.6	33205	PASS
442	442	100	100	100.0	218445	PASS
443	442	15	24	19.4	42307	PASS