

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018764.D
 Acq On : 12 Dec 2023 12:55
 Operator : MA/JU
 Sample : 05675-14
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AB7

Quant Time: Dec 12 21:37:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 11 22:02:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	167325	20.000	ng/u1	0.00
20) Naphthalene-d8	10.634	136	625095	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.469	164	403224	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.216	188	918315	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.304	240	1054153	20.000	ng/u1	# 0.00
88) Perylene-d12	23.668	264	1292678	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	19174	3.905	ng/uL	0.00
4) Pyridine-d5	3.681	84	123321	9.376	ng/u1	0.00
7) Phenol-d5	7.005	99	74557	4.440	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	236899	23.804	ng/u1	0.00
11) 2-Chlorophenol-d4	7.369	132	243770	18.605	ng/u1	0.00
15) 4-Methylphenol-d8	8.552	113	145428	10.702	ng/u1	0.00
21) Nitrobenzene-d5	8.999	128	150944	27.131	ng/u1	0.00
24) 2-Nitrophenol-d4	9.722	143	159341	27.624	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.257	165	292831	24.828	ng/u1	0.00
31) 4-Chloroaniline-d4	10.775	131	369861	23.995	ng/u1	0.00
46) Dimethylphthalate-d6	13.887	166	1024670	28.472	ng/u1	0.00
49) Acenaphthylene-d8	14.163	160	1090911	27.529	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	27380	4.635	ng/u1	0.00
60) Fluorene-d10	15.463	176	886572	29.349	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	159605	28.986	ng/u1	0.00
73) Anthracene-d10	17.316	188	1536107	31.818	ng/u1	0.00
81) Pyrene-d10	19.551	212	2073875	25.273	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.521	264	2474569	32.831	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.293	88	11186	2.077	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018764.D
Acq On : 12 Dec 2023 12:55
Operator : MA/JU
Sample : 05675-14
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AB7


Quant Time: Dec 12 21:37:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 11 22:02:13 2023
Response via : Initial Calibration

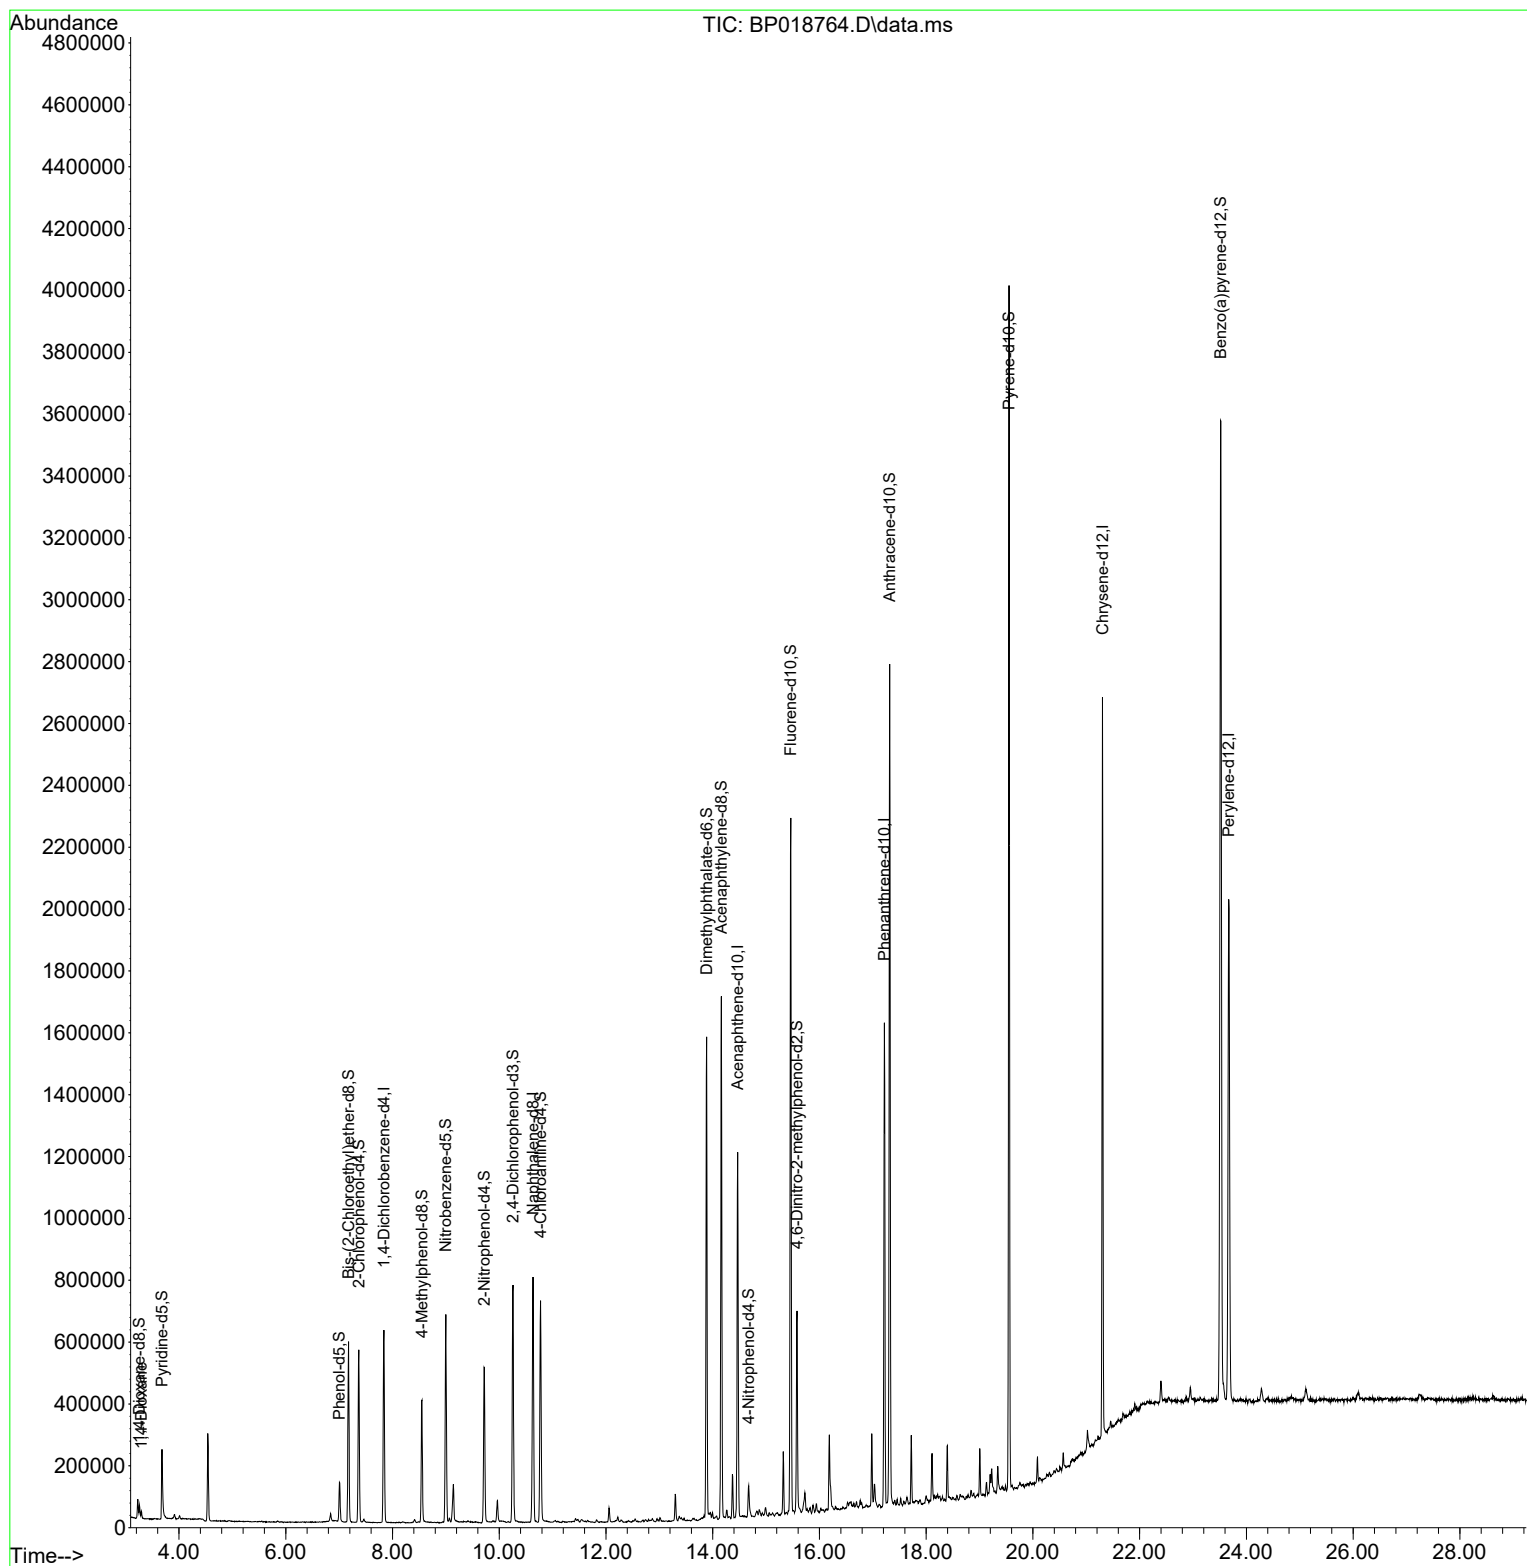

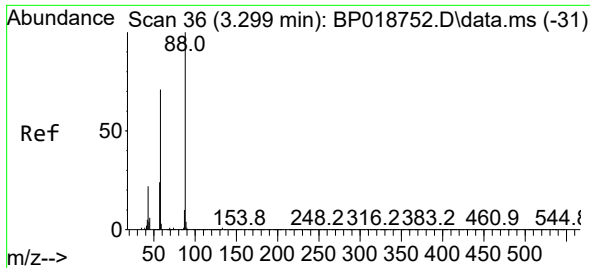

#2
 1,4-Dioxane
 Concen: 2.077 ng/uL
 RT: 3.293 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BP018764.D
 Acq: 12 Dec 2023 12:55

Instrument :
 BNA_P
 ClientSampleId :
 H0AB7

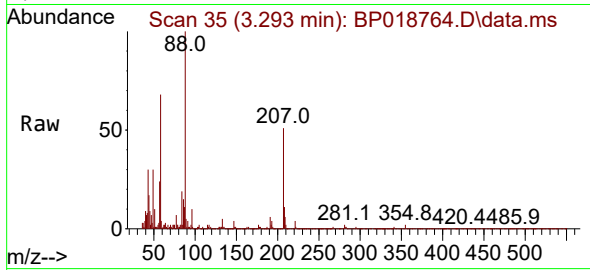

Tgt Ion:	88	Resp:	11186
Ion	Ratio	Lower	Upper
88	100		
43	30.3	21.8	32.6
58	68.3	56.5	84.7

