




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018790.D
 Acq On : 13 Dec 2023 04:11
 Operator : MA/JU
 Sample : 05675-03
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA4

Manual IntegrationsAPPROVED

Quant Time: Dec 13 04:38:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 11 22:02:13 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/13/2023
 Supervised By :mohammad ahmed 12/14/2023

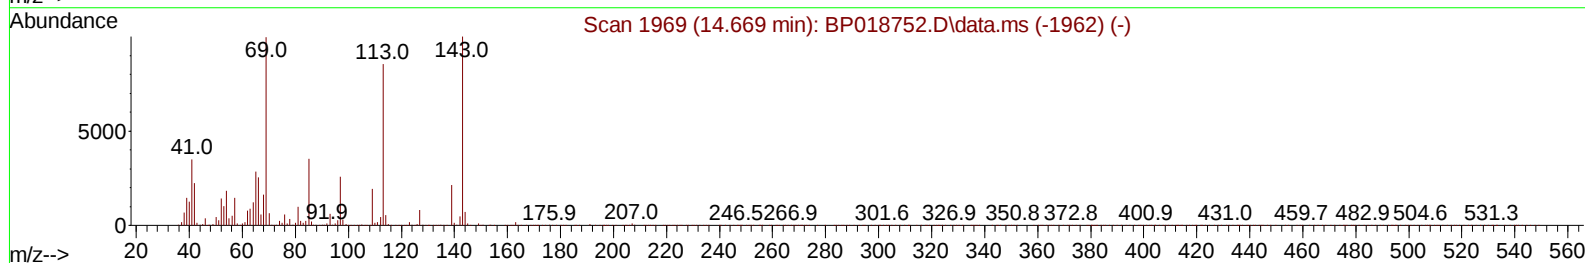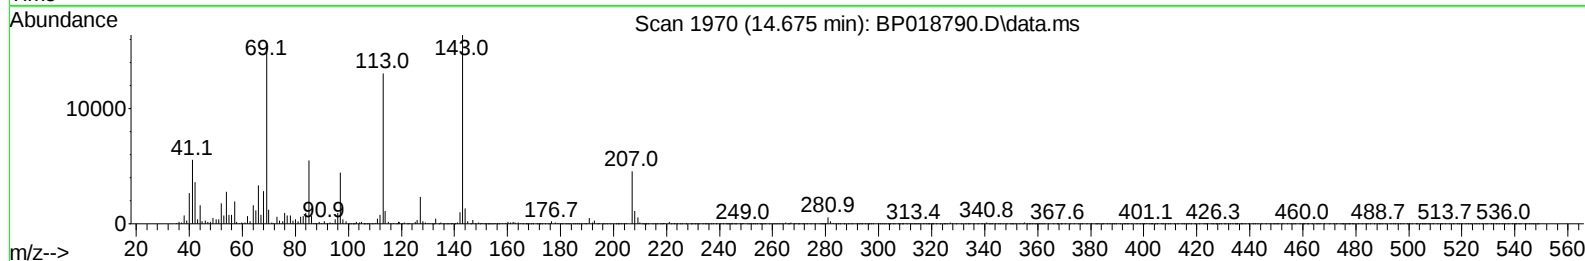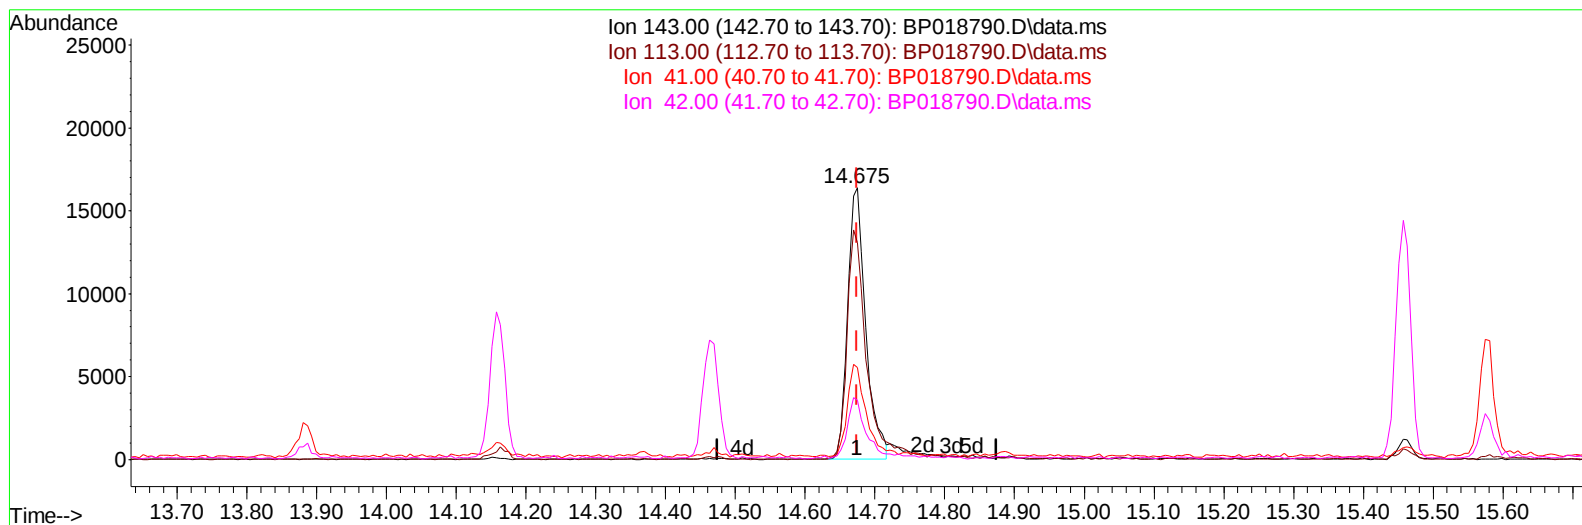

TIC: BP018790.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (+ 0.000) 4.68 ng/u1

response 29531

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.80	79.72
41.00	34.60	33.83
42.00	23.00	21.92




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018790.D
 Acq On : 13 Dec 2023 04:11
 Operator : MA/JU
 Sample : 05675-03
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA4

Manual IntegrationsAPPROVED

Quant Time: Dec 13 04:38:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 11 22:02:13 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/13/2023
 Supervised By :mohammad ahmed 12/14/2023

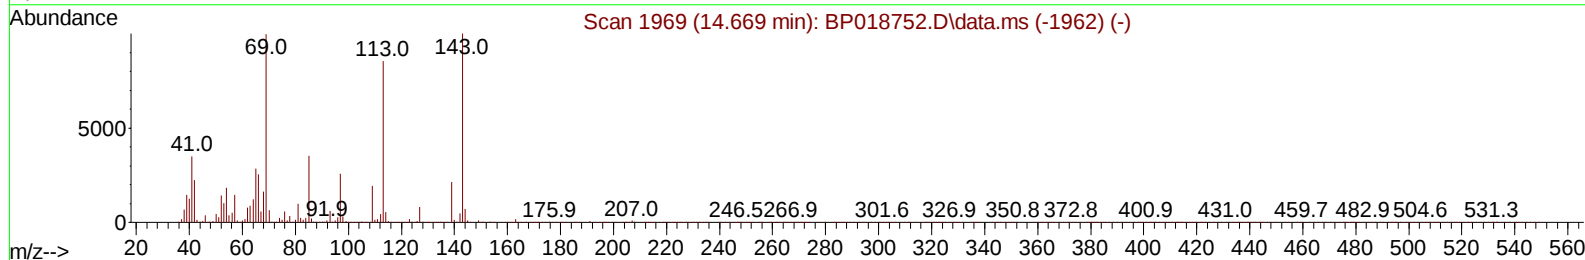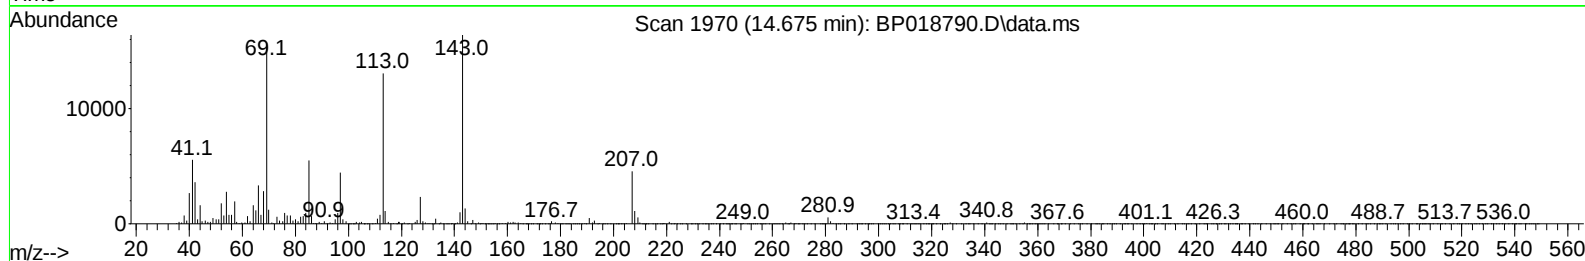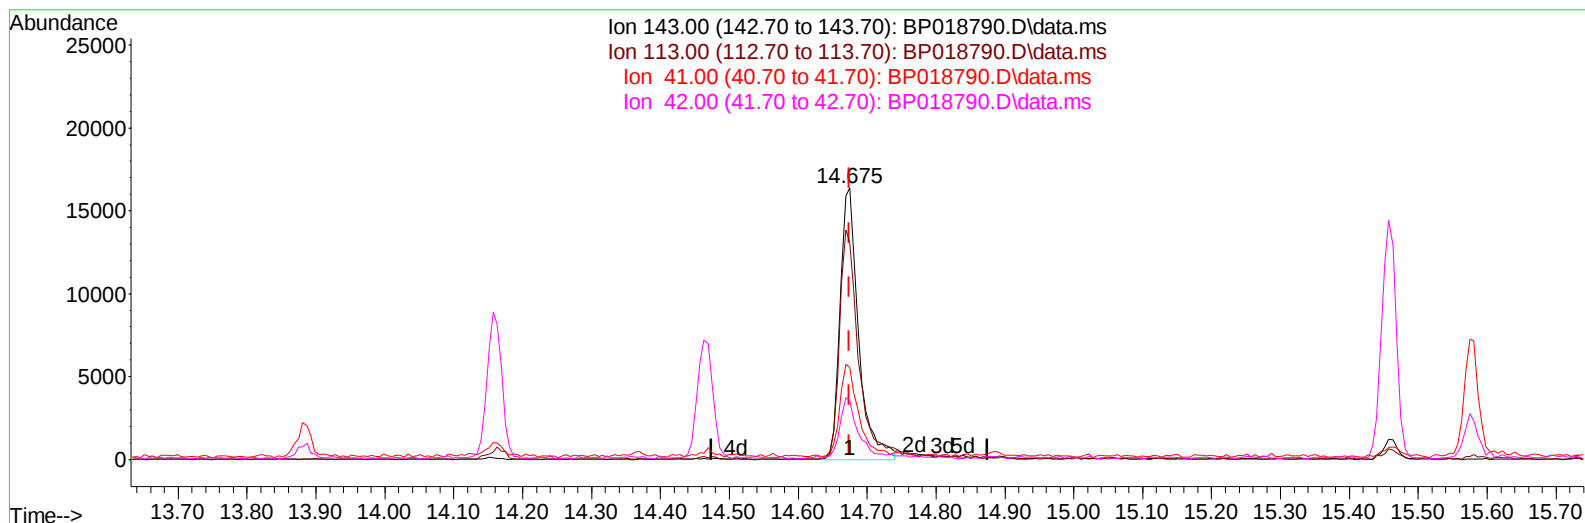

TIC: BP018790.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.675min (+ 0.000) 4.86 ng/ul m

response 30621

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.80	79.72
41.00	34.60	33.83
42.00	23.00	21.92

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
 Data File : BP018790.D
 Acq On : 13 Dec 2023 04:11
 Operator : MA/JU
 Sample : 05675-03
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0AA4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/13/2023
 Supervised By :mohammad ahmed 12/14/2023

Quant Time: Dec 13 04:39:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 11 22:02:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	176079	20.000	ng/ul	0.00
20) Naphthalene-d8	10.634	136	656386	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.463	164	430400	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.210	188	1044077	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.304	240	1198688	20.000	ng/ul	# 0.00
88) Perylene-d12	23.663	264	1412942	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	20509	3.969	ng/uL	0.00
4) Pyridine-d5	3.693	84	31168	2.252	ng/ul	0.02
7) Phenol-d5	7.011	99	86558	4.899	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.175	67	272623	26.031	ng/ul	0.00
11) 2-Chlorophenol-d4	7.369	132	282316	20.475	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	166112	11.616	ng/ul	0.00
21) Nitrobenzene-d5	8.999	128	184734	31.621	ng/ul	0.00
24) 2-Nitrophenol-d4	9.716	143	191428	31.605	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.252	165	344963	27.853	ng/ul	0.00
31) 4-Chloroaniline-d4	10.775	131	11895	0.735	ng/ul	0.00
46) Dimethylphthalate-d6	13.887	166	1219080	31.736	ng/ul	0.00
49) Acenaphthylene-d8	14.163	160	1267060	29.955	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	30621m	4.856	ng/ul	0.00
60) Fluorene-d10	15.457	176	1057745	32.804	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.581	200	169908	27.141	ng/ul	0.00
73) Anthracene-d10	17.310	188	1781534	32.457	ng/ul	-0.01
81) Pyrene-d10	19.551	212	2300469	24.655	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.510	264	2642605	32.076	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121123\
Data File : BP018790.D
Acq On : 13 Dec 2023 04:11
Operator : MA/JU
Sample : 05675-03
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0AA4

Manual IntegrationsAPPROVED

Quant Time: Dec 13 04:39:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 11 22:02:13 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/13/2023
Supervised By :mohammad ahmed 12/14/2023

